MILITARY SPECIFICATION

FORCEPS, KIDNEY PEDICLE, GUYON-PEAN, 9 INCH

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of kidney pedicle forceps of the Guyon-Pean design suitable for crushing and grasping pedicle of kidney during nephrectomy.

2. APPLICABLE DOCUMENTS

2.1 Specitications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

| | |
|---|---|
| GG-I-526 | Instruments, Dental and Surgical, General Specifications. |
| PPP-B-566 | Boxes, Folding, Paperboard. |
| PPP-B-585 | Box, Wood, Wirebound. |
| PPP-B-601 | Box, Wood, Cleated-plywood. |
| PPP-B-621 | Box, Wood, Nailed and Lock-corner. |
| PPP-B-636 | Box, Fiberboard. |
| PPP-B-676 | Box, Set-up |

Military

| | |
|---|---|
| MIL-P-116 | Preservation, Methods of |
| MIL-L-10547 | Lines, Case and Sheet, Overwrap; Watervaporproof or Waterproof, Flexible |

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

| | |
|---|---|
| MIL-STD-105 | Sampling Procedures and Tables for Inspection by Attributes. |
| MIL-STD-129 | Marking for Shipment and Storage. |

(Copies of specifications and standards, required by suppliers in connection with specific procurement functions shall be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENT

3.1 General Requirements. The forceps shall be in accordance with the applicable requirements of GG-I-526 and the following option exercises under that specification:

3.2 Material. The forceps shall be fabricated from Class 4, type 410 or type 420 material.

3.3 Hardness. Except for pin, hardness shall be Rockwell C40 to C45, after proper stress relieving.

3.4 Style, design and dimensions. Shall be a kidney pedicle forceps, of the Guyon-Pean design, suitable for crushing and grasping the kidney pedicle during nephrectomy. Shall be in accordance with Figure 1.

3.5 Finish. Finish shall be mirror, or mirror and satin.

3.5.1 Passivation. The entire item shall be properly passivated.


3.6 Lock stiffness. Forceps of box construction shall have shanks tested for lock stiffness in accordance with GG-I-526.

3.7 Identification marking. In addition to GG-I-526 requirements, forceps of foreign manufacture shall also be marked "stainless".



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

[illegible] sample shall be rejected.

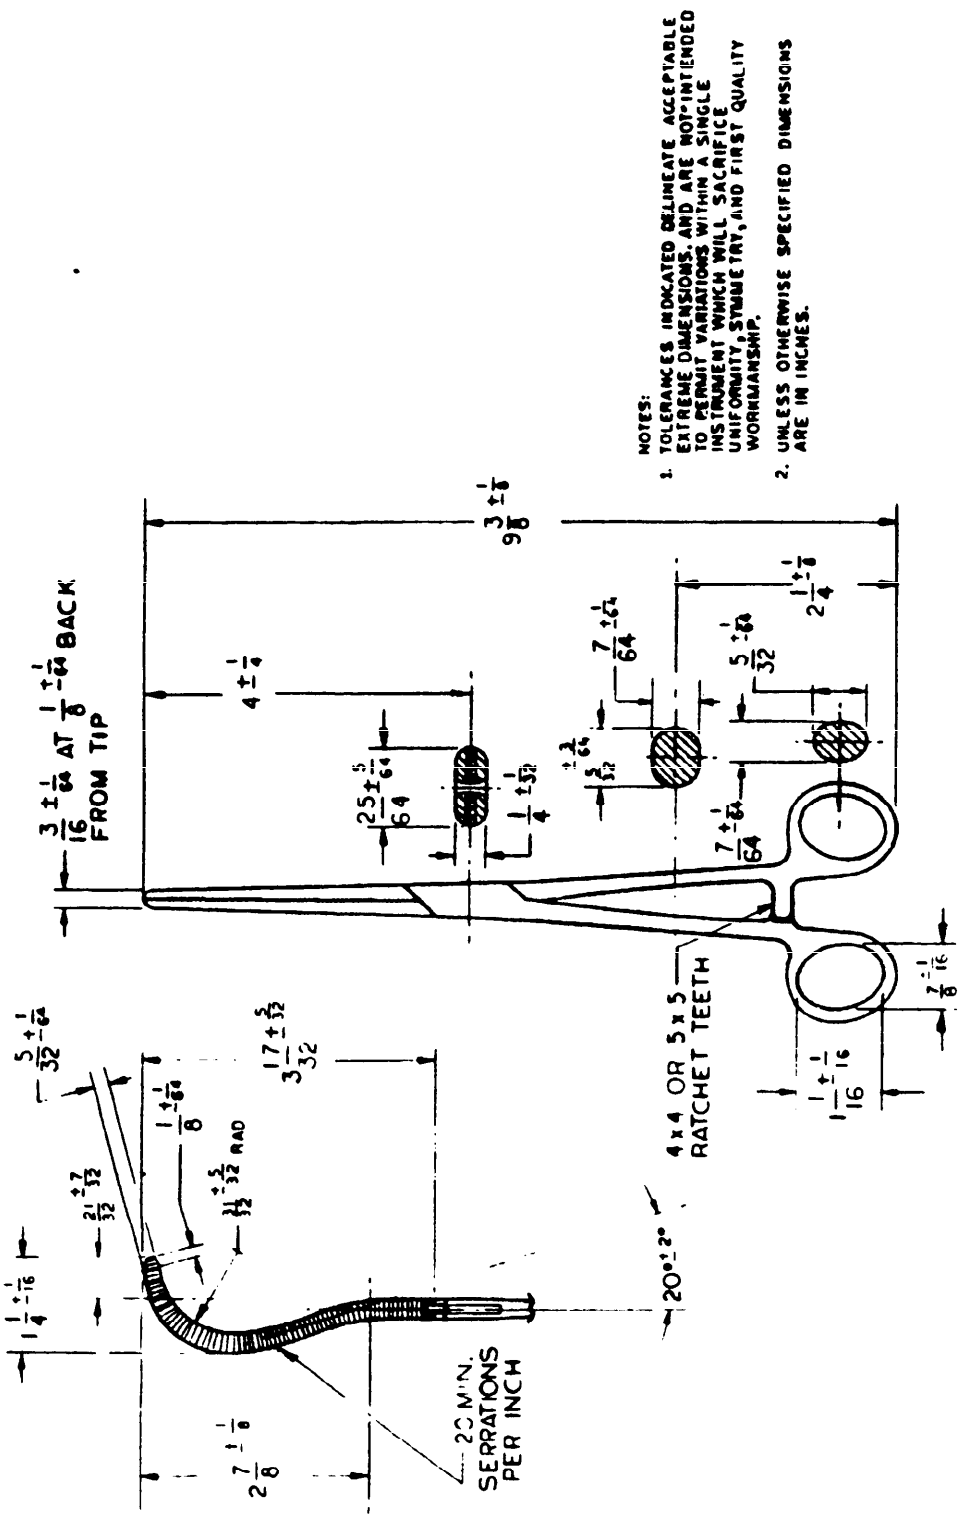


NSN 5515-00-335-5800

FORCEPS, KIDNEY PEDICLE

FIGURE 1



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN. the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in Table I. The unit of product for examination purposes shall be one kidney pedicle forceps.

Table I. Sampling Criteria for Examination

| Type of defect | Inspection level | AQL (Percent defective) |
|---|---|---|
| Major | II | 1.0 |
| Minor | II | 2.5 |

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. Unit of product for test purposes shall be one forceps.

Table II. Sampling Criteria for Tests

| Component | Characteristic | Requirement | Test procedure | Inspection level | AQL |
|---|---|---|---|---|---|
| 1-Forceps | Composition analysis | 3.2 and GG-I-526 | GG-I-526 | ** | * |
| | Hardness | 3.3 and GG-I-526 | GG-I-526 | S-2 | * |
| | Dimensions | 3.4 | -------- | S-2 | 2.5 |
| | Boil test | GG-I-526 | GG-I-526 | S-2 | * |
| | Copper sulfate | GG-I-526 | GG-I-526 | S-2 | * |
| | Box lock stiffness | 3.6 | GG-I-526 | II | 6.5 |

* Acceptance number shall be zero for all sample size.
** Four ounces of each lot of metal used in the construction of the forceps shall be selected for chemical analysis. Wherever feasible, the same sample unit shall be used for the determination of two or more test-characteristics.

4.3 Examination. The forceps shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in Table I and III. Examination however, shall not be restricted to defects listed in Table III. Any forceps in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects

| Categories | Defects |
|---|---|
| Critical | None defined. |
| Major | |
| 101 | Style and design not as specified. |
| 102 | Forceps not free from cracks, pits, dents, nicks, sharp edges and burrs. |
| 103 | Serrations not as specified. |
| 104 | Ratchet teeth not uniform or function poorly. |
| 105 | Forceps not of box lock design. |
| 106 | Forceps not free from excessive play in box lock area. |
| Minor | |
| 201 | Finish not mirror, and not uniform. |
| 202 | Identification marking not present, correct. complete or legible. |

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be Level A or C as specified (see 6.2).

5.1.1 Unit of issue. One forceps, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

| Unit package | Intermediate package | Exterior container |
|---|---|---|
| 1 unit | 6 units | 96 units |

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be throughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Preservative shall not be applied.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue of other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method 1C-2.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-566, PPP-B-676 or PPP-B-636, class domestic. Commercial colors are acceptable on intermediate cartons and closure shall be adequate to prevent spilling of contents under normal handling. Style FPF may be used of PPP-B-636 in lieu of style RSC.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Levels A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof in accordance with paragraph 30.4 of PPP-B-636.

5.2.2 Level B.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The forceps are intended for use in crushing and grasping pedicle of kidney before severing and ligating in removal of kidney.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

6.3 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

| National Stock No. | Item Identification |
|---|---|
| 6515-00-335-5800 | FORCEPS, KIDNEY PEDICLE, Guyon-Pean, 9 inch |

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 6, dated 15 August 1966 for FSN 65115-335-5800.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1764

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval No. 22-R285

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

**DD FORM 1 JAN 72 1426** REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

C 18061

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:45Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.