MIL-F-37010A
13 April 1976
SUPERSEDING
MIL-F-37010
2 October 1973

MILITARY SPECIFICATION

FORCEPS, BIOPSY, UTERINE, GAYLOR, THOMS MODIFICATION

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type and size of uterine biopsy forceps of the Gaylor design, suitable for use in obtaining punch biopsy specimens from the uterine cervix.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

GG-I-526	-	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	-	Boxes, Folding, Paperboard.
PPP-B-585	-	Boxes, Wood, Wirebound.
PPP-B-601	-	Boxes, Wood, Cleated-Plywood.
PPP-B-621	-	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	-	Boxes, Shipping, Fiberboard.
PPP-B-676	-	Boxes, Set-up.

MILITARY

MIL-P-116	-	Preservations, Methods of.
MIL-L-10547	-	Liners, Case, and Sheet, Overwrap; Water-vaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:46Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications and standards, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General requirements. The forceps shall be in accordance with the applicable requirements of GG-I-526 and the following specific requirements.

3.2 Material. The forceps shall be fabricated from Class 4, type 420 material.

3.3 Hardness. After proper stress relieving, the forceps shall have a Rockwell hardness of C40 to C45, with the exception of the screw or pin.


3.4 Style, design and dimensions. The forceps shall be a uterine biopsy forceps of the Gaylor design, Thoms modification. Shall have one of the punch cups with an elevated inner cutting rim which telescopes into the other cup. Shall be in accordance with Figure 1.

3.5 Finish. Finish shall be mirror. Locks and ratchets shall be smooth and shall be polished but need not be buffed to a mirror-finish.

3.6 Identification marking. In addition to GG-I-526 requirements, forceps of foreign manufacture shall also be marked "stainless".

3.7 Performance requirement. The forceps shall be tested as specified in 4.4.1 and shall punch a clean cut hole (without ragged edges or puckering) in the test material. The set of the instrument shall be such that cutting is complete before the first ratchet catch is engaged.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:46Z
Check the source to verify that this is the current version before use.

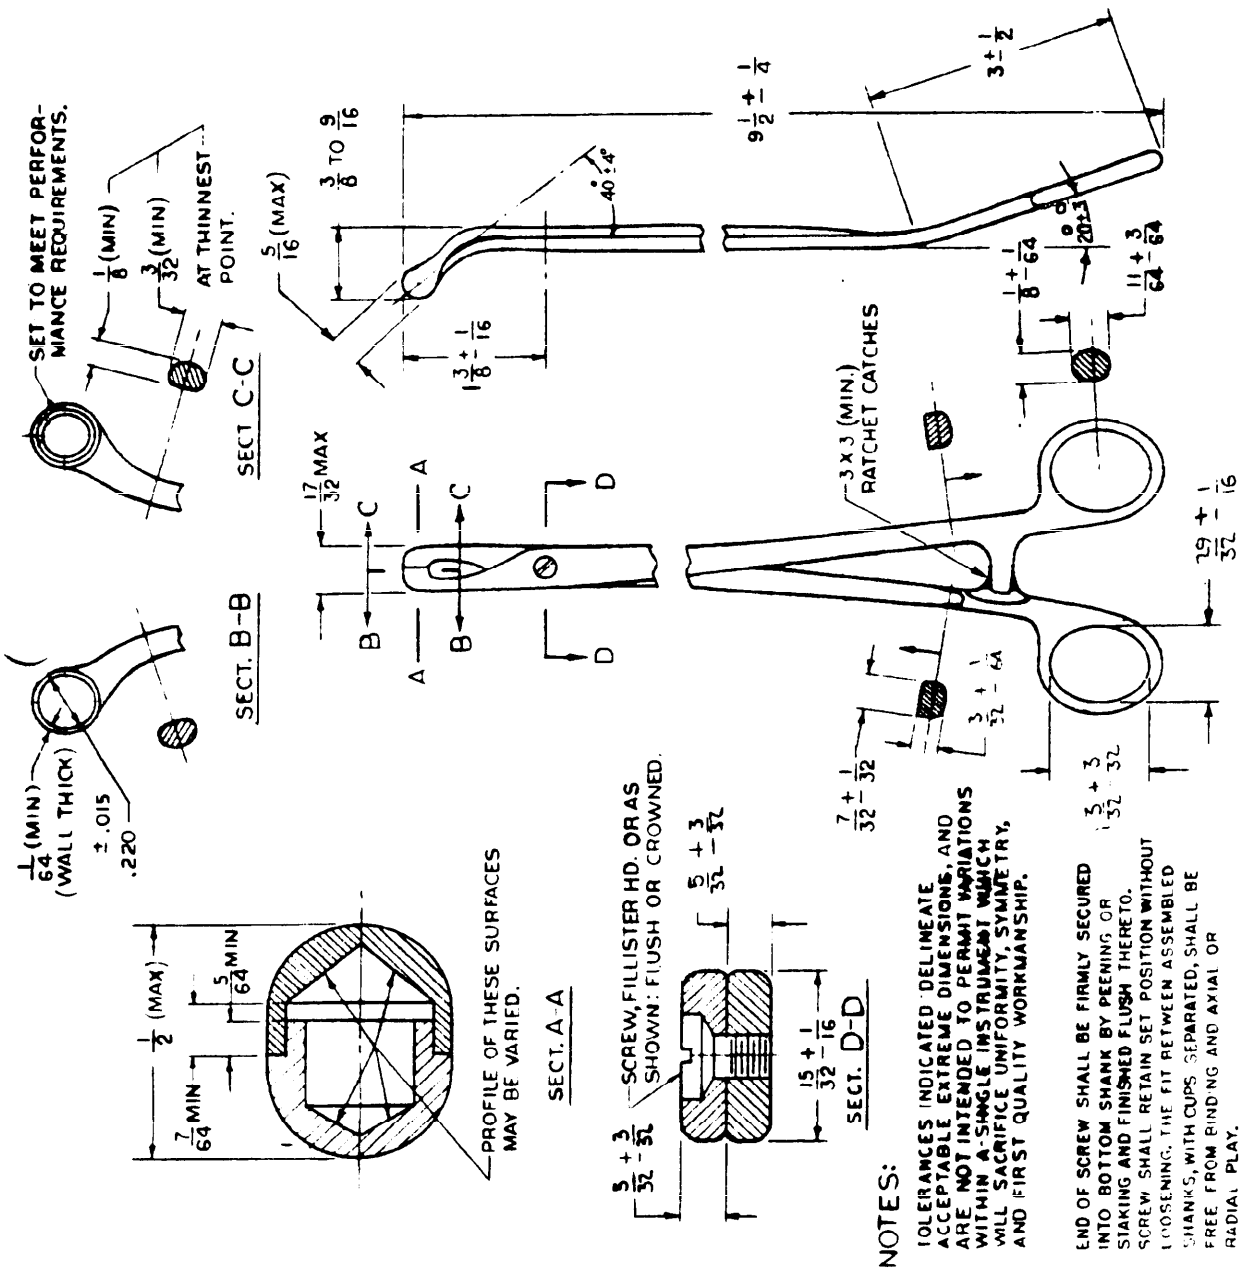

NSN 6515-00-331-0500

Figure 1. Forceps, biopsy, uterine, Gaylor-Thoms modification

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:46Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection shall be in accordance with GG-I-526.

4.1.2 Records. Records of examination and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the corrosion resisting steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificates shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number (NSN), the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, the individual test results, and the specification requirements.

4.2 Sampling.

* 4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in table I. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics. The unit of product for examination purposes shall be one hemostatic forceps.

TABLE I. Sampling criteria for examination

Type of defect	Inspection level	AQL (Percent defective)
Major	II	1.0
Minor	II	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:46Z
Check the source to verify that this is the current version before use.

* 4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table II. Unit of product for test purposes shall be one forceps.

TABLE II. Sampling criteria for tests

Component	Characteristic	Requirement	Test procedure	Insp. level	AQL
1-Forceps	Hardness	3.3 and GG-I-526	GG-I-526	S-2	1.5
	Dimensions	3.4	--------	S-2	2.5
	Boil test	GG-I-526	GG-I-526	S-2	1.0
	Copper sulfate	GG-I-526	GG-I-526	S-2	1.0
	Performance test	3.7	4.4.1	S-2	1.0

* 4.2.3 Raw materials. A sufficient quantity of each lot of metal used in the manufacture of the forceps shall be selected for composition analysis in accordance with GG-I-526.

* 4.3 Examination. The forceps shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in tables I and III. Examination, however, shall not be restricted to defects listed in table III. Any forceps in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.

TABLE III. Classification of defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Forceps not free from cracks, pits, dents, nicks, sharp edges and burrs.
103	Ratchet teeth not uniform, or function poorly.
104	Forceps do not retain set position.
105	Forceps not free from binding.
106	Finish not as specified or not uniform.
Minor	
201	Identification marking not present, correct, complete or legible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:46Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Performance test. The test material shall be newspaper having a thickness of 0.003 inch (plus or minus 0.0005 inch). Two separate consecutive tests shall be made with each instrument. Test material shall be punched, using the forceps in the normal manner (i.e., with the examiner's fingers in the finger rings of the instrument). Forceps not meeting the criteria set forth in 3.7 (for both tests per instrument) shall be considered defective.

* 4.5 Packaging inspection. The inspection of the preservation-packaging and interior package marking shall be in accordance with the group A and B quality conformance inspection requirements of MIL-P-116. The inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

5. PACKAGING

5.1 Preservation-packaging. Preservation-packaging shall be level A or C, as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Cleaning and drying. Each forceps shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.1.2 Preservative. Preservative shall not be applied.

5.1.1.3 Unit packaging. Each forceps shall be wrapped in neutral tissue or other suitable anticorrosive material. Each forcep shall be further packaged in accordance with MIL-P-116, IC-2.

5.1.1.4 Intermediate packaging. Six (6) forceps shall be packaged in a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class domestic. Closure shall be as specified in the appendix of the box specification.

5.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:46Z
Check the source to verify that this is the current version before use.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.1).

5.2.1 Level A. One hundred forty-four (144) forceps shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraph of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed as specified in the appendix of PPP-B-636.

5.2.2 Level B. One hundred forty-four (144) forceps shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601 domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking. Each unit, intermediate package and each exterior container shall be marked as specified in MIL-STD-129.

6. NOTES

6.1 Intended use. The uterine biopsy forceps are intended for use in obtaining punch biopsy specimens from the uterine cervix.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(c) National stock number.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:46Z
Check the source to verify that this is the current version before use.

6.3 National Stock Number coverage. This specification covers the following item appearing in the Federal Supply Catalog:

National Stock No.	Item Identification
6515-00-331-0500	FORCEPS, BIOPSY, UTERINE, GAYLOR, THOMS MODIFICATION, 9-1/2 inch

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and Contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the previous issue.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1984

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:46Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-F-37010A FORCEPS, BIOPSY, UTERINE, GAYLOR, THOMS MODIFICATION

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:46Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:46Z
Check the source to verify that this is the current version before use.