MIL-H-37020
12 December 1973

MILITARY SPECIFICATION

HANDLE, BONE CUTTING WIRE SAW, GIGLI

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers two styles of Gigli bone cutting wire saw handles suitable for use with a conductor and wire saw in neurosurgery.

1.2 Classification. Handles covered by this specification shall be of the following style:

Style I - Gigli

Style II - Strully modification.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical, General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-plywood.
PPP-B-621	Box, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Set-up.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case and Sheet, Overwrap; Watervaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS


3.1 General requirements. The handles shall be in accordance with the applicable requirements of GG-I-526 and the following option exercises under that specification:

3.2 Material. The handles shall be fabricated from Class 3, type 302, 303 or 304 material or Class 4, type 420 material.

3.3 Hardness. After proper stress relieving, handles fabricated of Class 3 material shall have a Rockwell hardness of B-75 to B-85. When fabricated of Class 4 material, after proper stress relieving, Rockwell hardness shall be C-40 to C-45.

3.4 Style design and dimensions. The handles shall be used with bone cutting wire saws. Shall be in accordance with Figure 1 (for style I) or Figure 2 (for style II). Shall be furnished in pairs. Shall be suitable for use with NSN 6515-00-363-2300 Conductor, Bone Cutting Wire Saw and NSN 6515-00-363-2700 Saw, Bone Cutting, Wire, 20 inch.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.

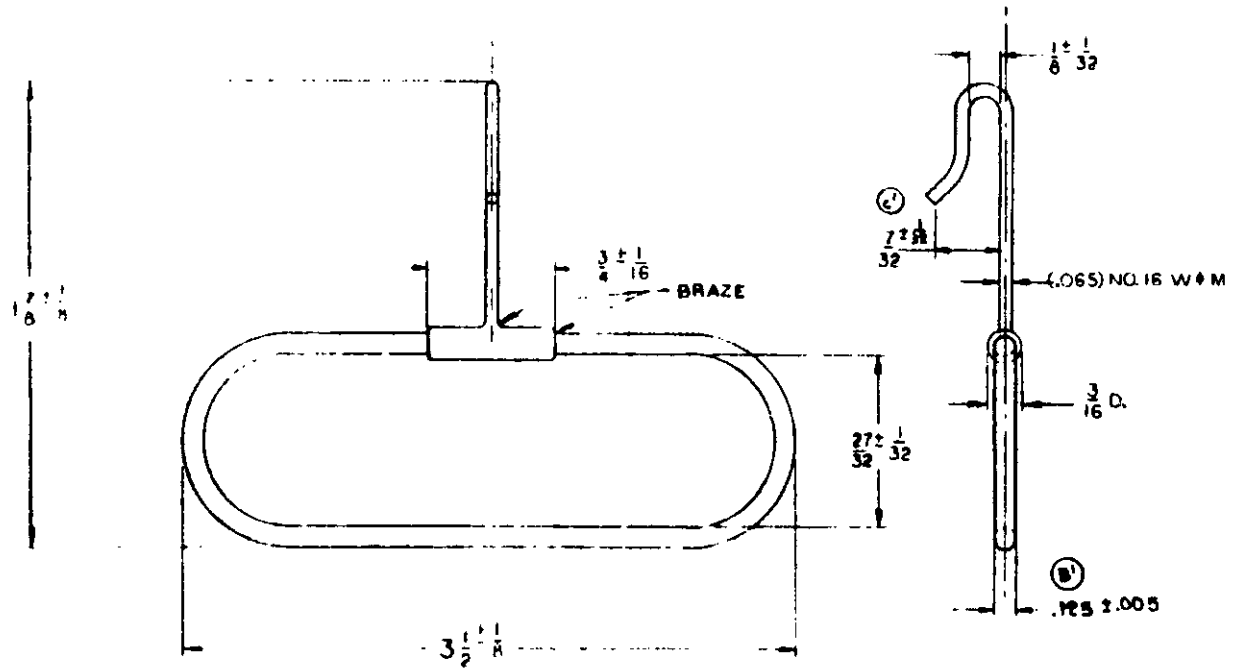

NSN 6515-(X)-363-2400

STYLE I (c)

20620

(B')


DEFENSE PERSONNEL SUPPORT CENTER
DIR. OF MEDICAL MATERIEL PHILA PA

HANDLE, BONE CUTTING WIRE SAW, GIGLI

FIG. 1

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.

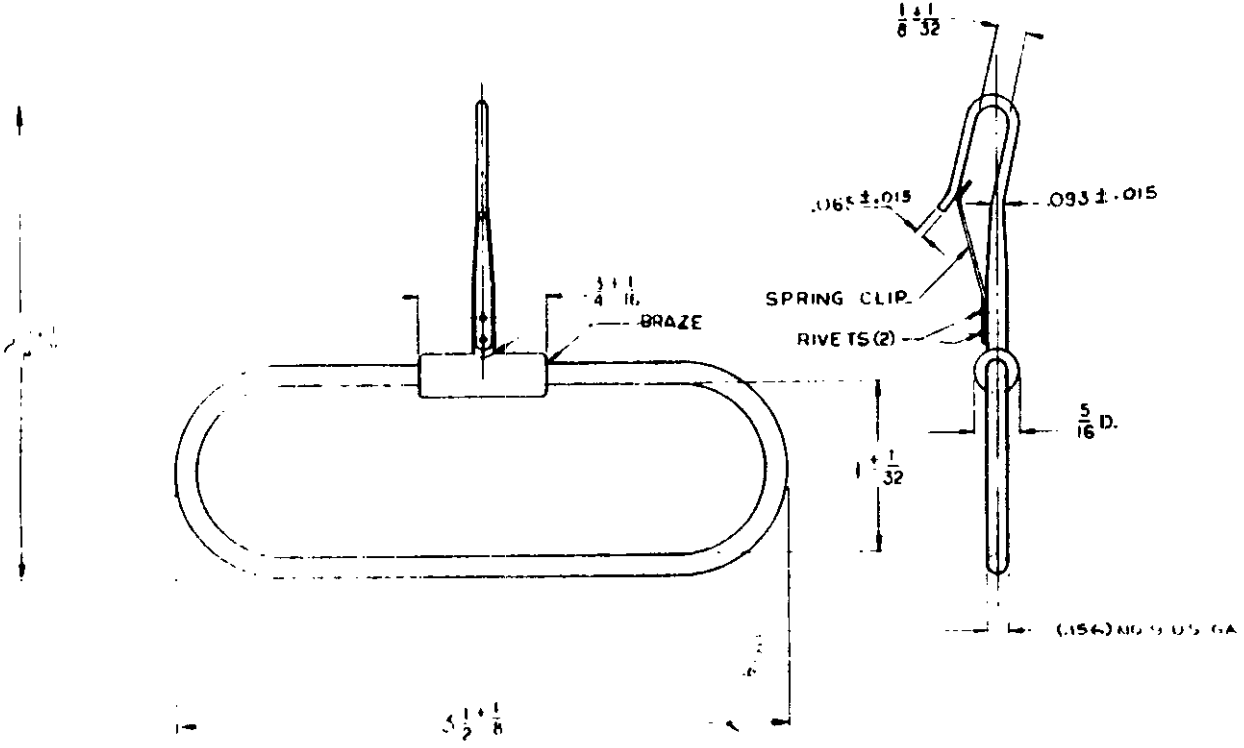

(A)

NSN 6515-00-363-2400

STYLE II (B)

(B2)

DEFENSE PERSONNEL SUPPORT CENTER
DIR. OF MEDICAL MATERIEL PHILA PA

HANDLE, BONE CUTTING WIRE SAW, GIGLI

FIG. 2

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.

3.5 Finish. Shall be mirror finish.

3.6 Identification marking. In addition to GG-I-526 requirements, handles of foreign manufacture shall also be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.

4.2 Sampling

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in Table I. The unit of product for examination purposes shall be one handle.

Table I. Sampling Criteria for Examination

Type of defect	Inspection level	AQL (Percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in the following Table II. The unit of product for test purposes shall be one handle.

Table II. Sampling Criteria for Tests

Component	Characteristic	Rqmt.	Test procedure	Insp. level	AQL
Handle	Hardness	3.3	GG-I-526	S-2	*
	Boil test	GG-I-526	GG-I-526	S-2	*
	Copper sulfate	GG-I-526	GG-I-526	S-2	*
	Composition analysis	3.2 and GG-I-526	GG-I-526	**	*

* Acceptance number shall be zero for all sample sizes.
** Four ounces of each lot of metal used in the construction of the handles shall be selected for chemical analysis. Wherever feasible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination. The handles shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in Table I and III. Examination, however, shall not be restricted to defects listed in Table III. Any handle in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Handles not free from cracks, pits, dents, nicks, sharp edges and burrs.
103	Hook not capable of securely holding wire.
Minor	
201	Finish not mirror.
202	Identification marking not present, correct, complete, or legible

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One handle, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in the following table shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	576 units

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Preservative shall not be applied.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method 1C-1.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors will be acceptable; or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements of applicable table shall apply for PPP-B-636 box.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof in accordance with paragraph 30.4 of PPP-B-636.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The handles are intended for use with Gigli wire bone saws in neurosurgery.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

National Stock No.	Item Identification
6515-00-363-2400	HANDLE, BONE CUTTING WIRE SAW, Gigli

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 8, dated 20 May 1968 for FSN 6515-363-2400 HANDLE, BONE CUTTING WIRE SAW, Gigli.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1787

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:47Z
Check the source to verify that this is the current version before use.