FED. SUP CLASS
6630

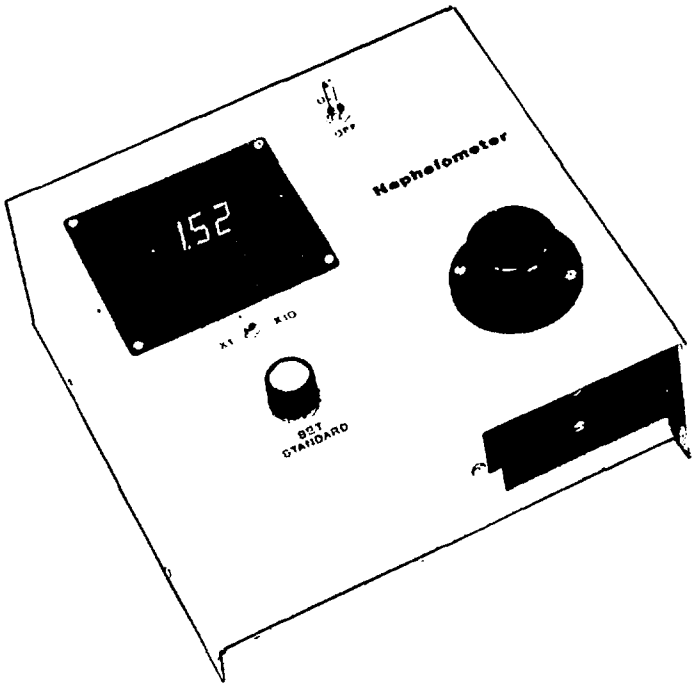

MATERIAL: Case shall be made of aluminum. All other parts and material shall be as required for proper operation of the instrument.

DESIGN: The nephelometer shall be approximately ten inches square and four inches high. It can be equipped with either a digital meter as shown or an analog meter. The power source shall be 50 to 60 Hz AC 105 to 130 volts or 210 to 260 volts, 40 watts and may also be operated from DC inverter for field use. It shall be readable to ±0.5% of 0.01 NTU on the 0-9.99 NTUs range and 0.1 NTUs on the 0-99.9 range with reproducibility of ±2% of full scale.

All electrical components shall conform to the standards of Underwriters Laboratories, Incorporated.

NOTE: Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements specified herein.

USER ACTIVITIES: ARMY - MD, DM
NAVY - MS

REVIEWER ACTIVITIES: ARMY - ME
NAVY - OS
AIR FORCE - 82

APPROVED 20 MAY 1983 REVISED

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A. EA	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust MS 99		NEPHELOMETER, INTEGRATING	MS51448
Procurement Specifications NONE	SUPERSEDES:		SHEET 1 OF 1

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

PROJECT NUMBER 6630-0354

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T18:02Z
Check the source to verify that this is the current version before use.