INCH-POUND

MIL-H-42076
6 March 1992
SUPERSEDING
GG-H-00584A(DSA-DM)
19 March 1974
GG-H-584
20 September 1960

MILITARY SPECIFICATION

HOLDERS, HOSPITAL BED PATIENT IDENTIFICATION CARD

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers cardholders for patient identification suitable for attachment to the rail at the foot end of a hospital bed.

1.2 Classification.

1.2.1 Types. The holders shall be of the following types:

Type I - Aluminum, for hospital beds with square tubing.

Type II - Carbon steel, for hospital beds with round tubing.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, DPSC-MST, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal, (DD Form 1426) appearing at the end of this document or by letter.

AMSC/NA FSC 6530

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.

2. APPLICABLE DOCUMENTS

2.1 Government Documents.

2.1.1 Specifications, standards, and handbooks. The following specifications, standards, and handbooks form a part of this document to the extent specified herein. Unless otherwise specified, the issues of these documents shall be those listed in the issue of the Department of Defense Index of Specifications and Standards (DoDISS) and supplement thereto, cited in the solicitation (see 6.2).

SPECIFICATIONS

Federal

QQ-A-250\2	-	Aluminum Alloy 3003, Plate and Sheet
PPP-B-566	-	Boxes, Folding, Paperboard
PPP-B-601	-	Boxes, Wood, Cleated - Plywood
PPP-B-621	-	Boxes, Wood, Nailed and Lock-Corner
PPP-B-636	-	Boxes, Shipping, Fiberboard
PPP-B-676	-	Boxes, Setup

Military

MIL-P-116	-	Preservation, Methods Of
MIL-L-10547	-	Liners, Case, and Sheet, Overwrap; Water Vaporproof, or Waterproof, Flexible

STANDARDS

Military

MIL-STD-105	-	Sampling Procedures and Tables for Inspection by Attributes
MIL-STD-129	-	Marking for Shipment and Storage
MIL-STD-147	-	Palletized Unit Loads
MIL-STD-794	-	Parts and Equipment, Procedures for Packaging and Packing of

(Unless otherwise indicated, copies of federal and military specifications, standards, and handbooks are available from:

Standardization Documents Order Desk
Building 4D
700 Robbins Avenue
Philadelphia PA 19111-5094).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.

2.1.2 Other Government documents, drawings and publications. The following other Government documents, drawings, and publications form a part of this document to the extent specified herein. Unless otherwise specified, the issues are those cited in the solicitation.

2.2 Non-Government publications. The following documents form a part of this document to the extent specified herein. Unless otherwise specified, the issues of the documents which are DoD adopted are those listed in the issue of the DoDISS cited in the solicitation. Unless otherwise specified, the issues of documents not listed in the DoDISS are the issues of the documents cited in the solicitation (see 6.2).

AMERICAN IRON AND STEEL INSTITUTE (AISI)

Steel Products Manual, Stainless and Heat Resisting Steel

(Application for copies should be addressed to the American Iron and Steel Institute, 150 East 42nd Street, New York, NY 10017).

(Non-Government standards and other publications are normally available from the organizations that prepare or distribute the documents. These documents also may be available in or through libraries or other informational services.)

2.3 Order of precedence. In the event of a conflict between the text of this document and the references cited herein (except for related associated detail specifications, specification sheets, or MS standards), the text of this document takes precedence. Nothing in this document, however, supersedes applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 Material.

3.1.1. Aluminum alloy. The aluminum alloy shall be alloy 3003-H14 in accordance with QQ-A-250/2.

3.1.2 Carbon-steel. The carbon steel sheet shall be not less than 0.0239 inch thick (No. 24 standard gage).

Source: https://assist.dla.mil -- Downloaded: 202610-21T20:20Z
Check the source to verify that this is the currentversion before use.

3.1.3 Corrosion-resisting steel. The corrosion-resisting steel shall be American Iron and Steel Institute (AISI) type 302 or 304.

3.1.4 Felt. The felt shall be lining grade, gray or black.

3.2 Construction.

3.2.1 Type I. The type I hospital bed patient identification cardholder shall be in accordance with figure 1. The holder shall be hinged to afford ease in reading the contained card. The hinge shall be of the piano type, and shall be formed integrally with the cardholder and hook portions. The hinge shall incorporate a position stop to prevent the cardholder from striking the bed slats when the cardholder is raised for reading and then released.

The hook portion shall be formed of 0.051 inch thick (No. 16 standard gage) American Iron and Steel Institute (AISI) type 3003-H14 aluminum alloy. The body portion shall be formed from not less than 0.045 inch thick (No. 17 standard gage) type 3003-H14 aluminum alloy. The hinge pin shall be made of AISI type 302 or 304 corrosion-resisting steel.

The hook portion shall be covered with a black neoprene rubber coating applied by dipping. The coating shall be securely bonded to the aluminum metal. As an alternate, the hooks shall be hot dipped with black plastisol material. The thickness of the plastisol shall be the same as specified for the rubber. The thickness of the coating on each side of the hook portion shall be not less than 0.032 inch (not less than 0.064 inch total thickness on each hook).

3.2.2 Type II. The type II hospital bed patient identification cardholder shall be in accordance with figure 2. The cardholder shall be fabricated from one piece of carbon steel sheet not less than 0.0239 inch thick (No. 24 standard gage). The bolt shall be a slotted roundhead machine screw with screwpost, each not less than one inch long. The bolt and screwpost shall be corrosion-resisting steel or brass or carbon steel, zinc coated.

The inside surface of the holder which grips the bedpost shall be lined with a 1/16 inch thick gray or black, lining grade, felt liner securely cemented in place. The cardholder shall be furnished completely assembled with the bolt and nut in proper position.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.

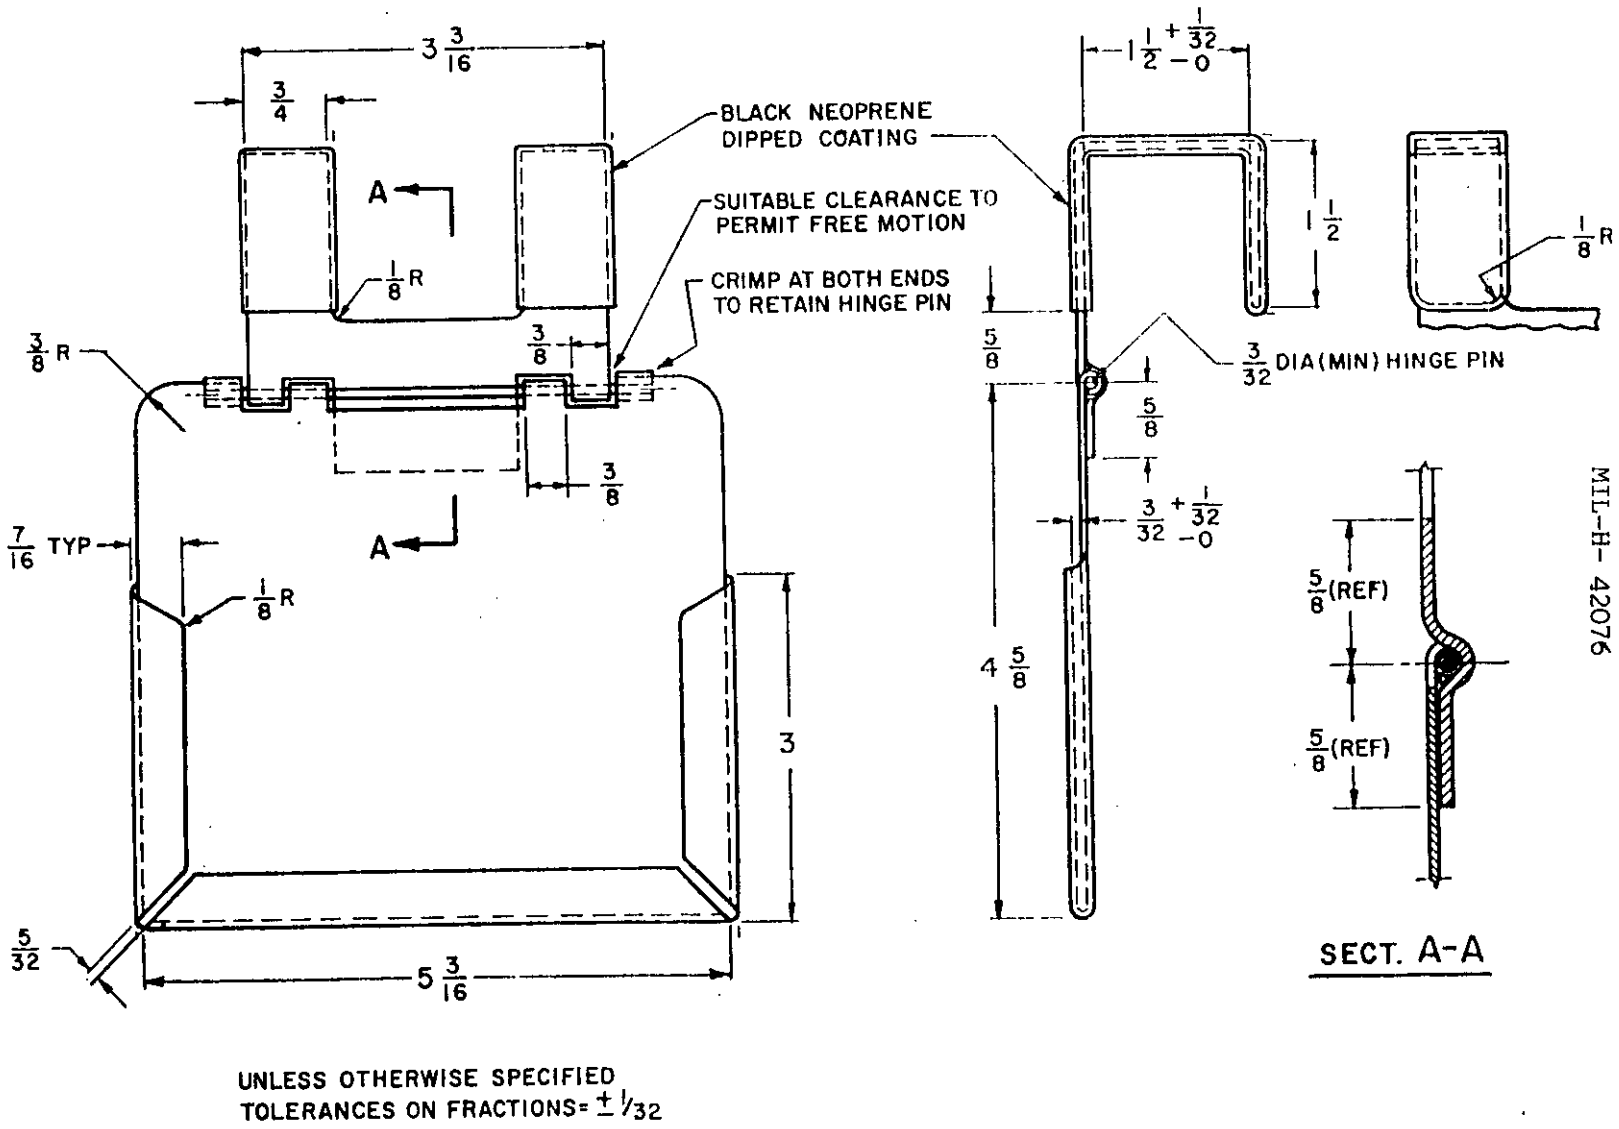


FIGURE 1. Holder, Hospital Bed Patient Identification Card.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.

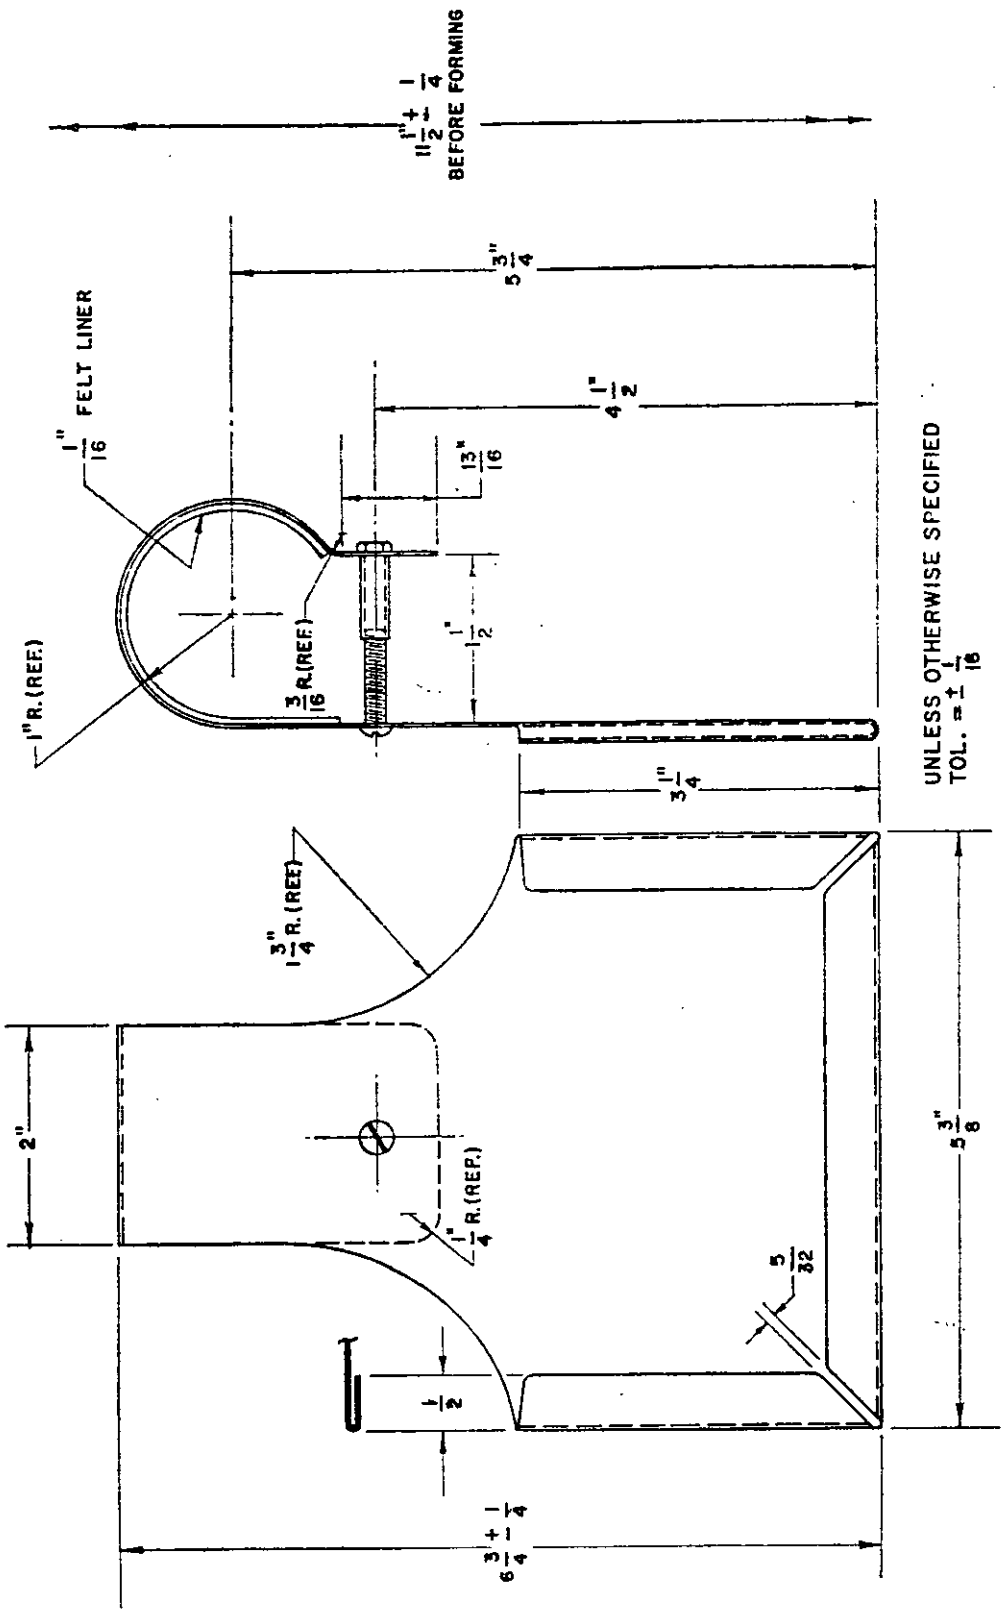


FIGURE 2. Holder, Hospital Bed Patient Identification Card.

Source: https://assist.dla.mil -- Downloaded: 2026Ø10-21T20:20Z
Check the source to verify that this is the current version before use.

3.3 Finish.

3.3.1 Type I. The cardholder shall be polished or burnished to remove surface imperfections and burrs, then thoroughly cleaned and chemically degreased.

3.3.2 Type II. The cardholder shall be bright zinc plated.

3.4 Identification marking. Each holder shall be permanently stamped with the National Stock Number, the contract or purchase order number, the letters U.S., and the name or registered trademark of the manufacturer. Marking shall be clear, legible, and distinct. Marking secured by adhesives shall not be acceptable.

3.5 Workmanship. The holder shall be free of cracks, tears, and ruptures. Exposed and acessible edges, corners, and surfaces, shall be free of burrs. The holder shall be free from defects which detract from its appearance or which may affect its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements (examinations and tests) as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to ensure supplies and services conform to prescribed requirements.

4.1.1 Responsibility for compliance. All items shall meet all requirements of sections 3 and 5. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in the specification shall not relieve the contractor of the responsibility of ensuring that all products or supplies submitted to the Government for acceptance comply with all requirements of the contract. Sampling inspection, as part of manufacturing operations, is an acceptable practice to ascertain conformance to requirements, however this does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to accept defective material.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.

4.1.2 Records. Records of examinations and tests performed by, or for, the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract, and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.3 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.4 Certificates of quality. Certificates of quality supplied by the manufacturer of the component or material may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number (NSN), the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and table I. The unit of product for examination purposes shall be one identification cardholder.

TABLE I. Sampling for examination.

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Minor defects	II	4.0
For dimensional examination	S-2	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-3. The unit of product for test purposes shall be one identification cardholder.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.

4.3 Examination. The identification card holder shall be examined for defects including, but not limited to, those listed in table II.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table II below. Examination shall not be restricted to the classification of possible defects.

TABLE II. Categories and defects.

Categories	Defects
Major	
101	Holder not free of cracks, tears, and ruptures
102	Exposed and accessible edges, corners, and surfaces, not free of burrs
103	Construction does not permit ready insertion and removal of card
104	Hinge not securely attached to type I holder
105	Screwpost and machine screw of type II holder are not properly aligned and do not engage properly
106	Type II holder not of one-piece construction
107	Finish not as specified
Minor	
201	Hinge not crumped at each end to retain hinge pin (type I holder)
202	Neoprene coating nonadherent (type 1 holder)
203	Felt lining not securely cemented in place (type II holder)
204	Position stop does not perform intended function (type I holder)
205	Identification marking not complete, legible, or permanent
206	Hinge does not move freely without binding (type I holder)

4.3.2 Dimensional examination. The holder shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

Source: https://assist.dla.mil -- Downloaded: 202610-21T20:20Z
Check the source to verify that this is the currentversion before use.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

4.5 Inspection of packaging. The sampling and inspection of the preservation and interior package marking shall be in accordance with groups A and B quality conformance inspection requirements of MIL-P-116. The sampling and inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

5. PACKAGING

5.1 Preservation. Preservation shall be level A or C, as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Cleaning and drying. Each holder shall be cleaned and in accordance with MIL-P-116.

5.1.1.2 Preservative applications. Preservatives shall not be used.

5.1.1.3 Unit package. Each holder shall be packaged in accordance with MIL-P-116, method IC-1.

5.1.1.4 Intermediate package. Twelve unit packages containing holders shall be packaged in a box conforming to PPP-B-566, PPP-B-636, class domestic or PPP-B-676. Closure shall be as specified in the applicable box specification.

5.1.2 Level C.

5.1.2.1 Unit package. Preservation for the holders shall conform to the requirements of MIL-STD-794 for level C.

5.1.2.2 Intermediate package. Twelve intermediate packages (144 units) containing holders shall be packaged in accordance with the requirements of MIL-STD-794 for level C.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.2).

5.2.1 Level A. Twelve intermediate packages (144 units) containing holders shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, overseas type, PPP-B-621, class 2, or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the applicable box specification

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall be as specified in the liner specification. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed as specified in PPP-B-636.

5.2.2 Level B. Twelve intermediate packages (144 units) containing holders shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, domestic type, PPP-B-621, class 1, PPP-B-636, class domestic. Closure shall be as specified in the applicable box specification.

5.2.3 Level C. Twelve intermediate packages (144 units) containing holders shall be packed in accordance with the requirements of MIL-STD-794 for level C.

5.2.4 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.2.5 Unitized loads. Unitized loads, commensurate with the level of packing specified in the contract or order, shall be used whenever total quantities for shipment of one destination exceed 250 pounds or 20 cubic feet. Loads shall be unitized on pallets conforming to MIL-STD-147. Quantities less than 20 cubic feet need not be unitized. Pallet loads including the pallet shall not exceed 43 inches in length, 52 inches in width, and 54 inches in height. Pallet shall conform to type IV or type V.

5.2.5.1 Levels A and B. Holders packed as specified in 5.2.1 and 5.2.2 shall be unitized on pallets as specified in 5.2.5.

5.2.5.2 Level C. Holders packed as specified in 5.2.3 shall be unitized as specified in MIL-STD-794.

Source: https://assist.dla.mil -- Downloaded: 202610-21T20:20Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Levels A, B and C. Each unit pack, intermediate package, exterior container and unitized load shall be marked as specified in MIL-STD-129.

5.4 General.

5.4.1 Exterior container. Exterior container (see 5.2.1, 5.2.2, and 5.2.3) shall be of minimum tare and cube consistent with the protection required and shall contain equal quantities of identical stock numbered items to the greatest extent practicable.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.5.

6. NOTES

(This section contains information of a general or explanatory nature that may be helpful, but is not mandatory.)

6.1 Intended use. The hospital bed patient identification card holder is intended to hold an ID card which shows the patient's name and other pertinent data.

6.2 Acquisition requirements.

a. Title, number, and date of the specification.

b. Issue of DODISS to be cited in the solicitation and if required, the specific issue of individual documents referenced (see 2.1).

c. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

d. National Stock Number

6.3 Subject term (key word) listing

Cardholder
Clinic
M.U.S.T.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.

6.4 National Stock Number (NSN) coverage. This specification covers the following items as listed in the Federal Supply Catalog.

NSN	Item Identification	Type
6530-00-781-8450	HOLDER, HOSPITAL BED PATIENT IDENTIFICATION CARD, Aluminum	I
6530-00-781-8475	HOLDER, HOSPITAL BED PATIENT IDENTIFICATION CARD, Steel	II

6.5 Commodity coverage. This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the type which is normally procured to meet requirements.

6.6 Changes from previous issue. Marginal notations are not used in this revision to identify modifications, additions, corrections, and deletions from the previous issue due to the extensiveness of the changes.

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing activity:

DoD - MB

Review activities:

Army - TM
Navy - YD
Air Force - 50

Agent:

DLA - DM

Civil Agency Coordinating Activities:

FDA - MPQAS
USPHS
VA - OSS

Project No. 6530-2240

Location: CARDM13A.DOC

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	MIL-H-42076	6 March 1992

3. DOCUMENT TITLE
HOLDERS, HOSPITAL BED PATIENT IDENTIFICATION CARD

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME DEFENSE PERSONNEL SUPPORT CENTER ATTN: DPSC-MSE	b. TELEPHONE (Include Area Code) (1) Commercial: AC 215-737-2870 (2) AUTOVON: AV 444-2870
c. ADDRESS (Include Zip Code) 2800 SO. 20TH STREET PHILADELPHIA, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous editions are obsolete — 98/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:20Z
Check the source to verify that this is the current version before use.