A-A-30100B
July 24, 1991
SUPERSEDING
A-A-30100A
July 1, 1986

COMMERCIAL ITEM DESCRIPTION

RAZOR, SURGICAL PREPARATION, Safety, Disposable

The General Services Administration has authorized the use of this commercial item description.

This commercial item description describes a double-edged, disposable, safety razor with a coated stainless steel blade suitable for use in surgical preparation.

Salient characteristics:

Classification. The surgical preparation razor shall be of the following types:

Type I - Sterile
Type II - Nonsterile

The safety razor shall consist of a handle, a double-edged blade and a protective cover, assembled to provide a functional disposable razor with a protective shield. Type I razor shall be sterile and packaged to insure sterility.

Materials.

Razor (without blade). The razor shall be fabricated of polystyrene, polypropylene, or styrene-butadiene, with a minimum average tensile strength of 3000 pounds per square inch (p.s.i.), when tested as specified in ASTM D638, and a minimum Izod impact strength of 0.45 foot pound force per inch (ft. lbf./in.) of notch 23 Centrigrade, when tested as specified in ASTM D256. As an alternate, razor handle and blade seat shall be fabricated of styrene-butadiene molding and extrusion material, and the blade cover shall be fabricated of polystyrene.

Blade. The cutting blade shall be fabricated from corrosion-resisting steel containing 0.90 to 1.05 percent carbon, 0.15 to 0.25 percent silicon, 0.90 to 1.10 percent manganese, 12.0 to 14.0 percent chromium, and maximums of 0.040 percent phosphorus and 0.040 percent sulfur. As an

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:36Z
Check the source to verify that this is the current version before use.

alternate, the corrosion-resisting steel shall contain 0.53 to 0.70 percent carbon, 0.15 to 0.50 percent silicon, 0.20 to 0.80 percent manganese, 12.0 to 14.70 percent chromium, and maximums of 0.030 percent phosphorus and 0.025 percent sulfur. The beveled edge shall be treated with a fluorocarbon-telomer coating such as polytetrafluoroethylene or shall have a fine silicon fluid coating.

Design and construction. Type I razor shall be a sterile razor and Type II razor shall be a nonsterile razor. Both types of razors shall be double-edged and disposable with a coated stainless steel blade suitable for use in surgical procedures. The safety razor shall consist of a handle and head (frame and cap) which permanently secures the blade. Razor shall be of the disposable type, as shown in Figure 1 and shall conform to the following dimensions:

Overall length:	3-5/8 to 4-1/8 inches (9.21 to 10.48 cm)
Length of handle:	3-1/4 to 3-9/16 inches (8.26 to 9.05 cm)
Length of head:	1-1/2 to 1/7/8 inches (3.81 to 4.76 cm)
Width of head:	7/8 to 1-1/8 inches (2.22 to 2.86 cm)
Handle diameter (when round) or handle width across flats (when rectangular) at smallest cross section.	1/4 inch (0.64 cm) minimum

Razor shall have a protective cover (plastic or cardboard) fitting over the blade. Cover may be snap-off type or may slide over the head of the razor. Razor shall have from 9 to 10 teeth on both sides of the razor head. As an alternate, one side of the razor head may be smooth with the other side having from 9 to 10 teeth. The teeth shall be spaced and beveled to prevent clogging and to facilitate rinsing. In figure 1, the teeth on the corners shall be wide enough to prevent scratching of the tissue. The assembly of the head frame, cap and blade shall be properly orientated with respect to each other, to preclude any movement of the blade cutting edge. The assembly shall not

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:36Z
Check the source to verify that this is the current version before use.

exhibit clearance at the interface of the head frame, cap and blade. The straight beveled edges of the blade shall be parallel and equidistant from the tips of the razor head teeth. The handle of the razor shall have a suitable gripping surface to minimize slippage during use. Gripping surface may be of any design shown in Figure 1.

Blade. The blade shall be a coated stainless steel blade and shall be permanently assembled in the razor. Each cutting edge of the blade shall be 1-7/16 + or - 1/16 inches (3.65 cm + or - 0.157 cm) in length and shall be exposed from beneath the cap of the razor no less than 1/32 inch (0.079 cm) and no more than 1/20 inch (0.127 cm). Thickness of the blade shall be from 0.0036 to 0.0067 inch (0.0091 to 0.017 cm).

Color. The color of the razor shall be the manufacturer's option.

Sterility. Type I razor shall be sterile when tested for sterility in accordance with the method specified in the U.S.P. or A.A.M.I. guidelines.

Hardness of blade. The coated blade shall be uniformly hardened to the hardness range indicated below for the applicable composition, when tested in accordance with ASTM Designation E18 or E92 and E140, or equivalent British Standard Method.

Material	Rockwell superficial hardness number 30-N scale 1/	Vickers hardness number 2/
Regular (0.90 to 1.05 % carbon)	68-73	500-600
Alternate (0.53 to 0.70 % carbon)	71-76	550-650

1/ using a 30-kilogram force (kgf) load and superficial diamond penetrator.

2/ using a 5-kgf load.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:36Z
Check the source to verify that this is the current version before use.

Finish of the blade (uncoated). The cutting edges of the blade shall be bilaterally ground and honed to razor sharpness. The final honed bevels shall be flat, smooth, and continuous throughout the entire length of the blade. Except for the extreme 1/8 inch (0.32 cm) at either end, the cutting edge shall be free from micro-cracks, and no more than 5% of the edge length shall show nicks, notches, or unhoned portions when viewed microscopically. The remainder of the blade shall have a smooth and bright polished finish. The entire blade shall be free from rust, scale, burrs, pits and cracks.

Identification marking. The razor and blade shall be permanently and legibly marked with the name or trademark of the manufacturer.

Workmanship. The safety razor shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG).

Type I. One package containing 100 individualy packaged sterile razors, constitutes one unit. The individual package shall be a sealed peel-open type container capable of maintaining sterility of contents, unless the package is damaged or opened.

Type II. One package containing 100 nonsterile razors, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:36Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection, examination, and test characteristics. The unit of product for inspection, examination, test purposes shall be one safety razor of each type. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, except for dimensions which shall be conducted at inspection level S-1, and sampling for tests (when applicable) shall be conducted at inspection level S-1.

Tests. Tests shall be conducted to determine compliance with this commercial item description requirements.

Chemical analysis. In the absence of contractor certification for the raw material, a chemical analysis shall be conducted. The chemical analysis shall be performed by reagent solutions, combustion methods, nonemission methods, or by spectrochemical analysis. Any ASTM method shall be acceptable.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:36Z
Check the source to verify that this is the current version before use.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to detemine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contract certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to the degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receivng activity, and shall conform to applicable carrier's rules and regulations. Intermediate and external package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:36Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Numbers are covered by this document:

6515-01-098-5805 Type I

6515-01-322-5898 Type II

Copies of Federal Standard No. 376, Preferred Metric Units for General use by the Federal Government and MIL-STD-105, Sampling Procedures and Tables for Inspection by Attributes, may be obtained by writing Commanding Officer, Navy Publications and Form Center, (code 1032), 5801 Tabor Avenue, Philadelphia, PA 19120.

Ordering data. Purchasers should select the preferred options permitted herein, and include the following information in procurement documents:

(a) Title, number, and date of this commercial item description.
(b) Type of razor.

MILITARY INTERESTS:

Military Coordinating Activity:

DoD-MB

CIVIL AGENCY COORDINATING ACTIVITIES:

PHS
FDA-MPQAS

PREPARING ACTIVITY:

VA-OSS VAMKC (904)
Agent VA-OSS VACO (92A)

AGENT:


DLA-DM

Custodians:


Army-MD
Navy-MS
Air Force-03

Project No. 6515-5118

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:36Z
Check the source to verify that this is the current version before use.

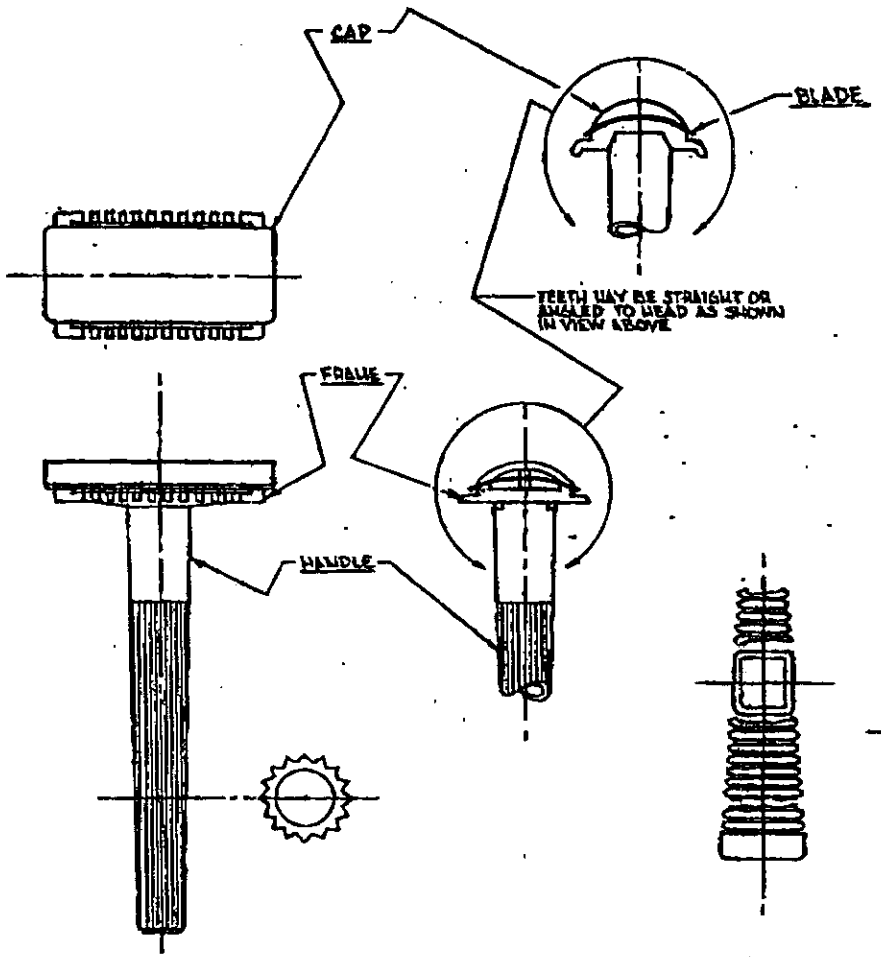

NOTE:
THE ILLUSTRATIONS SHOWN ABOVE ARE TYPICAL FOR THE TYPES IN THIS SPECIFICATION.

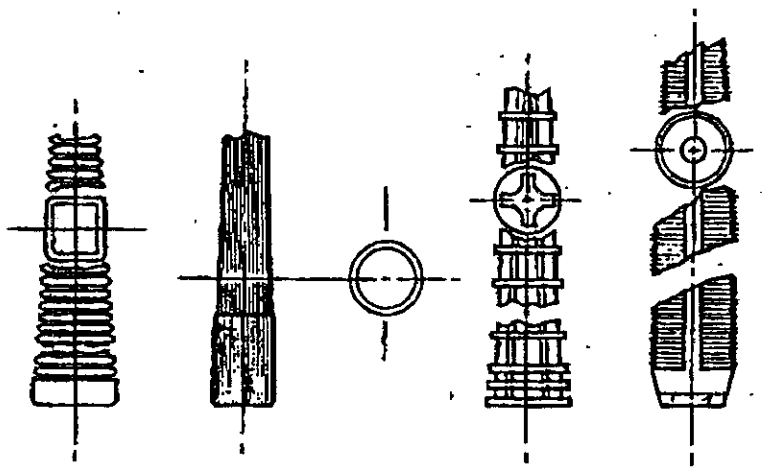

ALTERNATE HANDLES

NOTE:
AS AN ALTERNATE, HANDLES MAY BE TAPERED.

FIGURE 1 RAZOR AND BLADE ASSEMBLY

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:36Z
Check the source to verify that this is the current version before use.