MILITARY SPECIFICATION

MATTRESS, PNEUMATIC, FIELD HOSPITAL FOLDING COT

1. SCOPE

1.1 This specification covers one type of pneumatic mattress, suitable for use with cots in field hospitals.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

CCC-T-191	Textile Test Methods.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-Up, Paperboard.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper, Water-Resistant (for Carton Sealing).

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.
MS16686	Medical Services Symbol.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

FSC 7210

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Material.

3.1.1 Basic fabric. The basic fabric shall be 36-inch 4.0 cotton sheeting which shall be constructed and processed to have the following minimum characteristics:

Yarn count	Warp 56 Filling 53
Breaking strength	Warp 50 pounds Filling 45 pounds
Weight per square yard	3.5 ounces
Color	Olive drab or khaki

3.1.1.1 Coating. The basic fabric shall be rubber coated, as follows:

2 spreader coats	Total weight 3/4 ounce per square yard
2 calendered coats	Total weight 13-1/2 ounces per square yard

The total weight of the finished fabric shall be 18 ounces per square yard. Reclaimed rubber shall not be used.

3.1.2 Cement. The compound shall be a synthetic or natural rubber cement, completely compatible with the coating on the fabric. Conformance of the cement shall be based on the successful performance of the mattress and its component beams and seams, when subjected to the inflation test specified in 4.4.1.

3.2 Construction. The mattress shall be constructed with one-piece top and bottom panels of coated fabric. The two pieces shall be joined around the edges, and reinforced along this seam by means of an additional strip of fabric. The mattress shall be reinforced in the longitudinal direction by not less than four I-beams. A screw-type inflation valve (see 6.1) shall be fitted into one corner of the assembled mattress. All seams shall be cemented and vulcanized. Construction shall conform to figure 1. Dimensions shown are of the inflated mattress. Tolerance on overall dimensions shall be ± 1/2 inch.

3.3 Identification marking. Each mattress shall be marked on the underside with the manufacturer's name or registered trademark, the contract or purchase order number, and the medical services symbol conforming to type I of Standard MS16686. The letters "U" and "S" shall be 1 inch high, and the caduceus of appropriate size. Markings shall be stenciled or printed with black waterproof stencil paint or black waterproof ink, and shall be in a conspicuous location. All markings shall be distinct, legible, and of a permanent nature.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.


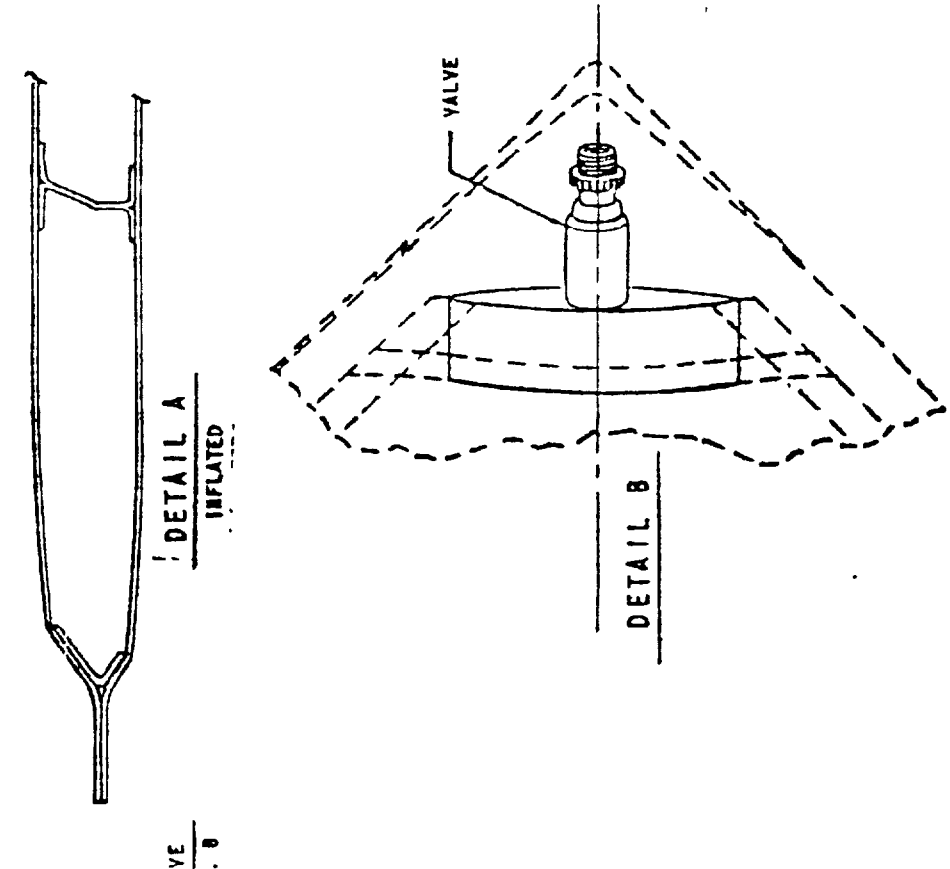


FIGURE 1

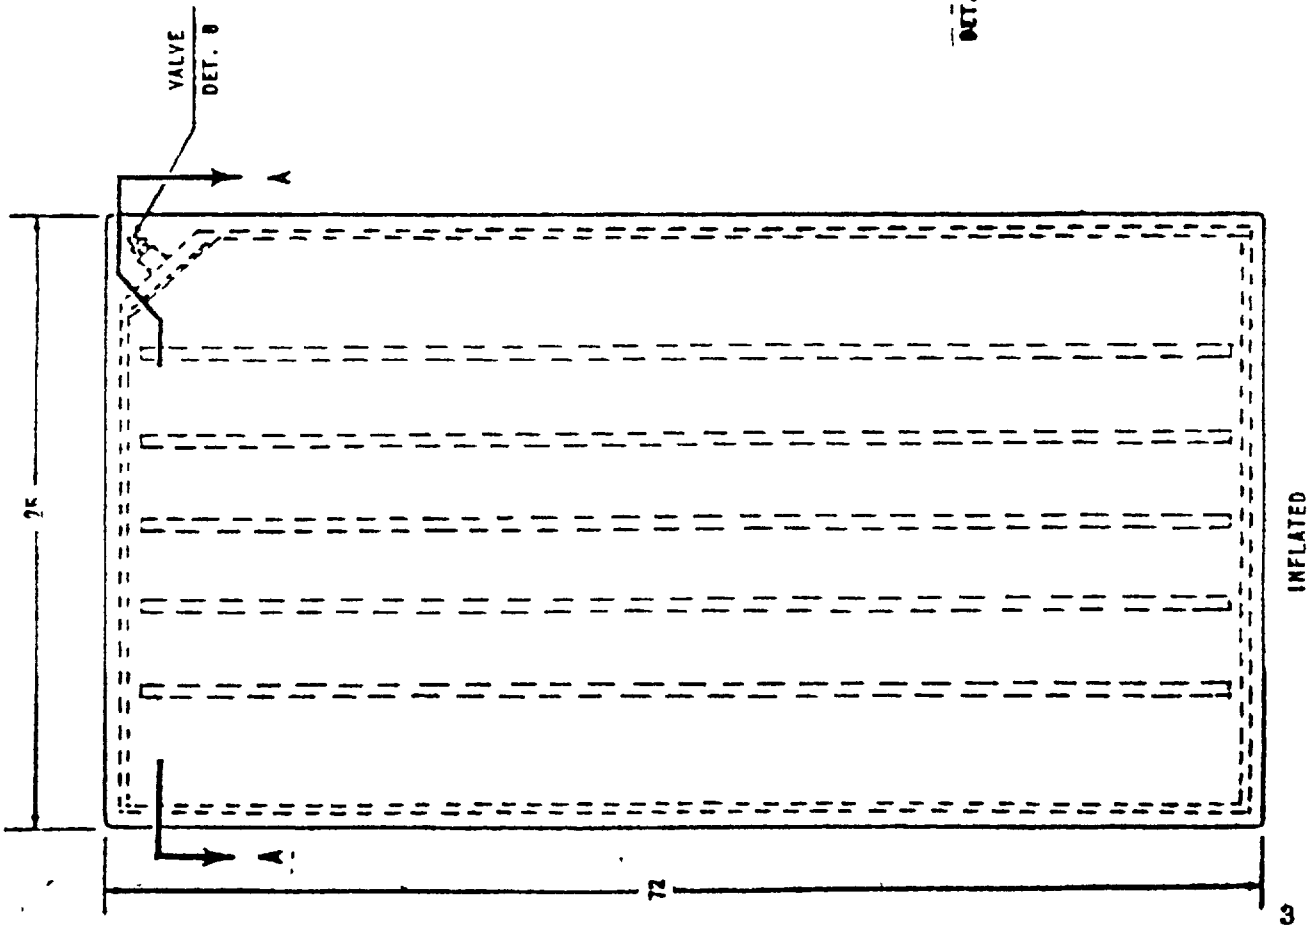

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

3.4 Workmanship. Workmanship shall be first class throughout. Mattresses shall be free from defects which detract from their appearance or may impair their serviceability. The mattress shall conform to the quality and grade of product established by this specification. The occurrence of defects shall not exceed the applicable quality levels. A fully adhered single patch, not less than 1 inch nor more than 2 inches in any linear dimension, may be used on each mattress to repair coating.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.2 Preacceptance inspection.

4.2.1 Preproduction inspection. When required, inspection and testing of the preproduction sample shall be made of a completely fabricated mattress for all provisions of this specification applicable to end product examination and tests.

4.3 Inspection for acceptance. Unless otherwise indicated, inspection shall be conducted in accordance with Standard MIL-STD-105.

4.3.1 Inspection of components.

4.3.1.1 Component testing. Testing shall be performed on components and materials listed in table I for the test characteristics shown.

4.3.2 Certification of compliance. Components and materials listed below may be accepted on the basis of a contractor's certification of compliance for the characteristics indicated.

Component	Characteristics	Requirement
Base fabric	Cotton sheeting shall be 3.5 ounces/ square yard prior to dyeing.	3.1.1
Coated fabric	Fabric coated with 2 spreader coats (total weight of 3/4 ounce/square yard) and 2 calendered coats (total weight of 13-1/2 ounces/square yard).	3.1.1.1
Cement	Compound used for cementing shall be synthetic or natural rubber cement, completely compatible with the coating on the fabric.	3.1.2

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

TABLE I

COMPONENT	LOT EXPRESSED IN TERMS OF	CHARACTERISTIC	REQMT	TEST METHOD (CCC-T-191)	REQUIREMENTS APPLY TO SPL UNIT	REQUIREMENTS APPLY TO LOT AVG	# DET PER SPL UNIT	S.Q.	RESULTS REPORTED AS	INSP LV	AQL
Base fabric prior to coating	1 yard	Yarn count Warp	3.1.1	5050	X		5	½ yard	Avg of 5 det to nearest unit	S-1	6.5
		Yarn count Filling			X		5				
		Breaking Strength Warp		5100	X		5		Avg of 5 det to nearest 1 lb	S-1	6.5
		Breaking Strength Filling			X		5				
		Weight		5041	X		3		Avg of 3 det to nearest 0.1 ounce/sq. yd.	S-1	6.5
		Color		Visual		X	1		Pass or Fail	S-1	
Coated fabric	1 yard	Weight	3.1.1.1	5041	X		3	½ yard	Avg of 3 det to nearest 0.1 oz/sq. yd	S-1	6.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

4.3.3 In-process inspection. Inspection shall be made at any point or during any phase of the manufacturing process to determine whether operation or assemblies are accomplished as specified. The Government reserves the right to exclude from consideration for acceptance any material for which in-process inspection has indicated nonconformance. In-process inspection shall be conducted to see that accomplishment of the following is in accordance with the specification requirements:

Requirement, operation, or assembly	Requirement
Hinge material properly cemented around entire inside perimeter of the matress (when required).	3.2
That 70-inch-long stays are used to reinforce the seams between air chambers.	

4.3.4 End item examination. The defects found during examination shall be classified in accordance with 4.3.4.1, 4.3 4.2, and 4.3.4.3. The lots shall be inspected in accordance with 4.3.4.4. The sample unit for these examinations shall be one completely fabricated pneumatic mattress.

4.3.4.1 Examination for visual charecteristics. Examination of the mattress for defects in material, design, construction, workmanship, and marking:

EXAMINE	DEFECT	MAJOR	MINOR
Quality of coated fabric:	Not fabricated from specified material	X	
Material	Hole, cut, tear, or weak place	X	
Finish	Any visible deterioration	X	
	Shade variations between panels affecting appearance		X
	Fabric not soft and pliable		X
	Color and shade not as required		X
Odor	Rancid or objectionable	X	
Spots or stains	Fabric dirty or greasy to an extent that it cannot be completely removed with a damp cloth	X	
	Clearly noticeable when viewed at a distance of 6 feet		X
Design and construction	Mattress not vulcanized all in one piece	X	
	Top or bottom not one piece	X	
	Any component missing	X	

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

4.3.4.1 Examination for visual characteristics (continued)

EXAMINE	DEFECT	MAJOR	MINOR
Fin edge	Missing	X	
	Not cemented or molded along entire perimeter of mattress	X	
	Any open or unfilled channel in fin edge	X	
	Uneven trim (with some areas under minus tolerance)	X	
	Uneven trim (with some areas over plus tolerance)		X
Seams	Missing, loose, or broken	X	
	Misplaced, seriously affecting serviceability or appearance	X	
	Misplaced, not seriously affecting serviceability or appearance		X
	Not pressure vulcanized along entire length	X	
Valve	Not specified type	X	
	Not located as required: Seriously affecting serviceability	X	
	Not seriously affecting serviceability		X
	Valve not air-tight sealed	X	
	Valve stopper does not function properly	X	
Workmanship	Any adhesion between top and bottom panels (except where required)	X	
	Any sharp crease or wrinkle affecting appearance		X
Marking	Missing, incorrect, illegible		X
	Not accomplished in specified manner		X
	Not in conspicuous location		X

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

4.3.4.2 Examination of inflated mattress for dimensions. Any dimension that is not within the specified tolerances shall be classified as a defect.

4.3.4.3 Examination for inflation characteristics. Examination of the mattress for defects in the inflated condition:

EXAMINE	DEFECT
Inflated mattress	Evidence of leakage (not air-tight)
	Not easily inflatable by mouth or pump
	Blocking resulting in closure and lack of inflation of any chamber

4.3.4.4 AQL's and inspection levels. The inspection levels and acceptable quality levels (AQL's) expressed in defects per hundred units shall be as follows:

	Inspection level	AQL's Major	AQL's Total
For defects applicable to 4.3.4.1	I	2.5	6.5
For defects applicable to 4.3.4.2	S-5	One class	4.0
For defects applicable to 4.3.4.3	S-5	One class	4.0

4.3.5 Examination of preparation for delivery requirements. An examination shall be made to determine that applicable packaging, packing, and marking requirements are complied with. Defects shall be scored in accordance with the list below. The sample unit shall be one exterior container fully prepared for delivery with the exception that it need not be sealed. Defects of closure listed below shall be examined on exterior containers fully prepared for delivery. The lot size shall be the number of exterior containers in the end item inspection lot. The inspection level shall be S-2 and the AQL shall be 4.0 defects per hundred units.

Examine	Defect
Marking (exterior and interior)	Omitted, incorrect, illegible, of improper size, location, sequence, or method of application
Materials	Any component missing
	Any component damaged, affecting serviceability
Workmanship (exterior and interior)	Inadequate application of components, such as incomplete closure of container flaps, inadequate stapling
	Cover not zippered closed, not packed flat with every other one reversed.
	Bulging or distortion of containers
Weight or content (exterior and interior)	Number of end items is more or less than required; gross/net weight exceeds requirements

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specified construction requirements.

4.4.1 Inflation. The finished mattress shall be inflated to form a firm mattress. After tightening the valve, the fully inflated mattress shall remain firm for 24 hours. The inflated mattress shall be observed to determine that there is complete adhesion of the cemented beams and seams.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One (1) mattress, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table II shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table II. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	12 units

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Unit package shall be a carton of appropriate size constructed in accordance with Specification PPP-B-566 or PPP-B-676, except that commercial colors shall be acceptable. Closure shall be adequate to prevent spillage of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with Specification PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type I, class 2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to Specification MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix of Specification PPP-B-636. In addition, all seams, including manufacturer's joint, shall be closed by tape conforming to the requirements of Specification PPP-T-76. The tape shall be not less than 2 inches wide. Three strips shall be applied to both top and bottom so that all seams and joints shall be covered their full length. Tape applied over the lengthwise seams shall extend a minimum of 2 inches onto each of the end panels. Tape applied over the end edge seams shall extend a minimum of 2 inches along the side and top, and side and bottom panels.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to Specification PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with Specification PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type I, class 1.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package shall be marked in accordance with Standard MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

5.3.2 Exterior container. Exterior container shall be marked in accordance with Standard MIL-STD-129. In addition, the letter "L" shall precede the Federal stock number. One space shall be allowed between the letter "L" and the first digit of the stock number. The terms "Stock number" or "FSN" shall not be indicated.

6. NOTES

6.1 The valves referred to in 3.2 are available as

Halkey-Roberts No. 260-AS, or
Parker and Harper No. 610, or
Dill No. 8630A, or
Schrader No. 9933

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.

Custodians:
Army. - MD
Navy. - BuMed
Air Force. - AFMSC

Preparing activity:
Defense Supply Agency. - DM

Review activities:
Army. - MD
Navy. - BuMed
Air Force. - AFMSG
Defense Supply Agency. - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

FORM APPROVED BUDGET BUREAU NO. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use of the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner and send to preparing activity.

SPECIFICATION: MIL-M-36226(DM) MATTRESS, PNEUMATIC, FIELD HOSPITAL FOLDING COT

ORGANIZATION	CITY AND STATE

CONTRACT NO.	QUANTITY OF ITEMS PROCURED	DOLLAR AMOUNT
		$

MATERIAL PROCURED UNDER A ☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

   A. GIVE PARAGRAPH NUMBER AND WORDING

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

   ☐ YES ☐ NO IF "YES" IN WHAT WAY?

4. REMARKS (ATTACH ANY PERTINENT DATA WHICH MAY BE OF USE IN IMPROVING THIS SPECIFICATION. IF THERE ARE ADDITIONAL PAPERS, ATTACH TO FORM AND PLACE BOTH IN AN ENVELOPE ADDRESSED TO PREPARING ACTIVITY)

SUBMITTED BY (PRINTED OR TYPED NAME AND ACTIVITY)	DATE

DD FORM 1426

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE SUPPLY AGENCY
DEFENSE MEDICAL SUPPLY CENTER
3RD AVENUE AND 29TH STREET
BROOKLYN N Y 11232

OFFICIAL BUSINESS

POSTAGE FEES PAID
DEFENSE SUPPLY AGENCY

Defense Supply Agency
Defense Medical Supply Center
ATTN Directorate of Technical Operations (Code T-K2)
3rd Avenue and 29th Street
Brooklyn N Y , 11232

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:14Z
Check the source to verify that this is the current version before use.