MIL-N-36149A
13 March 1968
SUPERSEDING
MIL-N-36149
24 April 1963

MILITARY SPECIFICATION

NEEDLES, HYPODERMIC, TONSIL

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers tonsil anesthesia hypodermic needles.

1.2 Classification. Needles shall be of the following styles, as specified (see 6.1):

Style A - Straight (23 gage, 3/4 inch)

Style B - Curved (23 gage, 1/2 inch).

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-up, Paperboard.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.
MIL-P-116	Preservation, Methods of.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:08Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

UNITED STATES OF AMERICA (USA) STANDARDS INSTITUTE

USA Z70.1-1955 American Standard Dimensions of Glass and Metal. Luer Tapers for Medical Applications.

(Application for copies should be addressed to the United States of America Standards Institute 10 East 40th Street, New York, New York 10016).

3. REQUIREMENTS

3.1 Material.

3.1.1 Cannula. The cannula shall be fabricated from either seamless drawn, or welded and drawn tubing. Material shall be class 3, type 304 in accordance with GG-I-526.

3.1.2 Hub and extension tube. The hub and the extension tube shall be fabricated from brass, nickel plated, or chromium over nickel plated in accordance with plating requirements for class 8 material of GG-I-526. The corrosion tests shall be the salt-spray and boil tests. As an alternate, the extension tube shall be fabricated from class 3, type 304 material in accordance with GG-I-526.

3.1.3 Cleaning wire. The cleaning wire shall be fabricated from class 3, type 304 material in accordance with GG-I-526.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:08Z
Check the source to verify that this is the current version before use.

3.2 Construction. The style A and style B needles shall be in accordance with figure 1. Style A needle shall be straight and shall have a 23 gage cannula with 3/4 inch of the distal end of the cannula exposed as shown on the figure. Style B needle shall be curved and shall have a 23 gage cannula, with 1/2 inch of the distal end of the cannula exposed as shown on the figure.

3.2.1 Cannula and extension tube. The cannula and the extension tube shall project into the hub sufficiently to allow for secure swaging. In accordance with standard practice, the projection of the needle cannula into the hub shall not be such as to prevent the cleaning wire from being readily inserted into the lumen of the cannula or to create areas for possible accumulation of materials. The cannula and the extension tube shall be securely swaged into the hub so as to be concentric with the hub cavity. The straight portions of the cannula and the extension tube shall not deviate from the central longitudinal axis of the needle by more than 3 degrees. The point of the cannula shall be ground concave or flat and may have a center ridge at the distal end to strengthen the tip. The point shall be so ground at the outer end as to enhance the keenness of the tip and cutting edges. Both outer and inner edges of point shall be free from burs and slivers. The tip of the point shall be straight and strong, and of maximum keenness.

3.2.2 Hub. The hub, its cavity and its flange shall be constructed in accordance with the requirements of the USA Standard Z70.1-1955 for female Luer-lock connections. The hub shall be so shaped that it will not roll and will provide a satisfactory finger grip for attaching the needle to a syringe. The entire hub cavity wall, down to the entrance of the lumen of the needle cannula, shall be well plated.

3.2.2.1 Diameter and depth of Luer hub cavity. The hub shall be tested for diameter and depth of the Luer hub cavity as specified in 4.4.1. Hubs which do not fit the plug gage within the "GO" - "NO GO" limits specified in 4.4.1, shall be considered not acceptable. In addition, when the hub is fitted onto the plug gage as specified in 4.4.1, there shall be no movement of the hub on the gage when the cannula is pressed lightly from side to side in all directions.

3.2.2.2 Fluid tightness. The connection of the needle cannula with the hub and the connection of the hub with the test gage shall not show leakage exceeding the formation of a falling drop when the needle is tested as specified in 4.4.2.

3.2.3 Cleaning wire. The cleaning wire shall be as large as practicable for the diameter of the lumen of the needle cannula and not less than 1/2 inch longer than the overall length of the needle. The wire shall be reasonably straight and shall be free from rough ends or other defects which may prevent the wires from being readily inserted into the lumen of the needle cannula. The wire shall be furnished in the needle.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:08Z
Check the source to verify that this is the current version before use.

3.3 Security of assembly. When tested as specified in 4.4.3, the cannula shall not loosen or pull out of the hub.

3.4 Freedom from foreign matter. When tested as specified in 4.4.4, the hub cavity shall be substantially free from chips and other foreign matter. In addition, a visual examination of the lumen of the cannula shall reveal no presence of foreign matter, chips, burs, or occlusion of the lumen.

3.5 Identification marking. The hub shall be permanently stamped with the gage of the needle cannula and the manufacturer's name or registered trademark as shown on the figure.

3.6 Workmanship. Workmanship shall be first class throughout. Needles shall be free from defects which detract from their appearance or may impair their serviceability. The cannula and extension tube shall show a smooth finished outer surface free from pits and tool marks, and inner surface of the cannula shall be free from scale, deep pits, deep furrows, or die marks. The lumen of the cannula and the hub cavity shall be free from chips, dirt, or other foreign matter. Needles shall be sharp, not blunt or bent, and points shall be free of feathered edges, or other defects, when examined under 7 power magnification.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:08Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in table I.

Table I. Sampling criteria for examination

Type defect	Inspection level	AQL (percent defective)
Major A	S-4	1.0
Major B	S-1	1.0
Minor A	S-4	6.5
Minor B	S-1	4.0

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table II.

Table II. Sampling criteria for tests

Component	Characteristic	Reqmt.	Test Procedure	Unit of Product	Inspection Level	AQL
Cannula and Cleaning wire	Boil Test	GG-I-526	GG-I-526	1-needle	S-1	*
Hub and Extension Tube	Boil Test (for all Material)	3.1.2	GG-I-526	1-needle	S-1	*
	Salt Spray (For Class 8 material)	3.1.2	GG-I-526	1-needle	S-1	*
	Plating Test (For Class 8 material)	3.1.2	GG-I-526	1-needle	S-1	*
Hub	Diameter and Depth of Luer Hub Cavity	3.2.2.1	4.4.1	1-needle	S-1	*
Needle Assembly	Dimensions	3.2	---	1-needle	S-1	*
	Fluid Tightness	3.2.2.2	4.4.2	1-needle	S-1	*
	Security of Assembly	3.3	4.4.3	1-needle	S-1	*
	Freedom from Foreign Matter	3.4	4.4.4	1-needle	S-1	*

*Acceptance number shall be zero for all sample sizes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:08Z
Check the source to verify that this is the current version before use.

4.2.3 Raw materials. Sufficient quantity of each lot of each metal used in the construction of the needles shall be selected for chemical analysis.

4.2.4 Sample unit usage. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination. The needles shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in tables I and III. Examination, however, shall not be restricted to defects listed in table III. Any needles in the sample containing one or more defects shall be rejected and, if the number of defective needles in any sample exceeds the acceptance number for that sample, the lot represented by the sample shall be rejected.

Table III. Classification of Defects in accordance with MIL-STD-105

Categories	Defects
Critical:	None defined
Major A	
101	Exposed surface of cannula, and extension tube not smoothly finished, or free of cracks, pits, tool marks, burs, scale or corrosion.
102	Cannula inner passage not free of deep pits, deep furrows, or die marks.
103	Cannula outside diameter not as specified.
104	Point missing.
105	Point blunt or bent, not sharp, not symmetric or properly formed, or not free of burs, feathered edges, or other detrimental defects (examined under 7X magnification).
106	Hub not smoothly finished, free of cracks, pits, tool marks, burs, or scale.
107	Hub not properly and completely plated (particularly cavity) as specified.
108	Diameter and depth of hub cavity not in accordance with USA Standard as specified.
109	Cannula projects into the hub, preventing cleaning wire from being readily inserted.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:08Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects in accordance with MIL-STD-105

Categories	Defects
Major B	
151	Cannula inside diameter not as specified.
152	Point length not as specified.
Minor A	
201	Discoloration of outside surface of hub, extension tube, or cannula.
202	Dimensions (other than cannula O.D., I.D., and point length) not as specified.
203	Cannula and extension tube not concentric, not straight, deviates from central longitudinal axis of needle by more than 3 degrees.
204	Cleaning wire missing or not correct length.
205	Needle size or contractors identification missing, incorrect or not legible.
Minor B (Unit of product - Unit package and contents)	
251	Average count per unit package not a minimum of 12 needles.
252	Marking missing, incorrect, or not legible.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 Diameter and depth of hub cavity. Hub cavity shall be tested on the male Luer taper gage in accordance with plug gage of figure 5 of USA Standard Z70.1-1955. (This gage shall be as shown in the USA Standard, except that it shall be constructed with a suitable fluid path to permit performance of the fluid tightness test specified in 4.4.2). The hub shall be slipped onto this gage with very light pressure. The fit of the hub on this gage shall be tested by means of the feeler gage in accordance with figures 5 and 6 of USA Standard Z70.1-1955.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:08Z
Check the source to verify that this is the current version before use.

4.4.2 Fluid tightness test. With the needle in a horizontal position, the hub shall be attached by means of a plug gage as shown in figure 5 of USA Standard Z70.1-1955 (except that gage shall have been provided with a fluid path) to a water pressure source having a pressure gage. The water shall be permitted to run through the needle so as to fill any hub cavity space and the lumen of the cannula. The lumen shall then be sealed by a piece of solid rubber pressed on to the point. A pressure of 45 pounds per square inch gage (p.s.i.g.) shall be applied for 10 seconds.

4.4.3 Security of assembly. A straight pull of 8-pounds shall be applied between the cannula and hub for a period of 1 minute (weight suspended from the cannula).

4.4.4 Freedom from foreign matter. The hub cavity shall be examined under 7X magnification, and good illumination, for chips and other foreign matter. In addition, a cotton swab tightly wrapped on the end of a small wooden applicator shall be vigorously turned down into the bottom of cavity, withdrawn, and examined for chips and other foreign matter under 7X magnification and good illumination. The cannula shall be tested for blockage by inserting a wire through the lumen of the cannula.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. Each needle, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	576 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:08Z
Check the source to verify that this is the current version before use.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive materials.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method 1A-15.

5.1.3.5 Intermediate package. Intermediate package shall be a carton of appropriate size constructed in accordance with Federal Specification PPP-B-566 or PPP-B-676 except that commercial colors shall be acceptable. Closure shall be adequate to prevent spillage of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type I, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4, of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:08Z
Check the source to verify that this is the current version before use.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic and method I closure shall be utilized.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Style required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.

Custodians:

Army - MD
Navy - MS
Air Force - 03

Review activities:

Army - MD
Navy - MS
Air Force - 03

Preparing activity:

Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:08Z
Check the source to verify that this is the current version before use.

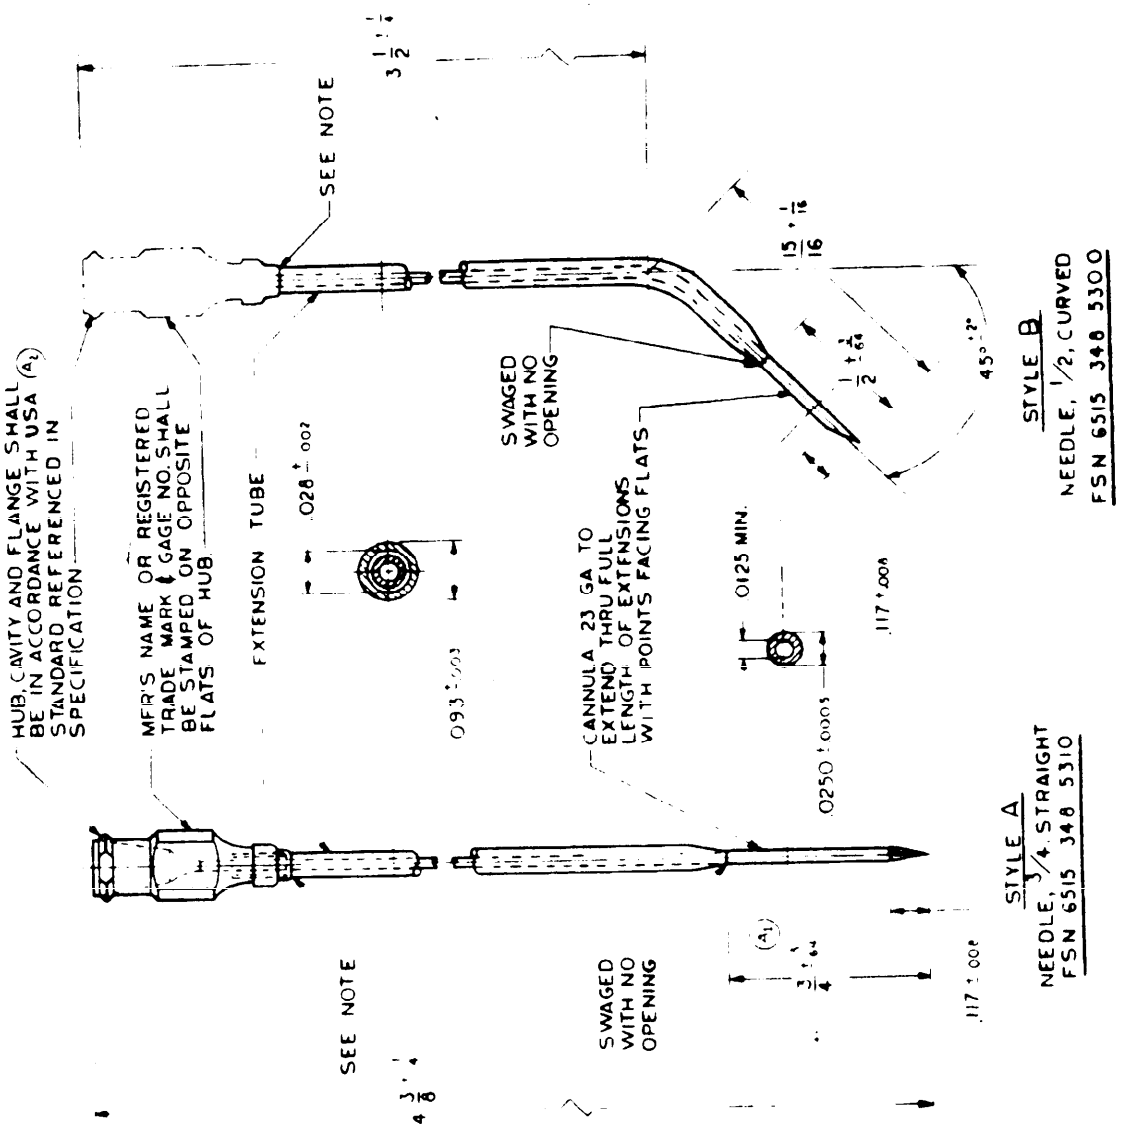


FIG. 1

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:08Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:08Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel using Government or contractor, involved in the use of this specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION: MIL-N-36149A

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)* | DATE

DD FORM 1 JAN 83 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:08Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM. SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL CODE ATS
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2413
AUG 68

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:08Z
Check the source to verify that this is the current version before use.