MIL-G-37300
13 January 1976

MILITARY SPECIFICATION

GOWN, PATIENT EXAMINING, DISPOSABLE

This specification is approved for use by all Departments and Agencies of the Department of Defense

1. SCOPE

1.1 Scope. This specification covers the requirements for one type and size of a disposable, patient examining gown.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

UU-P-268	Paper, Kraft, Untreated, Wrapping
PPP-B-636	Boxes, Shipping, Fiberboard
PPP-T-76	Tape, Pressure-sensitive Adhesive Paper, Water Resistant (For Carton Sealing)

Military

MIL-F-36911	Fabric, Nonwoven, Bedsheets and Gowns Disposable

FSC 6532

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-TEST METHOD STD NO. 191	Textile Test Methods

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Materials and components. The materials and components shall conform to the applicable specifications and standards listed or required herein.

3.1.1 Gown and belt fabric. The gown and belt shall be fabricated from the disposable fabric conforming to MIL-F-36911, blue, blue-green, blue-gray, aqua, misty green or white in color.

3.1.2 Adhesive. The seams of the gown shall be glued together with a suitable hot melted plastic or polyvinyl acetate adhesive. The adhesive shall be neutral, colorless or tan in color.

3.2 Design. The gown shall be knee length, sleeveless, collarless, overlapping back closure with a separate wraparound tie belt. The gown shall conform in appearance to Figure 1.

3.3 Construction. The gown shall be fabricated from one or three pieces of the fabric, 3.1.1. The gown shall consist of a front panel and right and left back panels. The seams of the gown shall be glued together with the adhesive, 3.1.2, as specified in Figure 1. The width of the glued area shall be a maximum of 1/2 inch. The glued portions shall not contain any trapped air, channels, wrinkles or skipped glued areas. The seams shall be glued together without tension. The adhesive when dry or cured shall present a neat and uniform appearance. The adhesive shall not be allowed to remain in clots nor permitted to extend in such a manner as to result in localized stiffness which might result

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

in discomfort to the wearer when the gown is donned, worn or removed. The adhesive upon drying or curing shall not cause the fabric to shrink or pucker at any point. The adhesive shall be applied in a straight line parallel to the edge of the gown. The gowns shall be free from any congealed mass of the adhesive and any spot or stain resulting from excess adhesive. The adhesive shall not bleed or strike through the fabric. No unrelated surfaces of the gowns shall be glued together. The gluing of the seams of the gown shall be undertaken utilizing the technique and precautions outlined so that, prior to the inspection of the assembled gown, the adhesive shall have developed its optimum bonding properties and the adherence of the seams shall comply with the requirements of this specification. Each gown shall contain two armholes and a neck opening conforming to Figure 1.

3.4 Dimensions. The gowns after assembly shall conform to the dimensions specified in Figure 1 when measured as specified in 4.3.3.

3.5 Performance inspection.

3.5.1 Seam strength. The seam strength of the glued seams when inspected as specified in 4.3.4, shall be not less than the cross direction breaking strength of the fabric.

3.6 Workmanship. The gowns shall not contain any tear, cut, mend, patch, spot, stain, hole, abraded area, or any other defect which may detract from their appearance or may impair their serviceability. The gowns shall conform to the quality of grade established by this specification. The occurrence of defects shall not exceed the acceptance criteria.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Material and component inspection. In accordance with 4.1, the materials and components shall be inspected and tested in accordance with all the requirements of the referenced specifications and standards, unless otherwise excluded, amended, modified, or qualified in this specification or purchase document.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

4.1.2 Certificate of quality. When certificates of quality are submitted in accordance with Table I, they shall contain verifiable actual test and inspection data. The Government reserves the right to inspect and test the components to verify the validity of the certification.

4.1.3 Inspection. Inspection, as used in this specification is defined as both examination (an investigation without the use of special laboratory apparatus or procedures such as visual) and testing (a determination by technical means of physical and chemical properties) of the item.

4.2 Quality conformance inspection. The sampling and inspection shall conform to MIL-STD-105, except where otherwise indicated hereinafter. The quality conformance inspection shall consist of the tests and examinations specified in Table I.

4.2.1 Sampling.

4.2.1.1 Inspection lot.

4.2.1.1.1 Adhesive. An inspection lot size shall be expressed in units of one gallon of the adhesive and shall consist of all the adhesive received by the gown manufacturer at one time. The sample unit for inspection shall be one gallon.

4.2.1.1.2 Gown. An inspection lot size shall be expressed in units of one gown made essentially under the same conditions and from the same materials and components. The sample unit for inspection shall be one gown.

4.2.1.2 Sampling for tests and examinations of the adhesive. The sample size, acceptance and criteria, tests and examinations required for the adhesive and gowns, as applicable, shall be as specified in Table I.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

sample or powder equivalent to approximately 100 mg of aspirin and

TABLE I. SAMPLE SIZE, ACCEPTANCE CRITERIA, TESTS AND EXAMINATIONS OF THE ADHESIVE AND GOWNS

Item	Inspection	Paragraph		Sample Size	Acceptance Criteria
		Requirement	Method		
Adhesive 1/	Identification	3.1.2	4.3.1	2/	2/ 3/
Gowns	Visual Examination	3.2, 3.3 and 3.6	4.3.2.1	Inspection Level II	An acceptable quality level of 4.0 defects per 100 units for Major defects and 10.0 defects per 100 units for total (Major plus Minor) defects
	Dimensional Check	3.4	4.3.2.1	Inspection Level S-3	An acceptable quality level of 4.0 defects per 100 units

1/ The inspection of the adhesive shall be conducted either at the contractor's or subcontractor's plant.

2/ The sampling for the testing of the adhesive shall be in accordance with 4.2.1.1.1 and as follows:

Lot Size (Gallons)	Sample Size
800 or less	2
801 up to and including 22,000	3
22,001 and over	5

The lot shall be unacceptable if one or more sample units fail to meet the requirement specified in Table I.

3/ A certificate of quality may be submitted for the stated requirement (see 4.1.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

4.3 Inspection methods.

4.3.1 Adhesive. The adhesive shall be identified by any standard commercial method.

4.3.2 Visual examination.

4.3.2.1 Gown. Each gown selected in accordance with Table I as a sample unit from the lot shall be thoroughly checked dimensionally and examined visually to determine conformance to this specification. The classification of defects listed in MIL-F-36911 and the classification and list of defects, Tables II and III of this specification, as applicable, shall be used to classify and enumerate the defects found.

TABLE II CLASSIFICATION OF DEFECTS FOR THE VISUAL EXAMINATION OF THE ASSEMBLED GOWNS

DEFECT	MAJOR	MINOR
GLUING		
a. Width of the glued area:		
1. More than 1/2 inch but not more than one inch		X
2. More than one inch	X	
b. Open seam:		
1. Any single opening in a glued seam area one to 4 inches		X
2. Any single opening in a glued seam area more than 4 inches	X	
3. Three or more unglued areas in any glued seam	X	
c. Any adhering of unrelated surfaces	1/	
d. Any glued area that has more than 4 wrinkles per inch		X
e. More than 3 spots or stains on the interior or exterior of the gown greater than one inch in any straight line dimension		X
f. Seam adherence quality	2/	

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

TABLE II. (continued)

DEFECT	MAJOR	MINOR
COMPONENTS AND ASSEMBLY		
a. Any component not as specified or any defect of component or defect of assembly, not herein classified	1/	
b. Any component, component part, or required operation omitted, or any operation improperly performed, not herein classified	1/	

1/ The defect shall be classified and scored as a major defect, when it seriously affects the serviceability or appearance, otherwise it shall be classified and scored as a minor defect.

2/ The quality of the seam adherence shall be determined by gently pushing the round edge of a circular typewriter eraser against all the glued seams. The seam shall be considered defective and classified and scored as a major defect if there is any evidence of separation of the seam such as lifting of a few fibers. As an alternate, the seam strength inspection may be substituted for the visual examination for the seam adherence quality. Samples for the seam strength inspection shall be selected as follows:

Lot Size (Number of gowns)	Sample Size
800 or less	2
801 up to and including 22,000	3
22,001 and over	5

The lot shall be unacceptable if one or more of the sample units fail to meet the seam strength requirement.

TABLE III. LIST OF DEFECTS FOR THE DIMENSIONS OF THE ASSEMBLED GOWNS

ASSEMBLED MEASUREMENT	DEFECT
Measure the length, width, neck opening, arm openings, location of glue lines, belt length and location of belt.	Any measurement deviating from the measurements specified in Figure 1 and applicable tolerance shall be enumerated as a dimensional defect.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

4.3.2.2 Packaging inspection. An inspection shall be made to determine compliance with the packaging, packing and marking requirements of section 5. Defects shall be scored as specified in table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with AQL of 4.0 expressed in terms of percent defective.

TABLE IV. Examination of preparation for delivery

Examine	Defect
Contents	Not as specified.
Container	Not as specified.
Marking	Omitted; incorrect; illegible; improper location, sequence or method of application.
Material	Component missing or damaged.
Workmanship	Bulging or distoration of containers.

4.3.2.2.1 Examination of closure, waterproofing and banding of container. When the shipping container is required to comply with PPP-B-636, the examination for defects in closure, waterproofing or banding shall be in accordance with the appendix of the box specification.

4.3.3 Procedure for measuring. The gown to be measured shall be laid flat, without tension, on a smooth, flat surface so that any wrinkles or creases shall not affect the measurement. The measurements shall be made with the use of any suitable measuring device.

4.3.4 Seam strength. Five specimens, 4 ± 1/16 or 1 ± 1/16 inches wide, as applicable, and 6 ± 1/16 inches long, shall be cut across and perpendicular to the seam. The specimens shall be cut from different locations so as to be representative of the gluing. One free end of one specimen (end not glued) shall be placed in the upper jaw and the other free end in the lower jaw of a suitable inspection apparatus equipped with an autographic recording device (see FED-TEST METHOD STD NO. 191, Method 5100 or 5102, as applicable). The seam portion of the specimen shall be in the center between the two jaws. The jaws shall be separated until failure occurs, either breaking of the fabric or separation of the bond. In either case, the result obtained shall be not less

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

than that specified in 3.5.1 (the cross direction breaking strength of the fabric specified in MIL-F-36911). The highest value obtained shall be taken as the result for the seam strength for the individual inspected specimen. The rate of jaw separation under no load shall be 12 ± 1/2 inches per minute. The front clamp of each jaw shall be one by one or at least one by two inches, as applicable. The remaining four specimens shall be similarly treated and inspected. The results of the five inspected specimens shall not be averaged. Each individual specimen shall conform to seam strength requirement specified in 3.5.1 and MIL-F-36911 for the cross direction breaking strength. The seam strength shall be determined in the same manner as that used to determine the cross direction breaking strength of the fabric (see MIL-F-36911).

5. PACKAGING

5.1 Packaging requirements. Packaging requirements shall be level A or C, as specified (see 6.2).

5.1.1 Unit of issue. One package containing one-hundred gowns, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Unit preparation. Each gown shall be neatly folded and band wrapped ten (10) gowns per bundle. Belt shall be inserted in the fold of the gown.

5.1.3 Level C. Gowns shall be packaged to afford adequate protection against physical damage during shipment from the supply source to the first receiving activity. The supplier may use his standard practice when it meets this requirement.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.2).

5.2.1 Level A. One unit, ten bundles (100 gowns), shall be packed in a snug fitting box constructed in accordance with PPP-B-636, class weather-resistant. Each box shall have the contents completely covered on top and bottom with a sheet of 30 - pound minimum basis weight kraft paper conforming to grade B of UU-P-268. All metal fasteners on the interior of the box shall be covered with tape conforming to PPP-T-76, or equal, to prevent damage to the gowns. Closure, strapping and waterproofing shall be as specified in the appendix of box specification.

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:23Z
Check the source to verify that this is the current version before use.

5.2.2 Level B. One unit, ten bundles (100 gowns), shall be packed as specified in 5.2.1, except that the exterior container shall conform to PPP-B-636, class domestic. In addition, strapping and water-proofing shall not be required.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery called for in the contract or purchase order.

5.3 Marking. Each exterior container shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name and address of contractor shall be shown.

6. NOTES

6.1 Intended use. The disposable, patient examining gown covered by this specification is intended for individual use during an X-ray examination.

6.2 Ordering data. Procurement documents shall specify the following:

(a) Title, number and date of this specification.
(b) Quantity desired.
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 Catalog Information. This specification is intended to cover the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6532-00-421-7828	GOWN, PATIENT EXAMINING, Nonwoven Fabric, Large, Disposable, 100s


Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6532-1106
CS

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:23Z
Check the source to verify that this is the current version before use.

exceed the acceptance criteria established herein.

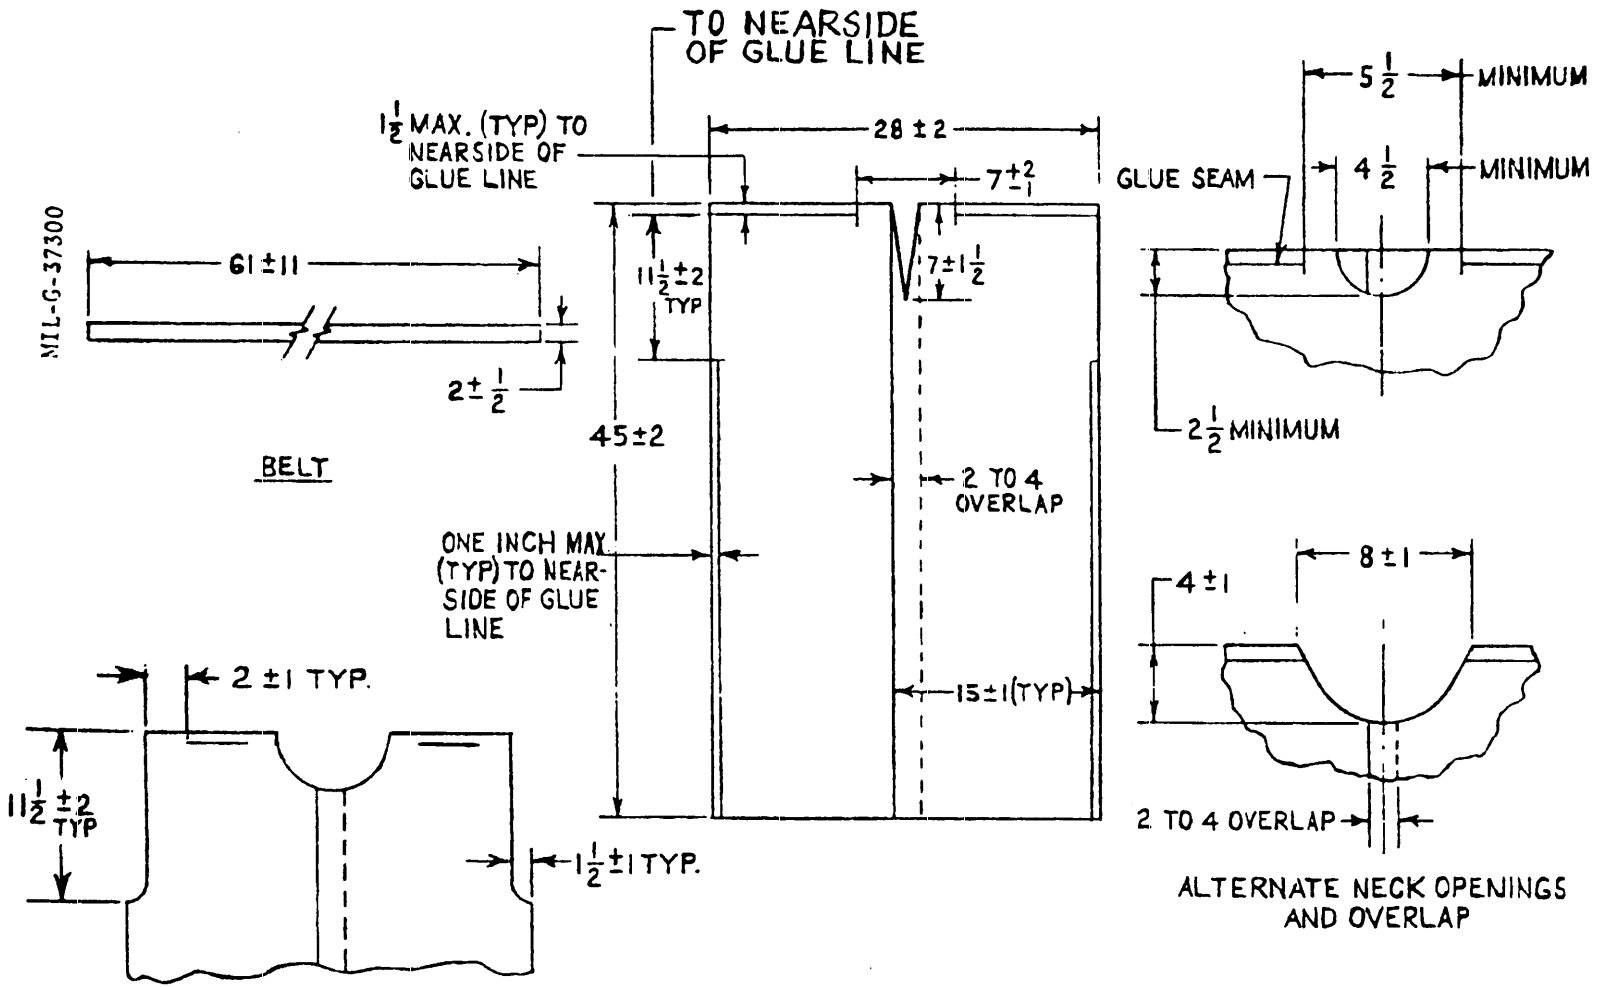

ALTERNATE NECK OPENINGS AND OVERLAP

ALTERNATE ONE PIECE CONSTRUCTION SHOWING SLEEVE INDENTATION, LENGTH OF SLEEVE OPENING AND DISTANCE OF SHOULDER SEAM FROM SIDE OF GOWN.

NOTE: DIMENSIONS IN INCHES

PATIENT EXAMINING GOWN
FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-G-37300 GOWN, PATIENT EXAMINING, DISPOSABLE

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:23Z
Check the source to verify that this is the current version before use.