MILITARY SPECIFICATION

GOWN, HOSPITAL, NONWOVEN FABRIC, DISPOSABLE, UNIVERSAL SIZE

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers the requirements for one type and color of a universal size, disposable, nonwoven fabric, hospital gown.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

FEDERAL

UU-P-268	Paper, Kraft, Untreated, Wrapping
PPP-B-636	Boxes, Shipping, Fiberboard

MILITARY

MIL-F-36911	Fabric, Nonwoven, Bedsheets and Gowns, Disposable

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

STANDARDS

FEDERAL

FED-TEST METHOD STD NO. 191	Textile Test Methods
FED-STD-751	Stitches, Seams and Stitching

MILITARY

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Materials and components. The materials and components shall conform to the applicable specifications and standards listed or required herein.

3.2 Design. The gown shall be knee length, long sleeves, collarless, overlapping back closure, waist attached tie kind of belt and closure at the neck area by means of tie tapes, adhesive tape, or hook and pile fastener tapes. The seams may be glued or sewn. The gown shall conform in appearance to Figures 1 through 4, as applicable.

3.3 Construction. The gowns shall be fabricated from the disposable fabric conforming to MIL-F-36911, yellow color.

3.3.1 Construction details.

3.3.1.1 Glued seams. The gown constructed with glued seams shall be fabricated from one or three pieces of the disposable fabric, 3.3. The gown shall consist of a front panel and right and left back panels. The seams of the gown shall be glued together with a suitable hot melted plastic or polyvinyl acetate adhesive, The adhesive shall be neutral, colorless or tan in color. The width of the glued area shall be a maximum of 1/2 inch. The glued portions shall not contain any trapped air, channels, wrinkles or skipped glued area. The seams shall be glued together without tension. The adhesive when dry

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:24Z
Check the source to verify that this is the current version before use.

or cured shall present a neat and uniform appearance. The adhesive shall not be allowed to remain in clots nor permitted to extend in such a manner as to result in localized stiffness which might result in discomfort to the wearer when the gown is donned, worn or removed. The adhesive upon drying or curing shall not cause the fabric to shrink or pucker at any point. The adhesive shall be applied in a straight line parallel to the edge of the gown. The gowns shall be free from any congealed mass of the adhesive and any spot or stain resulting from excess adhesive. The adhesive shall not bleed or strike through the fabric. No unrelated surfaces of the gown shall be glued together. The gluing of the seams of the gown shall be undertaken utilizing the technique and precautions outlined so that, prior to the inspection of the assembled gown, the adhesive shall have developed its optimum bonding properties and the adherence of the seams shall comply with the requirements of this specification. Each gown shall contain two sleeves, a belt and a neck opening conforming to Figures 1 and 2. The sleeves shall be inserted into the body so that the wide end shall be approximately flush with the edge of the gown. The sleeves and body shall then be glued together. The sleeves may be fabricated from one or two pieces of the fabric, 3.3. The belt, fabricated from the fabric, 3.3, may be attached as specified in Figure 1. As an alternate, the belt may be attached by two centered vertical glue lines approximately 4 inches apart from the farside to the farside of the glue lines. As another alternate, the belt may be attached by an area of approximately 5/8 inch of adhesive in the center of the belt. The seams at the shoulder may be formed by overlapping the back onto the front, vice versa, or folding the back and front together onto the front. The closure at the neck may be effected by the use of tie tapes, fabricated from the fabric, 3.3, hook and pile fastener tapes and the adhesive tape as specified in Figure 2. The inside of the neck area at the front may be reinforced. The assembled gown shall conform to Figures 1 and 2, as applicable.

3.3.1.2 Sewn seams. The gown fabricated with sewn seams shall be fabricated from one piece of the disposable fabric, 3.3 (without side seams). The gown shall consist of a front panel and right and left back panels. The seams shall be sewn together with a white (bleached) or natural (unbleached) thread suitable for the purpose intended. The number of stitches per inch shall be adequate for disposable kind of items. The seams shall be formed with sufficient stitches per inch and tension to maintain proper assembly of the gown without weakening the fabric. The sleeves shall be fabricated from one piece of the fabric, 3.3, with an underarm inseam. The sleeves shall be formed with Seam Type SSa-1 and overedge stitching

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

[UNITED STATES]

Stitch Type 500 class. The seam and stitch types shall conform to FED-STD-751. The sleeves may be raglan or set-in type. The wrist ends of the sleeves shall contain elastic binding to hold the sleeve end firmly around the wrist. The elastic binding shall be a strip of natural or synthetic rubber or covered natural or synthetic rubber (elastic braid), 1/8 to 3/16 inch wide, suitable for the purpose intended. As an alternate, the sleeves may terminate in knitted wristlets. The sleeves shall be attached with Seam Type SSa-1 and Stitch Type 500 class. The shoulders shall be joined together with Seam Type SSa-1, and Stitch Type 500 class. The belt and neck binding shall be fabricated from bleached or unbleached cotton tape or bias binding 3/4 ± 1/16 inch wide. Each side of the tape shall be folded under for approximately 3/16 inch resulting in approximately 3/8 inch wide binding and belt. The neck binding shall be attached with Seam Type BSc-1 and Stitch Type 301. The neck binding shall extend a minimum of 11 inches on each side. As an alternate, hook and pile fastener tapes of sufficient length and width may be substituted for the tie tapes. The belt shall be sewn together with Seam Type SSc-1 and Stitch Type 301. The belt shall be attached as specified in Figures 3 and 4. The assembled gown shall conform to Figures 3 and 4, as applicable.

3.4 Dimensions. The gowns after assembly shall conform to the dimensions specified in Figures 1 through 4, as applicable, when measured as specified in 4.3.3.

3.5 Performance inspection.

3.5.1 Seam strength. The seam strength of the glued seams, when inspected as specified in 4.3.4, shall be not less than the breaking strength of the fabric.

3.6 Workmanship. The gowns shall not contain any tear, cut, mend, patch, spot, stain, hole, needle chew, thread break, skipped stitch, abraded area, or any other defects which may detract from their appearance or may impair their serviceability. The gowns shall conform to the quality and grade of product established by this specification. The occurrence of defects shall not exceed the acceptance criteria established herein.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

4.1.1 Material and component inspection. In accordance with 4.1, the materials and components shall be inspected and tested in accordance with all the requirements of the referenced specifications and standards, unless otherwise excluded, amended, modified, or qualified in this specification or purchase document.

4.1.2 Certificate of quality. When certificates of quality are submitted in accordance with Table I, they shall contain verifiable actual test and inspection data. The Government reserves the right to inspect and test the components to verify the validity of the certification.

4.1.3 Inspection. Inspection, as used in this specification, is defined as both examination (an investigation without the use of special laboratory apparatus or procedures such as visual) and testing (a determination by technical means of physical and chemical properties) of the item.

4.2 Quality conformance inspection. The sampling and inspection shall conform to MIL-STD-105, except where otherwise indicated hereinafter. The quality conformance inspection shall consist of the tests and examinations specified in Table I.

4.2.1 Sampling.

4.2.1.1 Inspection lot.

4.2.1.1.1 Adhesive. An inspection lot size shall be expressed in units of one gallon of the adhesive and shall consist of all the adhesive received by the gown manufacturer at one time. The sample unit for inspection shall be one gallon.

4.2.1.1.2 Gown. An inspection lot size shall be expressed in units of one gown made essentially under the same conditions and from the same materials and components. The sample unit for inspection shall be one gown.

4.2.1.1.3 Preparation of delivery. An inspection lot size shall be expressed in units of one fully prepared shipping container, containing gowns, fully prepared for delivery from essentially the same materials and components. The sample unit for inspection shall be one shipping container, containing gowns, fully prepared for delivery with the exception that it need not be sealed.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

4.2.1.2 Sampling for tests and examination of the adhesive, gowns and preparation for delivery. The sample size, acceptance criteria, tests and examinations required for the adhesive, gowns or the preparation for delivery, as applicable, shall be as specified in Table I.

TABLE I. SAMPLE SIZE, ACCEPTANCE CRITERIA, TESTS AND EXAMINATIONS OF THE ADHESIVE, GOWNS AND PREPARATION FOR DELIVERY

Item	Inspection	Paragraph		Sample Size	Acceptance Criteria
		Requirement	Method		
Adhesive 1/	Identification	3.3.1.1	4.3.1	2/	2/ 3/
Gowns	Visual Examination	3.2 through 3.3.1.2, as applicable, and 3.6	4.3.2.1	Inspection Level II	An acceptable quality level of 4.0 defects per 100 units for Major defects and 10.0 defects per 100 units for total (Major plus Minor) defects
	Dimensional Check	3.4	4.3.2.1	Inspection Level S-3	An acceptable quality level of 4.0 defects per 100 units
	Preparation for Delivery	Section 5	4.3.2.2	Inspection Level S-2	An acceptable quality level of 2.5 defects per 100 units

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

1/ The inspection of the adhesive shall be conducted either at the contractor's or subcontractor's plant.

2/ The sampling for the testing of the adhesive shall be in accordance with 4.2.1.1.1 and as follows:

Lot Size (Gallons)	Sample Size
800 or less	2
801 up to and including 22,000	3
22,001 and over	5

The lot shall be unacceptable if one or more sample units fail to meet the requirement specified in Table I.

3/ A certificate of quality may be submitted for the stated requirement (see 4.1.2).

4.3 Inspection methods.

4.3.1 Adhesive. The adhesive shall be identified by any standard commercial method.

4.3.2 Visual examination.

4.3.2.1 Gown. Each gown selected in accordance with Table I as a sample unit from the lot shall be thoroughly checked dimensionally and examined visually to determine conformance to this specification. The classification of defects listed in MIL-F-36911 and the classification and list of defects, Tables II and III of this specification, as applicable, shall be used to classify and enumerate the defects found.

TABLE II. CLASSIFICATION OF DEFECTS FOR THE VISUAL EXAMINATION OF THE ASSEMBLED GOWNS

Defect	MAJOR	MINOR
GLUING		
a. Width of the glued area:		
1. More than 1/2 inch but not more than one inch		X
2. More than one inch	X	

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

TABLE II. CLASSIFICATION OF DEFECTS FOR THE VISUAL EXAMINATION OF THE ASSEMBLED GOWNS (Continued)

DEFECT	MAJOR	MINOR
GLUING		
b. Open seam:		
1. Any single opening in a glued seam area one to 4 inches		X
2. Any single opening in a glued seam area more than 4 inches	X	
3. Three or more unglued areas in any glued seam	X	
c. Any adhering of unrelated surfaces	1/	
d. Any glued area that has more than 4 wrinkles per inch		X
e. More than 3 glue spots or stains on the interior or exterior of the gown greater than one inch in any straight line dimension		X
f. Seam adherence quality	2/	
SEWING		
a. Any seam or attachment of any component twisted, puckered or pleated		X
b. Any part of the gown or of any component caught in an unrelated operation or stitching		X
c. Any needle chew	X	
d. Not specified seam or stitch	1/	

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:24Z
Check the source to verify that this is the current version before use.

TABLE II. CLASSIFICATION OF DEFECTS FOR THE VISUAL EXAMINATION OF THE ASSEMBLED GOWNS (Continued)

DEFECT	MAJOR	MINOR
COMPONENTS AND ASSEMBLY		
a. Any component not as specified or any defect of component or defect of assembly, not herein classified	1/	
b. Any component, component part, or required operation omitted, or any operation improperly performed, not herein classified	1/	

1/ The defect shall be classified and scored as a major defect, when it seriously affects the serviceability or appearance, otherwise it shall be classified and scored as a minor defect.

2/ The quality of the seam adherence shall be determined by gently pushing the round edge of a circular typewriter eraser against all the glue seams. The seam shall be considered defective and classified and scored as a major defect if there is any evidence of separation of the seam such as lifting of a few fibers. As an alternate, the seam strength inspection may be substituted for the visual examination for the seam adherence quality. Samples for the seam strength inspection shall be selected as follows:

Lot Size (Number of gowns)	Sample Size
800 or less	2
801 up to and including 22,000	3
22,001 and over	5

The lot shall be unacceptable if one or more of the sample units fail to meet the seam strength requirement.

TABLE III. LIST OF DEFECTS FOR THE DIMENSIONS OF THE ASSEMBLED GOWNS

ASSEMBLED MEASUREMENT	DEFECT
Measure the length, width, neck opening, arm openings, location of glue lines, belt length, location of belt.	Any measurement deviating from the measurements specified in Figures 1 through 4 and applicable tolerance, as applicable, shall be enumerated as a dimensional defect.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

4.3.2.2 Preparation for delivery. Each of the fully prepared shipping containers, containing gowns, selected in accordance with Table I as a sample unit from the lot, shall be visusally examined to determine that the packaging, packing, and marking conform to this specification. The list of defects, TAble IV, shall be used to enumerate the defects found.

TABLE IV. LIST OF DEFECTS FOR PREPARATION FOR DELIVERY

ITEM	DEFECT
Exterior markings	Missing, incorrect, incomplete, or illegible; improper size, location, sequence, or method of application not as specified.
Packaging and packing materials	Any non-conforming component; any component or component part missing, damaged, or otherwise defective.
Workmanship	Inadequate application of the components such as incomplete closure of any exterior container, container flap, or loose strapping; bulging or distortion of any container.
Exterior and interior weight or content	Gross or net weight exceeds the requirement; number per container more or less than specified.

4.3.3 Procedure for measuring. The gown to be measured shall be laid flat, without tension, on a smooth, flat surface so that any wrinkles or creases shall not affect the measurement. The measurements shall be made with the use of any suitable measuring device.

4.3.4 Seam strength. Five specimens, 4 ± 1/16 or 1 ± 1/16 inches wide, as applicable, and 6 ± 1/16 inches long, shall be cut across and perpendicular to the seam. The specimens shall be cut from different locations so as to be representative of the gluing. One free end of one specimen (end not glued) shall be placed in the upper jaw and the other free end in the lower jaw of a suitable inspection apparatus equipped with an autographic recording device (see FED-TEST METHOD STD NO. 191, Method 5100 or 5102, as applicable). The seam portion of the specimen shall be in the center between the two jaws. The jaws shall be separated until failure occurs, either breaking of

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

the fabric or separation of the bond. In either case, the result obtained shall be not less than that specified in 3.5.1 (the cross direction breaking strength of the fabric specified in MIL-F-36911). The highest value obtained shall be taken as the result for the seam strength for the individual inspected specimen. The rate of jaw separation under no load shall be 12 + 1/2 inches per minute. The front clamp of each jaw shall be one by one or at least one by two inches, as applicable. The remaining four specimens shall be similarly treated and inspected. The results of the five inspected specimens shall not be averaged. Each individual specimen shall conform to seam strength requirement specified in 3.5.1 and MIL-F-36911 for the cross direction breaking strength. The seam strength shall be determined in the same manner as that used to determine the cross direction breaking strength of the fabric (see MIL-F-36911).

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One package containing one hundred gowns constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Unit preparation. Each gown shall be neatly folded to approximate dimensions of 10 by 12 inches and band wrapped ten gowns per bundle.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. One hundred gowns (1 unit) shall be packed in a fiberboard box of appropriate size constructed in accordance with PPP-B-636, style RSC, grade V3c. Each container shall have the contents completely covered on top and bottom with a sheet of 30-pound minimum basis weight kraft paper conforming to grade B of UU-P-268. Each box shall be closed, waterproofed and strapped in accordance with the appendix of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 202640-21T10:24Z
Check the source to verify that this is the currentversion before use.

5.2.2 Level B.

5.2.2.1 Exterior container. One hundred gowns (1 unit) shall be packed in a fiberboard box of appropriate size constructed in accordance with PPP-B-636, style RSC, grade 275. Each box shall have the contents completely covered on top and bottom with a sheet of 30 pound minimum basis weight kraft paper conforming to grade B of UU-P-268. Each box shall be closed in accordance with method II, as specified in the appendix of the container specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Lot or control number shall be shown. The date of manufacture shall be shown in lieu of the date packed.

6. NOTES

6.1 Intended use. The universal size, disposable, nonwoven fabric, hospital gown covered by this specification is intended for individual use while in an isolation area.

6.2 Ordering data. Procurement documents shall specify the following:

(a) Title, number and date of this specification.
(b) Quantity desired.
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 Catalog Information. This specification is intended to cover the following item appearing in the Federal Supply Catalog:


National Stock No.	Item Identification
6532-00-104-9895	GOWN, HOSPITAL, Nonwoven Fabric, Universal Size, Disposable, 100s

Custodians
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM


Project No. 6532-1107
CS


Source: https://assist.dla.mil -- Downloaded: 202640-21T10:24Z
Check the source to verify that this is the currentversion before use.

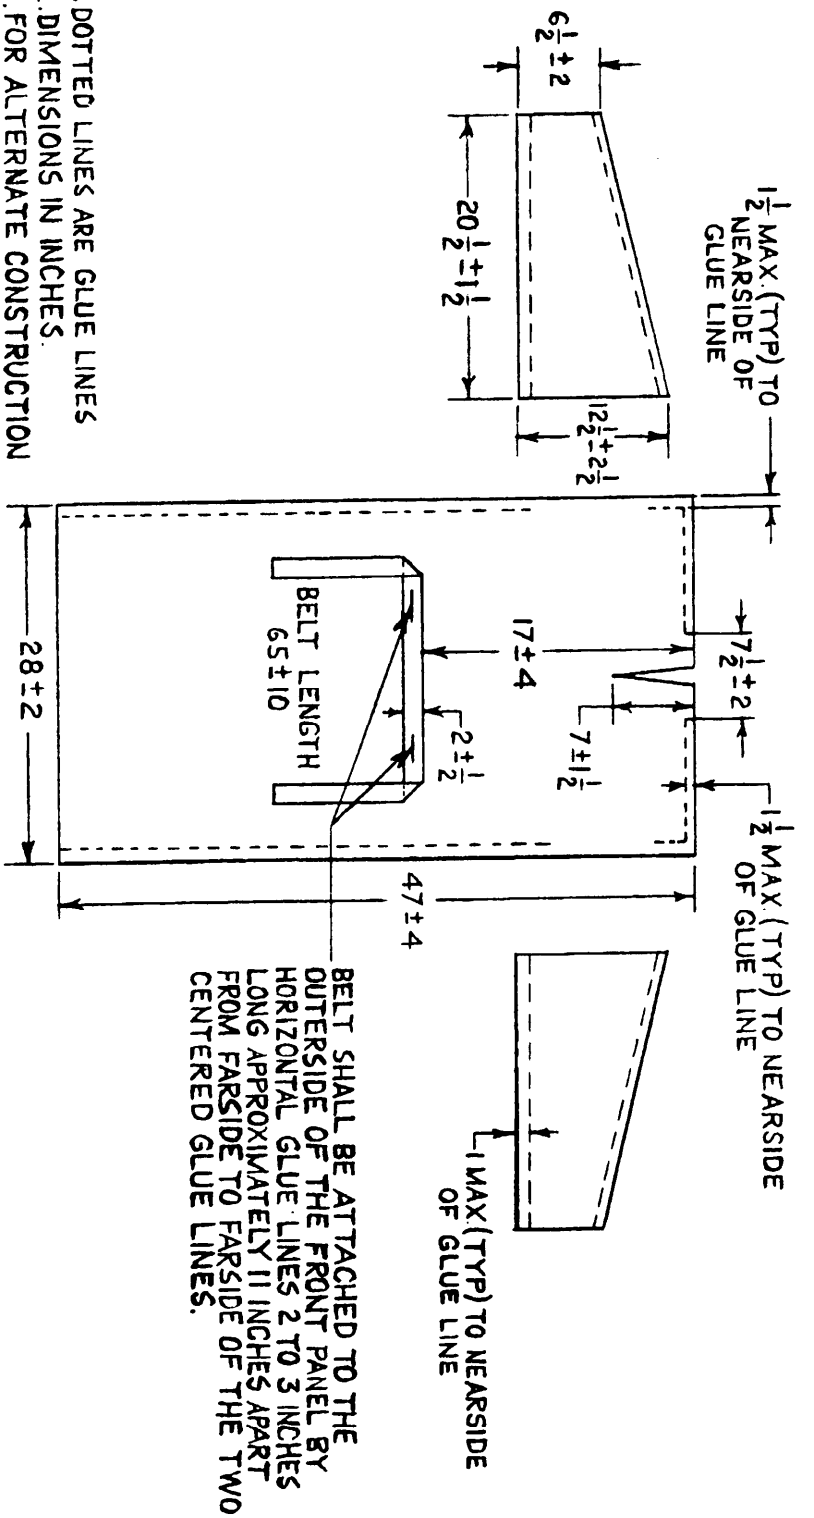

FRONT
GLUED SEAMS
FIGURE 1


Source: https://assist.dla.mil -- Downloaded: 202640-21T10:24Z
Check the source to verify that this is the current version before use.

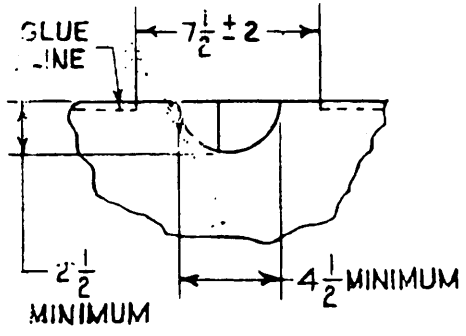

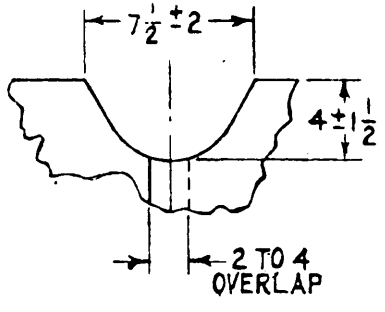


ALTERNATE NECK OPENINGS AND OVERLAP

NOTE: 1. DIMENSIONS IN INCHES
2. GLUE LINES & SLEEVES NOT SHOWN
3. FOR ALTERNATE CONSTRUCTION SEE 3.3.1.1.

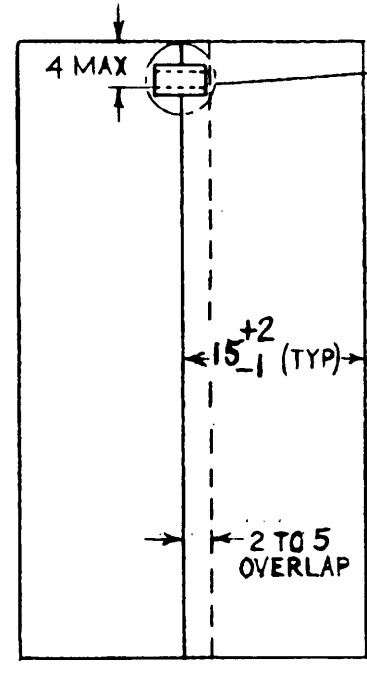


BACK
GLUED SEAMS
FIGURE 2

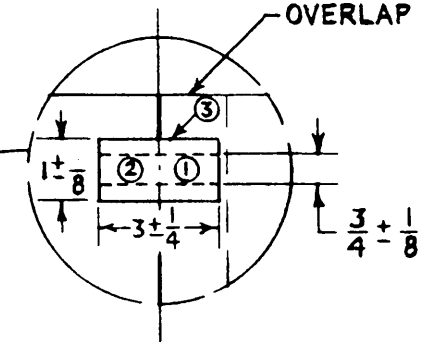

1. PORTION OF TAPE STRIP ON UNDERNEATH SIDE OF OVERLAP PANEL.
2. PORTION OF TAPE STRIP EXTENDING BEYOND PANEL.
3. SOLID LINE IS TREATED PAPER BACKING STRIP WITH THE WORD "PEEL" CONTINUOUSLY PRINTED ON IT.
4. BOTH TAPE AND BACKING SHALL BE 3 INCHES LONG. THE BACKING STRIP SHALL COMPLETELY COVER THE FREE ADHESIVE SURFACE


Source: https://assist.dla.mil -- Downloaded: 202640-21T10:24Z
Check the source to verify that this is the current version before use.

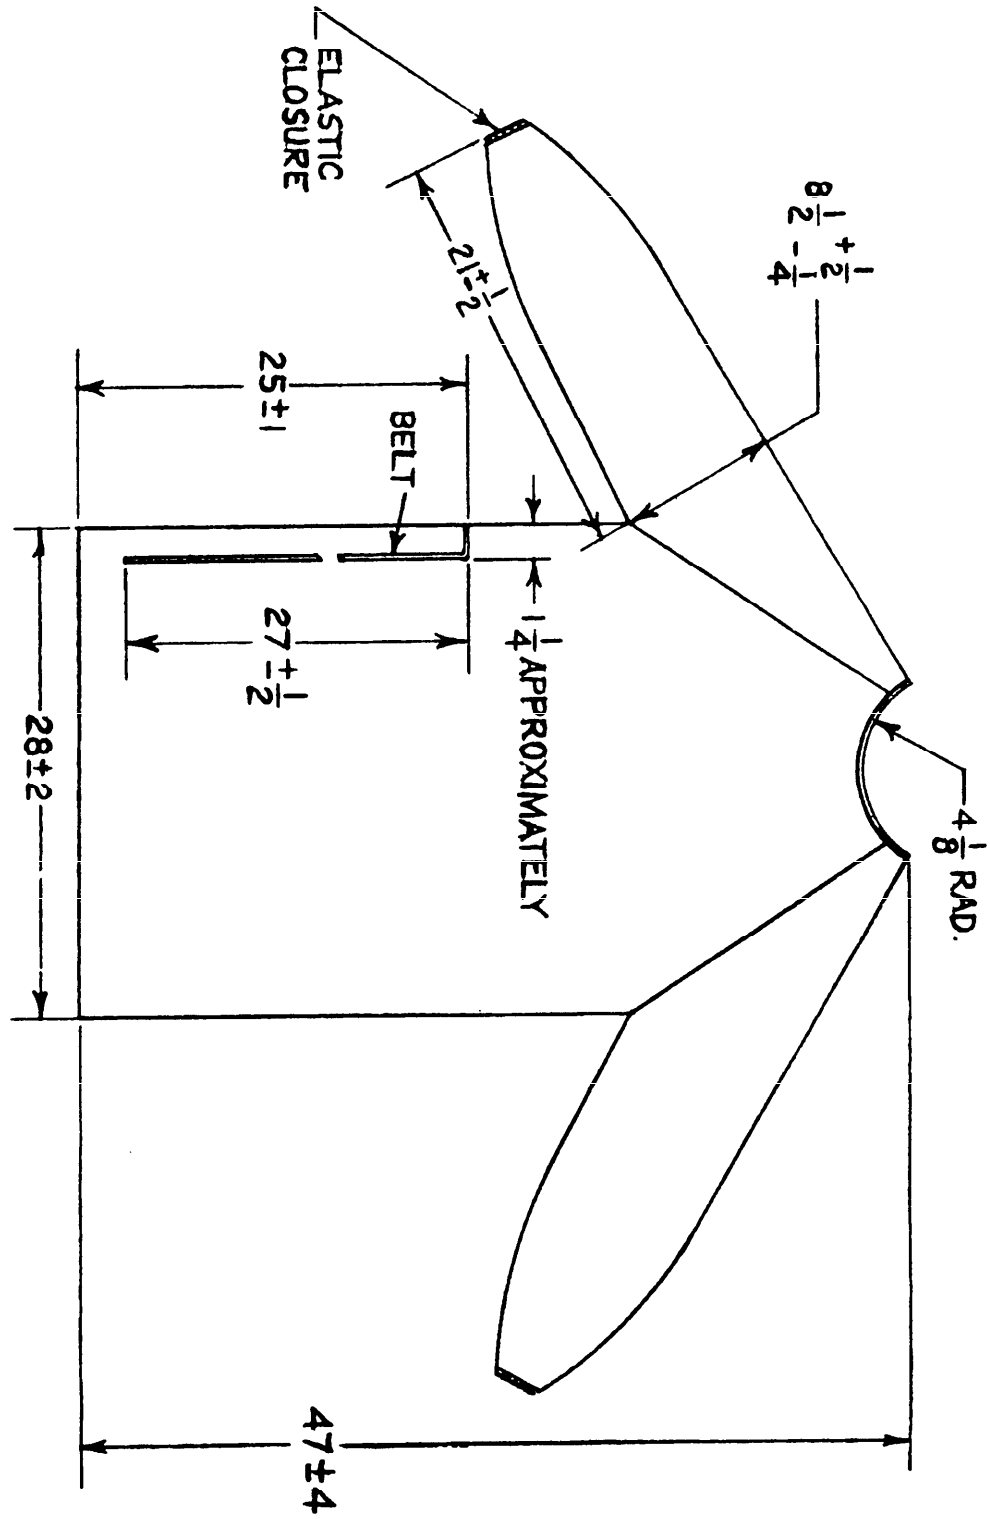

NOTES: 1. DIMENSIONS IN INCHES
2. FOR ALTERNATE CONSTRUCTION SEE 3.3.1.2.

FRONT
SEWN SEAMS
FIGURE 3

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

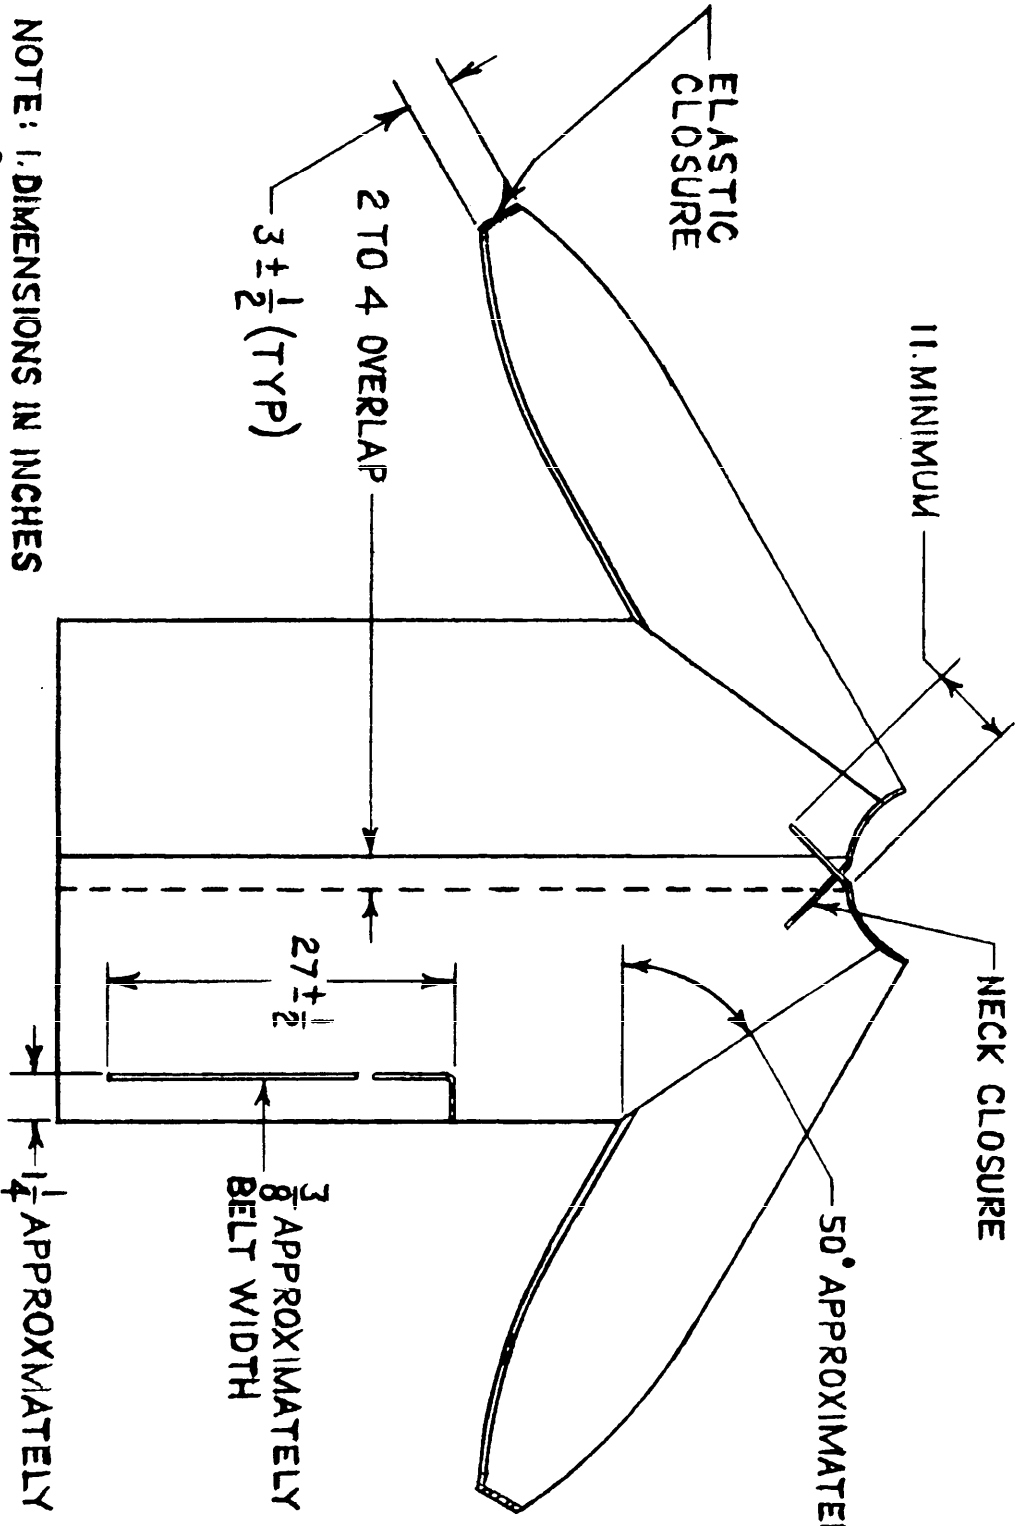

NOTE: 1. DIMENSIONS IN INCHES
2. FOR ALTERNATE CONSTRUCTION SEE 3.3.1.2.

SEWN SEAMS

FIGURE 4

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-G-37302 GOWN, HOSPITAL, NONWOVEN FABRIC, DISPOSABLE, UNIVERSAL SIZE

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304



OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:24Z
Check the source to verify that this is the current version before use.