MIL-L-37313A
21 August 1978
SUPERSEDING
MIL-L-37313
29 JULY 1976

MILITARY SPECIFICATION

LIGHTS, SURGICAL, CEILING

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers single and twin track-type suspension surgical ceiling lights, suitable for use in obstetrics and emergency surgery in military medical treatment facilities with ceiling heights ranging from 8 feet, 8 inches to 13 feet.

1.2 Classification. Surgical ceiling lights covered by this specification shall be of the following types (see 6.2).

Type I - Single track-type suspension

Type II - Dual track-type suspension (one light on each track)

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents, of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

PPP-B-601 - Boxes, Wood, Cleated-Plywood.
PPP-B-621 - Boxes, Wood, Nailed and Lock-Corner.
PPP-B-1055 - Barrier Material, Waterproofed, Flexible.

MILITARY

MIL-P-116 - Preservation, Methods of
MIL-M-7298 - Manual, Technical, Commercial Equipment

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

STANDARDS

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

ASTM A512 Cold-Drawn Butt Weld Carbon Steel Mechanical Tubing
ASTM B26 Aluminum Alloy Sand Castings

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103.)

NATIONAL FIRE PROTECTION ASSOCIATION (NFPA)

NFPA 56A Standard for the Use of Inhalation Anesthetics

(Application for copies should be addressed to the National Fire Protection Association, 470 Atlantic Avenue, Boston, MA 02210.)

UNDERWRITERS' LABORATORIES, INC. (UL)

UL 57 Standard for Electric Lighting Fixtures

(Application for copies should be addressed to the Underwriters' Laboratories, Inc., 1285 Walt Whitman Road, Melville, LI, NY 11749, 207 East Ohio Street, Chicago, IL 60611, 1655 Scott Boulevard, Santa Clara, CA 95050, and 333 Pfingsten Road, Northbrook, IL 60062.)

WELDERS HANDBOOK, 6th Edition

American Welding Society.

(Application for copies should be addressed to American Welding Society, Inc., 345 East 47th Street, New York, NY 10017.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Fire and casualty hazards.

3.1.1 The contractor shall submit proof, prior to delivery, that the items to be delivered under the contract conform to the applicable requirements of UL Standard of Safety 57 and all applicable requirements of NFPA 56A. Proof shall consist of one of the following:

A. UL label affixed to the product, provided the contractor agrees to have Underwriters' Laboratories, Inc. forward a copy of the UL report directly to the Contracting Officer, upon the latter's request.

B. Laboratory report from a nationally recognized independent laboratory. If an independent laboratory is used, it must be adequately equipped and competent to determine compliance with UL standards. The Government reserves the right to require a facilities report and to conduct a facilities survey. Any laboratory report submitted shall include actual test methods, data taken, and results of tests. Detailed findings of examinations necessary to determine compliance shall also be included. The test report shall also have a section that describes the test sample in such a way that the report can be used to insure identity of production items with the test sample. This section shall be supplemented with construction information such as materials used, spacings between electrical components, types of bushings, photographs, wiring diagrams, sketches, and parts list, all appropriately identified. Compliance with this paragraph does not excuse compliance with all other requirements of the contract and specifications.

3.2 Material.

3.2.1 Track. Each track shall be fabricated from extruded aluminum alloy having a minimum thickness of 1/8 inch.

3.2.2 Reflector. The reflector shall be fabricated from aluminum alloy sheet having a specular reflecting surface.

3.2.3 Bulb. The light source shall be an incandescent, spotlight service lamp, 150 watts, P-25, clear or medium inside frosted, 115 volt, medium screw base, rated at not less than 200 hours average life at rated voltage.

3.2.4 Carriage and suspension tube. Carriage and suspension tube shall be fabricated from cast and welded carbon steel parts.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

3.2.5 Crossarm and counterbalance. The crossarm and counter-balance assembly shall be fabricated from either aluminum casting alloy which is in accordance with ASTM B26 or carbon steel which is in accordance with ASTM A512.

3.2.6 Yoke and lamphead frame. The yoke and lamphead frame shall be fabricated from a suitable aluminum casting alloy which is in accordance with ASTM B26.

3.3 Construction. Each light shall consist of a ceiling mounted track, having a movable carriage from which an arm assembly supporting a light head shall be suspended, which shall be suitable for use in military medical facilities having ceiling heights ranging from 8 feet, 8 inches to 13 feet. Construction for type I and type II lights shall be in accordance with figures 1 and 2.

3.3.1 Track. Each track shall be designed and constructed to provide ease of movement and safe and stable support of a movable carriage carrying the suspension tube, crossarm and light head, when at rest or in motion. Track may be self-trimmed or may be fitted with a suitable cover. Design shall be such as to minimize dust catching, and track shall be furnished with suitable rubber gasket or trim for installation at the ceiling line when flush mounted to the ceiling. Track shall be provided with a means of leveling. The track shall be designed to prevent sparking and to provide current to the light carrying carriage over its full range of movement on the track. The track length shall not be less than 54 inches long for type I lights and approximately 9 feet long for type II lights; both types shall be suitable for mounting flush to the ceiling or on extension supports where required by ceiling height. Type II tracks shall be designed for mounting parallel. Also allowable will be tracks longer than 9 feet having keyed connections so that carriages track smoothly over the joints and the buss bars provide continuous electrical contact for the carriage power pickups to prevent flickering.

3.3.2 Carriage. The movable carriage shall be designed to operate with the track and the trolly system, and shall move freely along the operational length of the track while safely supoporting the suspension tube, crossarm assembly, and light head in a stable manner. All electrical current carrying components extending below the track shall be enclosed.

3.3.3 Suspension tube. The vertical suspension tube shall be attached to the carriage at its upper end, and to the crossarm assembly at its lower end in such a manner that the crossarm assembly can rotate 360° about the axis of the suspension tube. Electrical current carrying components shall be housed in the suspension tube, except that wires leading from the suspension tube to the crossarm assembly may be outside the swivel connection, in which case they shall be protected by a suitable flexible metal sheathing.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

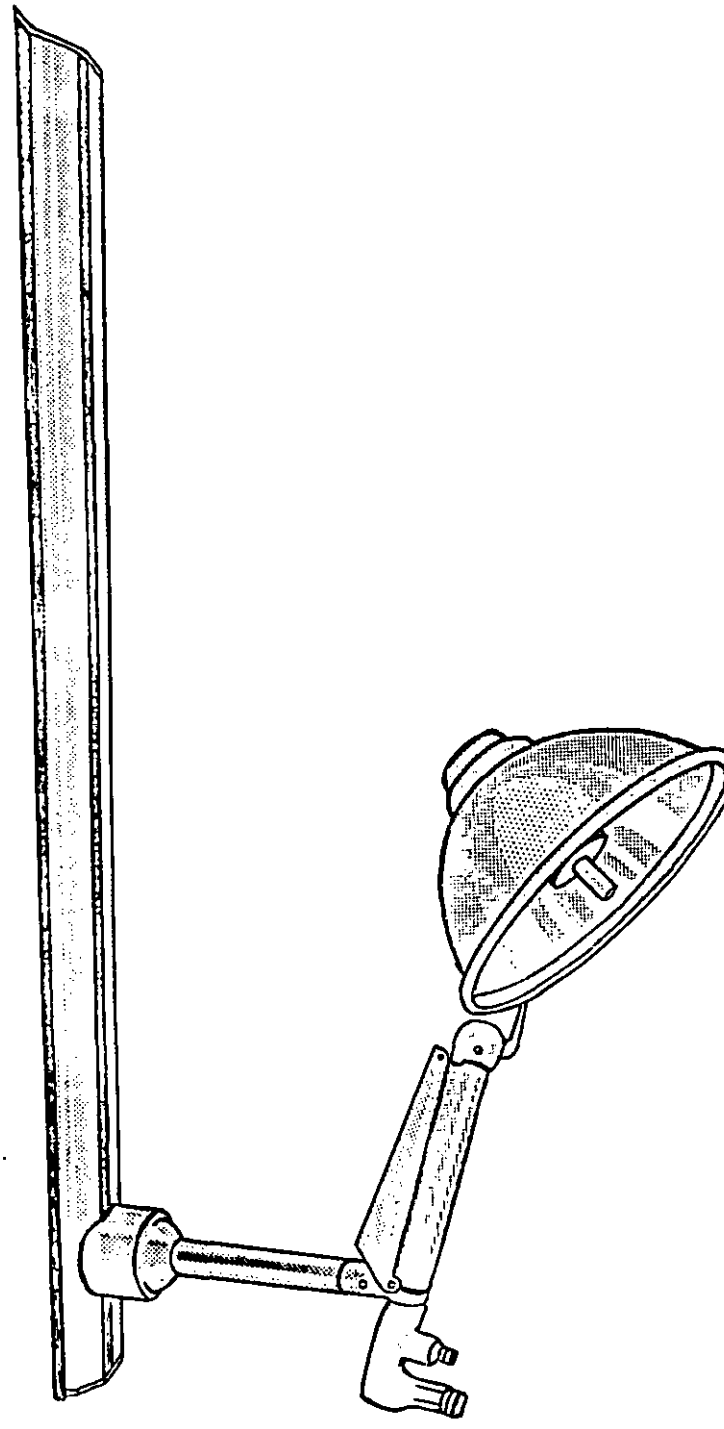


FIGURE 1. Single track-type suspension

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

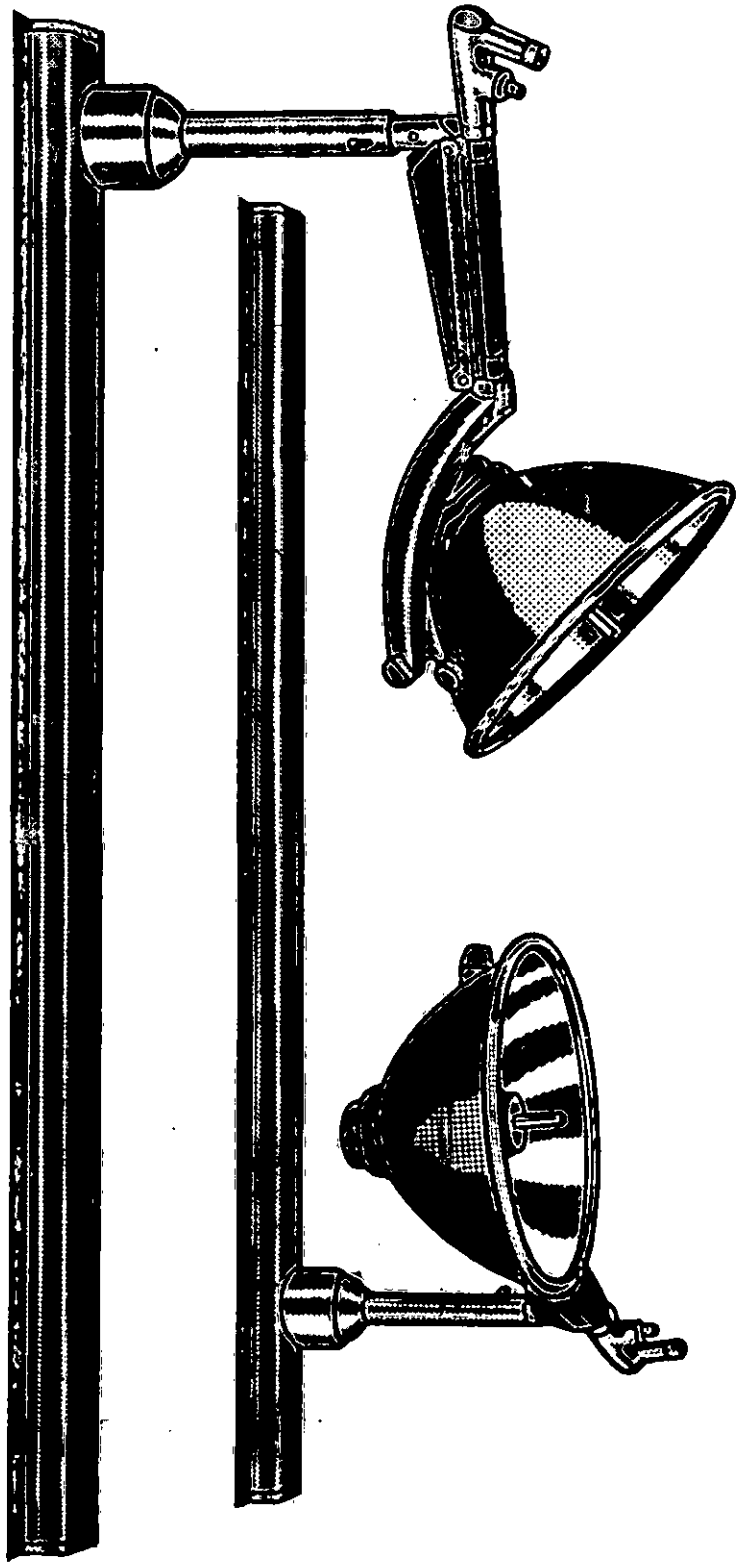


FIGURE 2. Twin track-type suspension

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

3.3.4 Crossarm assembly. The crossarm assembly for types I and II shall be designed to provide vertical adjustment of the lamphead assembly. The crossarm assembly shall have a yoke which is capable of safely and adjustably supporting a light head at one end; at the opposite end shall be a handle for positioning the light head together with a switch for controlling the light. The crossarm assembly shall be pivotally mounted on the bottom of the suspension tube. The angle that the light head end of the arm can be depressed below horizontal, the length of the suspension tube, and the length of the crossarm from suspension tube to light head pivot(s) shall be such that in combination, the light head or any electrical portion cannot be brought into any position where the hot or current carrying parts are less than 5 feet from the floor when the unit is properly installed for the specified ceiling height as defined by NFPA. The crossarm assembly shall be counter-balanced so that the light may be moved easily and will hold any position in which it is put, without the use of counter weights. The end of the arm opposite the light head shall project beyond the suspension tube the minimum distance compatible with easy positioning of the light, using the handle provided. For type II lights, it shall be possible to position the lights so that they may pass each other and will not interfere with the x-ray or other equipment which may be track mounted between the light tracks. The yoke shall be mounted on the crossarm so that it will rotate 90° to either side of the yoke position where the center line (light beam axis) of the light head is vertical. All electrical current carrying components shall be enclosed in the members of the crossarm assembly, except that the wires leading from the yoke to the light head may be brought out of the yoke arm(s), in which case, the length exposed shall be protected by suitable flexible metal sheathing.

3.3.4.1 Type II. The length of the control arm and yoke for type II shall be such that, when the control arm is horizontal and at right angles to the length of the track, with the light head between the two tracks and the center line of the light head (axis of beam) vertical, the distance between the center lines of the suspension tube and the light head shall be at least half the center to center distance between the tracks. It shall be possible to position the lights so that they may pass each other and shall not interfere with other equipment which may be track mounted between the light tracks.

3.3.5 Light head. The light head shall be designed to incorporate a reflector and optical assembly. The light head shall consist of an open type reflector 22 to 25 inches in diameter. The reflector shall be fabricated of aluminum, treated to provide a durable, highly reflective specular reflecting surface (reflectivity not less than 85 percent). Testing shall be as specified in 4.4.4. The reflecting surface shall have the specular finish protected by a film of clear anodize of sufficient

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

thickness to prevent clouding, staining, oxidizing or peeling during the life of the unit, and shall be tested as specified in 4.4.7. The light source shall be as specified in 3.2.3. The light source shall be totally enclosed within a heat-resisting, heat-absorbing glass enclosure having its base or bottom equipped with, or treated to provide, a shield against direct glare. The light source shall be mounted so that the light beam may be focused to provide large or small illuminated surgical fields. A conveniently located means of adjusting the focus shall be provided. The focusing shall be continuously variable between the "small" and "large" positions. A removable, sterilizable positioning handle shall be mounted in the optical axis of the light head to permit final positioning by the surgeon. Design of lamp and reflector shall provide for proper illumination; illumination requirements are indicated in 3.4.

3.3.6 Variable voltage control. A wall mounted variable voltage control unit to vary the voltage input in order to control the illumination intensity shall be provided. The variable voltage control unit shall be located at least five feet above the floor level of the room. The control unit shall have the following controls for operator accessibility: on-off switch and rotary selector switch to control voltage output to the light(s). The control unit shall be capable of furnishing approximately 135 volts to the lamp (for maximum intensity) with a line voltage of 115 volts, 60 Hertz, AC.

3.4 Performance.

3.4.1 Light beam characteristics. The light when operated at rated voltage shall provide the following beam characteristics:

a. Color temperature shall be within a range of 3500° to 6700° Kelvin (K.); recommended and acceptable trichromatic coefficients for this temperature range are found in table I, see 4.4.2.

TABLE I. Trichromatic coefficients

X	Y
0.310	0.310
0.400	0.375
0.400	0.415
0.375	0.415
0.310	0.365

b. Illumination in the surgical field from the light shall be as follows when the light is operated at rated voltage in a plane at 42 inches focal distance; surgical field pattern not less than 2500 foot candles or 27,000 lumens per square meter ($1/m^2$) for an 8 inch diameter field. Testing shall be conducted in accordance with 4.4.3.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

c. Illumination of the axis of the light beam shall not be reduced more than 50 percent when an opaque disc is inserted in the light beam when tested as specified in 4.4.3.2. More than 50 percent reduction constitutes a failure.

3.4.2 Lamp life. The lamp shall provide at least 200 hours of useful life at a cycle rate of 4 hours "ON" and 1/2 hour "OFF" when tested as specified in 4.4.5.

3.4.3 Heat cylinder. The glass heat cylinder shall absorb infrared rays to the degree such that a temperature rise on a black body in the light beam located 20 inches from the reflector rim shall be less than 3° Farenheit (F.) above ambient per 1000 foot candles when measured 42 inches from the reflector rim. Testing shall be in accordance with 4.4.6.

3.4.4 Dielectric strength. There shall be no electrical breakdown when tested as specified in 4.4.8.

3.5 Finish. Exposed surfaces of the track, light head, yoke, carriage and supporting parts shall have a baked painted finish. All other exposed parts shall be suitably finished to resist corrosion.

3.6 Identification marking. Each light shall be permanently and legibly marked with the national stock number, the manufacturer's name or registered trademark, the contract or purchase order number, the model and serial number and electrical characteristics (volts, amperes, watts and Hertz).

3.7 Workmanship. Workmanship shall be first class throughout. The finished product shall be clean, smoothly finished with no rough or protruding edges, and free from defects which detract from its appearance or may impair its serviceability.

3.7.1 Welding. Welding shall be durable, sound in every detail and in accordance with latest practices recommended by the American Welding Society. All welds shall be produced by qualified welding operators with satisfactory welding equipment using satisfactory filler metal and/or electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreign matter. Any cleaning method which will remove the substances and leave the surface clean is satisfactory. All aluminum parts shall be welded within 48 hours after a chemical cleaning treatment. Parts must be chemically recleaned if the 48 hour time period is exceeded. All weld joints shall blend into the adjacent metal in gradual smooth curves. Beads shall be smooth and free of slag, excessive undercut, or excessive spatter. Sufficient metal shall be added to provide a suitable fillet or reinforcement unless otherwise specified. Welds shall not be oxidized. All welds shall be continuous with no visible voids, pin holes, or cracks which

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

affect the quality, and have more strength than required for the purpose intended. For the purpose of requirements in this specification, welded fully, fully welded, continuously welded and continuous weld shall all have the same meaning such that all the mating surfaces between the parts welded are closed by welds without any breaks or voids. Grinding wheels used to remove excess weld metal and to prepare weld surfaces for subsequent polishing operations shall be of a suitable grit, free of metal filings or other iron materials such as iron oxides which would tend to cut into the parent metal surfaces and allow for rusting at a later date. Spot welds, if used, shall be free from surface burning, cracks, and porosity, and shall be of sufficient strength to pull the spot out of the parent metal when pulled apart.

3.8 Service data. The contractor shall furnish, with each unit, two copies each of a technical manual which contains complete instructions for installation, operation, and maintenance and lists of component parts. The manual shall comply with the requirements of MIL-M-7298. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer, via the cognizant Government inspector, two preliminary copies of his proposed technical manual for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract, or purchase order. In addition, the Contractor shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of the contract and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies shall be at the option of the Government.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component or materials may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government and provided also that the test methods and the results obtained comply with those described in this specification. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and table II.

TABLE II. Sampling for examination.

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Total (major and minor combined) defects	II	4.0
For dimensional examination	S-3	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

4.2.2 For tests. Sampling for tests shall be in accordance with MIL-STD-105 and table III. Certification establishing proof that testing required in 4.4.2, 4.4.4, 4.4.6 and 4.4.7 has sucessfully been passed with a surgical ceiling light of the identical design and construction as that being supplied under the current contract shall be considered acceptable providing such test was conducted within two years prior to the date of the contract or purchase order. In lieu of testing specified in 4.4.5, compliance with lamp life requirements may be established by the submission by the contractor of evidence that the lamp being supplied is advertised commercially on a national basis as having at least the required life. The Government reserves the right to verify compliance.

TABLE III. Sampling for tests.

Requirement	Para. No.	Test	Para. No.	Inspection level	AQL(defects per hundred units)
Crossarm assembly	3.3.4	System test	4.4.1	II	2.5
Variable voltage control	3.3.6	System test	4.4.1	II	2.5
Performance - Light beam characteristics	3.4.1	Color temperature	4.4.2	S-1	1/
Performance - Light beam characteristics	3.4.1	Surgical field pattern	4.4.3.1	S-1	1/
Performance - Light beam characteristics	3.4.1	Light beam Illumination reduction	4.4.3.2	S-1	1/
Light head	3.3.5	Reflectivity measurements	4.4.4	S-1	1/
Lamp life	3.4.2	Lamp life test	4.4.5	S-1	1/
Heat cylinder	3.4.3	Heat cylinder	4.4.6	S-1	1/
Light head	3.3.5	Sealing test	4.4.7	S-1	1/
Dielectric strength	3.4.4	Dielectric test	4.4.8	100%	1/

1/ Acceptance number is zero. Any test failure constitutes a rejection during these tests.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

4.3 Examination. The light assemblies shall be examined to determine compliance with the requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects listed in table IV. Examination shall not be restricted to the classified possible defects listed below.

TABLE IV. Classification of defects.

Categories and defects	
Major	
101	Any component part missing, broken, or otherwise unusable.
102	Exposed edges not free of burs or sharpness.
103	Components not properly aligned or fitted.
104	Wiring defective.
105	Carriage not easily movable along operational range of track.
106	Exposed surfaces not free of unpainted or corroded areas.
107	Crossarm assembly not pivoting properly about suspension tube.
108	Light reflector not pivoting properly about the yoke.
Minor	
201	Identification marking omitted, illegible, or not as specified.
202	Painted and plated surfaces not free of blisters, and peeled, scratched or uncoated areas.
203	Surfaces of components not clean and free of dirt and foreign matter.
204	Service data not as specified.

4.3.2 Dimensional examination. The light shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.3.3 Packaging inspection. The inspection of the preservation-packaging and interior package marking shall be in accordance with the group A and B quality conformance inspection requirements of MIL-P-116. The inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 System test. A system operation simulation test shall be performed to insure proper functioning of all applicable components except Major defects 105 and 107 as described in table IV above.

4.4.2 Color temperature. Color temperature as specified herein establishes the isothermal relationship between the Planckian locus and a point, which is a plot of the X, Y coordinate of color on the chromaticity diagram. Measurement shall be performed at room temperature by means of a suitable spectrophotometer of standard make and model. The chromaticity diagram and certification by the manufacturer of the heat cylinder and certification by the lamp manufacturer shall be acceptable as evidence that the heat cylinder and lamp meet the color temperature requirements as specified herein.

4.4.3 Illumination.

4.4.3.1 Surgical field pattern. The light shall be operated at rated voltage (115 volts, AC). The light beam shall be focused to provide a small illuminated surgical field. Measurements shall be made in a plane at 42 inches focal distance from rim of reflector surface with a brightness meter (see 6.3). Readings shall be recorded in foot candles and lumens per square meter.

4.4.3.2 Light beam illumination reduction. The illumination of the axis of the light beam at a focal distance of 42 inches from rim of reflector surface shall be taken with a brightness meter (see 6.3). The reading in foot candles shall be recorded. A 6 inch diameter disc fabricated of an opaque material shall be located in the light beam centered on and normal to its axis at a distance of 15 inches from the reflector rim. At a focal distance of 42 inches and with the opaque disc located and affixed in place, the illumination of the axis of the light beam shall again be taken with the meter and recorded.

4.4.4 Reflectivity measurements. Measurements shall be performed at room temperature by means of a suitable reflectometer of standard make and model. Certification by the company applying the finish to the reflector shall be acceptable as evidence that the finished reflector meets the reflectivity requirements specified herein.

4.4.5 Lamp life test. Using a 115 volt input at a cycle rate of 4 hours on and 1/2 hour off, the lamp shall be tested at room ambient conditions. A slight darkness observed on the interior of the frosted surface, resulting in some decrease of light output as the lamp ages with use, is a normal condition and is not a defect.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

4.4.6 Heat cylinder. A 0.5 inch by 0.5 inch thick steel body having a flat black finish shall be located in the light beam 20 inches from the rim of the reflector. A thermocouple shall be attached to the center of the body and with the light off, the room ambient temperature shall be noted. The light shall then be turned on for a period of three continuous hours until the temperature of the black body stabilizes. Temperature readings shall be taken during this period denoting temperature rise above ambient. The light shall be operated at rated voltage during this test.

4.4.7 Sealing test. Dissolve one gram of aluminum blue 2LW dye in 50 ml of distilled or deionized water. The pH of the dye test solution shall be adjusted to 5.0 $\pm$ 0.5 and maintained at this value with the addition of acetic acid or sodium hydroxide as required. A drop of the water solution shall be applied to the specular surface of the reflector at room temperature. Allow it to stand for 5 minutes then wash with running water. Saturate a soft cloth with a solution of mild soap and water and abrade the area tested. There shall be no evidence of stain or discoloration.

4.4.8 Dielectric withstand. After light has been operational for 1/2 hour, a slowly rising potential, from 0 to 1240 volts, 60 Hertz, shall be applied between live and dead metal parts. The potential shall be maintained at maximum for one minute. There shall be no evidence of breakdown.

5. PACKAGING

5.1 Preservation - packaging. Preservation-packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Cleaning. Lights shall be cleaned in accordance with MIL-P-116.

5.1.1.2 Drying. Lights shall be dried in accordance with MIL-P-116.

5.1.1.3 Preservative application. Preservatives shall not be used.

5.1.1.4 Unit packaging. Each light, type I or type II, shall be disassembled as far as is practicable and packaged in accordance with MIL-P-116, method III. All components comprising the light assembly shall be wrapped in kraft paper or other suitable non-corrosion material and cushioned with suitable cushioning material to prevent damage during shipping and handling.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

5.1.2 Level C. Each light, type I or type II, shall be packaged in a manner that will afford adequate protection against corrosion, and physical damage during shipment from supply source to the first receiving activity.

5.2 Packing. Packing shall be level A or C as specified (see 6.2).

5.2.1 Level A. Each light, type I or type II, shall be packed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-601, overseas type or PPP-B-621, class 2. The light shall be blocked, braced and cushioned within the container in such a manner to insure against damage or marring of components. All box panels, except the base, shall be lined with a waterproof barrier material conforming to PPP-B-1055, class L-2. As an alternate, each light shall be protected with a shroud fabricated of material conforming to PPP-B-1055, class L-2. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. Each packaged light, type I or type II, shall be packed in a manner that will afford adequate protection against damage during direct shipment form the supply source to the first receiving activity. This pack shall conform to the applicable carrier rules and regulations.

5.3 Marking. Each exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The lights shall be suitable for use in obstetrics and emergency surgery in military medical treatment facilities.

6.2 Ordering data. Procurement documents should specify the following:

(a) Title, Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(c) Type required (see 1.2).

6.3 An acceptable brightness meter is Luckiesh-Taylor Brightness meter or equivalent.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

6.4 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification	Type
6530-00-982-4374	LIGHT, SURGICAL, CEILING, Open Dome Type, 25 inch Maximum Diameter, 115 volt, 60 Hz, AC	I
6530-00-982-4375	LIGHT, SURGICAL, CEILING Open Dome Type, 25 inch Maximum Diameter, 115 volt, 60 Hz, AC	II

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Logistics Agency - DLA-DM

Project No. 6530-1463

Review activity:
DoD-MB

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

POSTAGE AND FEES PAID

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

DEFENSE PERSONNEL SUPPORT CENTER
DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS: This form is provided to solicit beneficial comments which may improve this document and enhance its use. DoD contractors, government activities, manufacturers, vendors, or other prospective users of the document are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity. A response will be provided to the submitter, when name and address is provided, within 30 days indicating that the 1426 was received and when any appropriate action on it will be completed.
NOTE: This form shall not be used to submit requests for waivers, deviations or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

DOCUMENT IDENTIFIER *(Number)* AND TITLE
MIL-L-37313A LIGHTS, SURGICAL, CEILING

NAME OF ORGANIZATION AND ADDRESS OF SUBMITTER

☐ VENDOR ☐ USER ☐ MANUFACTURER

1. ☐ HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE? ☐ IS ANY PART OF IT TOO RIGID, RESTRICTIVE, LOOSE OR AMBIGUOUS? PLEASE EXPLAIN BELOW.

A. GIVE PARAGRAPH NUMBER AND WORDING

B. RECOMMENDED WORDING CHANGE

C. REASON FOR RECOMMENDED CHANGE(S)

2. REMARKS

SUBMITTED BY *(Printed or typed name and address — Optional)*

TELEPHONE NO.

DATE

DD FORM 1 OCT 78 1426 EDITION OF 1 JAN 72 WILL BE USED UNTIL EXHAUSTED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:25Z
Check the source to verify that this is the current version before use.