A-A-51812A
20 February 1989
SUPERSEDING
A-A-0051812(DM)
5 February 1987

COMMERCIAL ITEM DESCRIPTION

FORCEPS, EYE, Suture

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers an iris forceps of the Troutman design with a Colibri type tip suitable for use in microsurgery.

Salient characteristics:

Material. Forceps shall be manufactured from martensitic corrosion-resistant steel of composition in accordance with American Society for Testing and Materials (ASTM) Designation F899.

Hardness. The forceps shall have a Rockwell Hardness C scale (HRC) of 45 to 50 when tested in accordance with ASTM Designations E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Style and design. Forceps shall be of the style and dimensions shown in Figure 1. Forceps shall have an integral typing platform (not shown in Figure 1). Forceps teeth shall meet and mesh exactly when closed in the normal manner.

Passivation. Forceps shall be properly passivated.

Finish. The finish of the forceps shall be satin. The finish shall be uniform and free from burrs, scale, rough areas, and tool marks.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

Identification marking and labeling. Forceps shall be permanently marked with the contractor's name or registered trademark and the word "stainless." In addition, forceps of foreign manufacture shall bear the name of the country of manufacture.

Corrosion resistance. The forceps shall show no signs of corrosion or plating of copper when tested in accordance with ASTM Designation F1089.

Performance. The forceps teeth shall mesh completely and uniformly and re-open to the normal position when tested as specified herein.

Workmanship. The forceps shall be processed in such a manner as to be uniform and free from defects which affect life, utility, or appearance.

Product Quality Level

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One forceps, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:01Z
Check the source to verify that this is the currenversion before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The forceps shall be examined to determine compliance with all requirements contained in this specification.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one forceps. Sampling shall be level S-2, AQL 1.0.

Performance. Remove the hinge screw and separate the forceps members. Reassemble the forceps. Close the forceps in the normal manner and examine the tip. The teeth shall mesh completely and uniformly. Release pressure on the forceps handles. The forceps tips shall separate to a distance of 3.2 mm plus or minus 0.5 mm with no manipulation by the user. Forceps whose teeth do not mesh or which do not re-open to the normal position shall be rejected. Further, any forceps in which the hinge pin threads strip or the pin breaks shall be rejected.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:01Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-098-5787	FORCEPS, EYE, Suture, Colibri, Angled, 6 cm

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 47109

Project No. 6515-4549

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

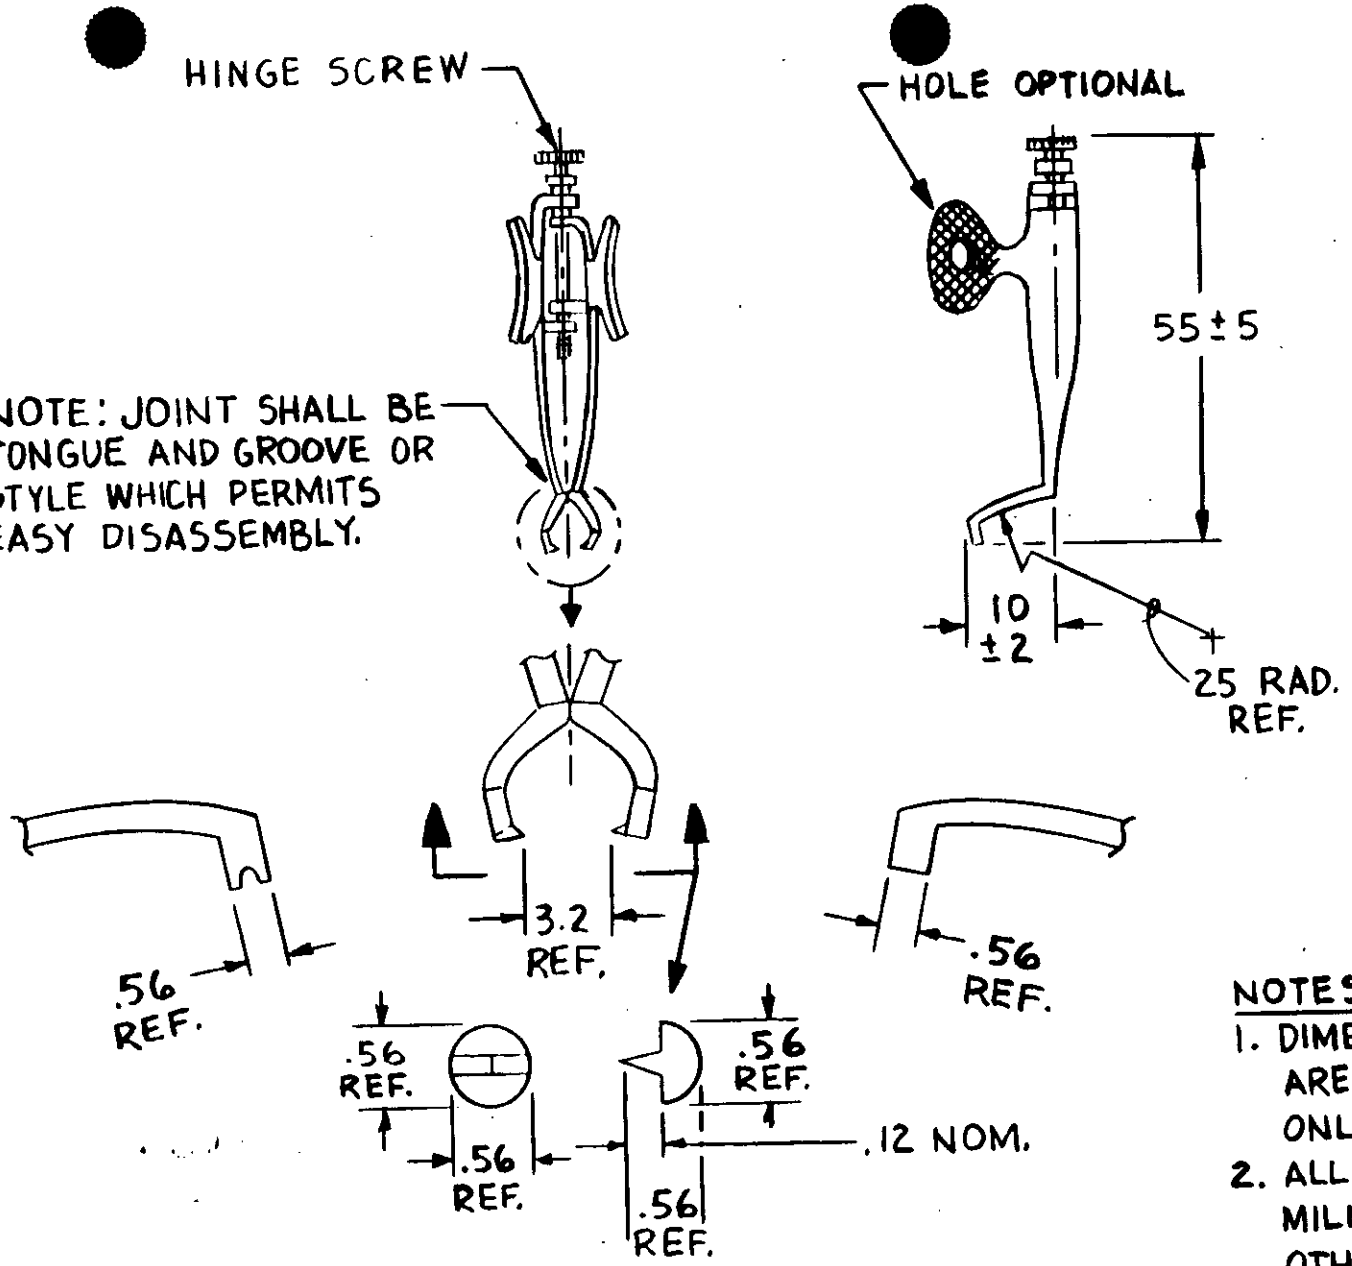

NOTES:

1. DIMENSIONS MARKED "REF." ARE FOR STYLE AND DESIGN ONLY.
2. ALL DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED.

A-A-51812A

FIGURE 1 FORCEPS, EYE, SUTURE

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T09:01Z
Check the source to verify that this is the current version before use.