A-A-51841
13 April 1987

COMMERCIAL ITEM DESCRIPTION

RULER, ENDODONTIC INSTRUMENT
(Finger ring, right handed)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a right handed finger ring endodontic instrument ruler used in measuring instruments from 1 to 35 mm in increments of 1/2 mm.

Salient characteristics:

The endodontic ruler shall be a right handed finger ring ruler used to measure endodontic instruments. The endodontic ruler shall be a two-piece construction, a flat scale and an open, adjustable ring configuration, to fit a left hand finger. The endodontic ruler shall have a range of 35 mm. The endodontic ruler shall have 2 scales. One scale shall be legibly and permanently numbered every 5 mm, with 1 mm markings and shall be nominally 3/16 inch high. The scale shall read from right to left, with the zero toward the finger tip and the highest number toward the knuckle. The other scale shall be marked at 1/2 mm increments with every second increment marking (1 mm) coinciding with the mm markings of the 1 mm scale and shall be nominally 1/16 inch high. The error on each scale shall be no more than 1/10 mm per 35 mm. The overall ruler shall be 38 $\pm$ 1 mm long, 12 $\pm$ 1/2 mm wide and 0.47 $\pm$ 0.015 mm thick. The finger ring shall be 8 $\pm$ 0.1 mm wide and 0.75 $\pm$ 0.03 mm thick. The ruler shall conform to the design shown in Figure 1.

Material. The endodontic ruler shall be fabricated of corrosion resisting steel, and shall be of sufficient stiffness for normal use. The endodontic ruler shall be autoclavable and shall show no sign of corrosion when tested in accordance with the autoclavability test as specified herein.

The finger ring shall be adjustable to fit any adult finger size, (5/8" dia. to 1" dia.). The finger ring shall be securely welded to the underside of the flat scale (ruler) at the center of the lengthwise axis and positioned between the 15 mm and 25 mm markings as shown in the design in figure 1. The endodontic ruler shall have a brightly polished finish with no burrs or burns.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

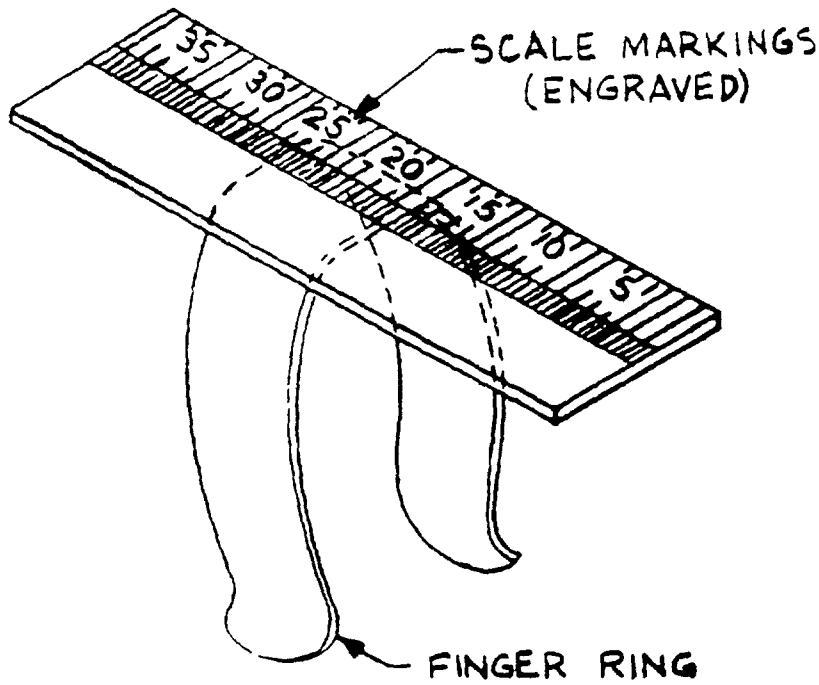


FIGURE 1.

RULER, ENDODONTIC INSTRUMENT, RIGHT-HANDED FINGER RING

Note: The endodontic instrument ruler shown is typical in design and is not intended to restrict or preclude the purchase of endodontic instrument rulers which are otherwise in accordance with the requirements of this document.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

Workmanship. The endodontic ruler shall be clean and free of sharp edges, burrs and pitting or any defect which detracts from its appearance or impairs its serviceability.

Unit. Each (EA). One endodontic ruler, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item. Inspection shall be conducted to determine compliance with specification requirements.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one endodontic ruler. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

Tests.

Autoclavability test. The endodontic ruler shall be cleaned in accordance with the instructions supplied by the manufacturer. The endodontic ruler shall then be autoclaved at 270° ± 5°F and 27 ± 1 pounds per square inch pressure for a minimum of 20 minutes. After the endodontic ruler is removed from the autoclave, the entire surface area of the endodontic ruler shall be examined for evidence of corrosion.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document.

Stock Number	Item Identification
6520-01-125-3247	RULER, ENDODONTIC INSTRUMENT, Finger Ring, Right Handed, Corrosion Resisting Steel.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:
Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA - DM

CIVIL AGENCY COORDINATING ACTIVITIES:
VA-OSS
PHS

49133

PROJECT NO. 6520-1981

Location: NCR Disk #2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements All users of military standardization documents are invited to provide suggestions This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C
POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-ATTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

NO POSTAGE
NECESSARY
IF MAILED
IN THE
UNITED STATES

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-51841	Ruler, Endodontic Instrument (Finger Ring, Right Handed)

3a. NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b ADDRESS *(Street, City, State ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5 PROBLEM AREAS

a. Paragraph Number and Wording

b Recommended Wording

c Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street, City, State ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 92 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.