INCH-POUND

A-A-54784
4 January 1993

COMMERCIAL ITEM DESCRIPTION

FORCEPS, TISSUE, Judd-Allis, Straight

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-F-36779, which is cancelled.

This commercial item description covers a tissue forcep of the Judd-Allis design, suitable for grasping portions of the gastrointestinal tract during surgical procedures.

Salient Characteristics:

General. Shall be a straight tissue forceps of the Judd-Allis design approximately 7-1/2 inches in overall length.

Material. Material shall be Class 4 corrosion resistant steel in accordance with ASTM F899.

Style, design and dimensions. Shall be a straight tissue forceps with jaws serrated and having 3 x 4 meshing teeth on the proximal end. The teeth shall mesh when the jaws are closed. Forceps shall be in accordance with Figure 1 for style, design and dimensions.

Hardness. Forceps shall have a Rockwell Hardness C scale (HRC) of 40 to 47 when tested in accordance with ASTM E18 or E92 whichever is applicable Conversion of hardness values shall be in accordance with ASTM E140

Finish. The finish of the forceps shall be satin, matte or mirror. The matte finish shall exhibit a uniform nondirectional surface texture equivalent to that produced by lightly blasting the prepared surface with fine abrasives under pressure

Passivation. Forceps shall be properly passivated.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:38Z
Check the source to verify that this is the currentversion before use.

Corrosion resistance. Forceps shall show no signs of corrosion or plating of copper when tested for corrosion resistance in accordance with ASTM F1089.

Identification marking and labeling. Forceps shall be legibly marked with the contractor's name or trademark and the word "stainless"; foreign manufactured forceps shall bear the name of the country of origin.

Workmanship. Forceps shall be processed in such a manner as to be uniform and free from cracks, pits, burrs, sharp edges, scale rough areas, corrosion, grind or tool marks, and dirt or polishing materials.

Unit. Each (EA) One forceps, as specified, constitutes one unit of issue.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection Unless otherwise specified in the contract of purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspection are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein Unit of product for examination purposes shall be one forceps as specified. Sampling shall be general inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one forcep Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:38Z
Check the source to verify that this is the currentversion before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-00-335-3500	FORCEPS, TISSUE, Judd-Allis, Straight, 7-1/2 inch

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5443
Location: c:\word\david\forcepcd

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

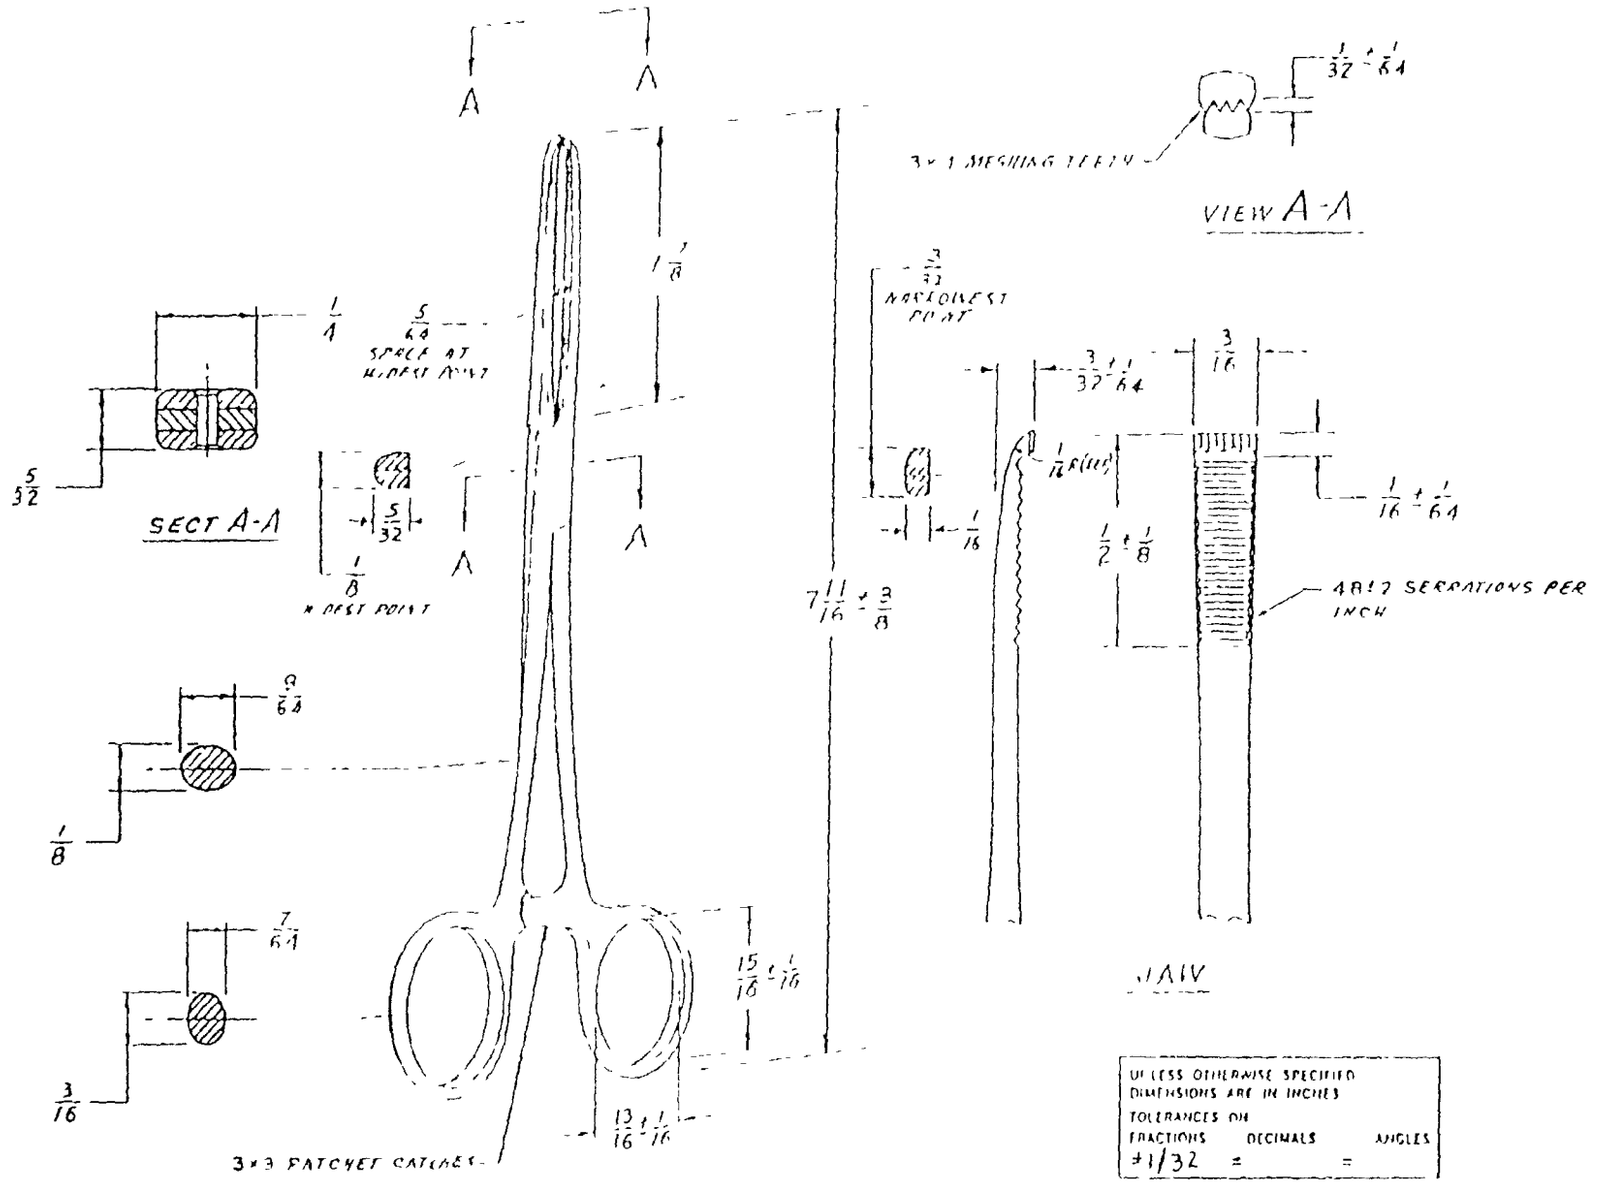

GENERAL NOTES

TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP

NSN 6515-00-335-3500

FIGURE 1 FORCEPS, TISSUE, JUDD-ALLIS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54784	2 DOCUMENT DATE (YYMMDD) 4 January 1993

3 DOCUMENT TITLE
FORCEPS, TISSUE, Judd-Allis, Straight

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite if possible Attach extra sheets as needed)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	e TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME Defense Personnel Support Center ATTN: DPSC-MSE	b TELEPHONE (Include Area Code) (1) Commercial: (215) 7372870 (2) AUTOVON: 444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 Previous editions are obsolete 190

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.