INCH-POUND

A-A-54786
8 January 1993

COMMERCIAL ITEM DESCRIPTION

STOPCOCK, INTRAVENOUS THERAPY

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-S-37174 which is cancelled.

This Commercial Item Description covers a sterile, disposable, stopcock with four separate fluid paths and Luer connectors.

Salient characteristics:

Material. The stopcock shall be manufactured from a rigid or semi-rigid plastic. The plastic shall be inert to blood and common IV fluids and meet the requirements of the USP for class II plastics.

Style, design and dimensions. The stopcock shall be one of the four styles shown in Figure 1.

The rotating plug shall be provided with three outwardly projecting arms which when superimposed over a body outlet port shall indicate the flow path through the stopcock. When all three rotating plug arms are superimposed over the three body ports, all fluid paths shall be flow interconnected.

The stopcock shall be furnished with plastic protectors on each connector which shall maintain sterility of the fluid path until removed.

Performance. The stopcock shall be suitable for use in administering and controlling the direction of flow of blood and solutions for simultaneous and with alternate intravenous therapy. Stopcocks shall be tested for freedom of pyrogens, leakage, clear passage of fluid, and security of assembly.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Sterility. The stopcock shall be sterile in accordance with USP or AAMI guidelines. Sterility Assurance Level shall be 0.000001.

Freedom from pyrogens. The stopcock shall be free from pyrogens when tested in accordance with the USP. As an alternate to the USP Pyrogen Test, the USP Bacterial Endotoxin Test (LAL) may be used.

Instructions for use. A detailed instruction sheet for proper use of the stopcocks shall be provided with each individual stopcock or with each unit package.

Workmanship. The Luer tapers and rotating plug shall be free from parting lines. The stopcock shall be free from flash, pitting, cracks, holes or any foreign matter. The stopcock shall be free from any defects which affect its appearance or utility.

Unit. Package (PG). One package containing fifty individually packaged sterile stopcocks, with instructions, as specified, constitutes one unit. The individual package shall be a sealed, peel-open type container capable of maintaining sterility of contents unless the package is damaged or opened.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one stopcock. Sampling shall be Inspection level S-4. A test failure shall be cause for rejection.

Clear passage of fluid. Each of the four fluid paths as shown in Figure 2, shall be tested using water or another suitable test fluid. Test fluid shall be applied to the fluid path at a pressure of 3-1/2 ± 1/2 psig and shall pass freely through all of the ports within 3 seconds of application utilizing the gages specified in ISO Standard 594.

Leakage. The stopcock shall be tested for leakage in accordance with ISO Standard 594. As an alternate, the testing may consist of an pneumatic circuit equivalent to ISO Standard 594 except that air shall be applied at a pressure of 10 psi. Any leakage shall be a test failure.

Security of assembly. The stopcock body shall be secured. A 25 lb. axial force shall be applied to the rotating plug arm for one (1) minute. Any stopcock which breaks or in which any component separates shall be considered a test failure.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Contractor Certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered material. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

NOTE 1: The following National Stock Number is covered by this document:

NSN	Item Identification
6515-00-926-9195	STOPCOCK, Intravenous Therapy, 3 way, Plastic, Disposable, 50s.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

NOTE 2: Copies of ISO Standards 594/1 and 594/2 may be obtained through the American National Standards Institute (ANSI), 11 West 42nd Street, New York, NY 10036.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5387


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

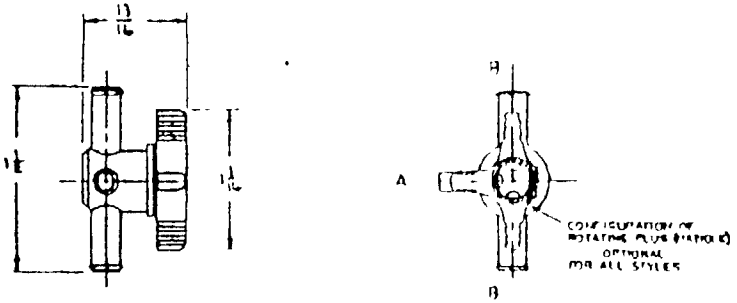


STYLE 1

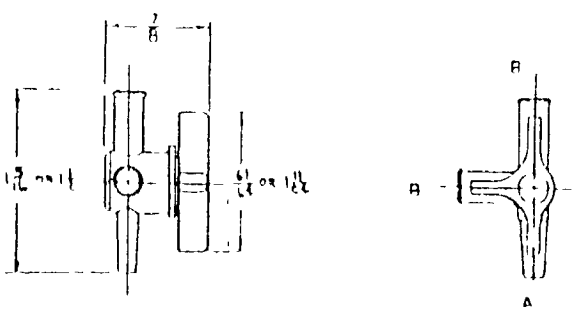

STYLE 2

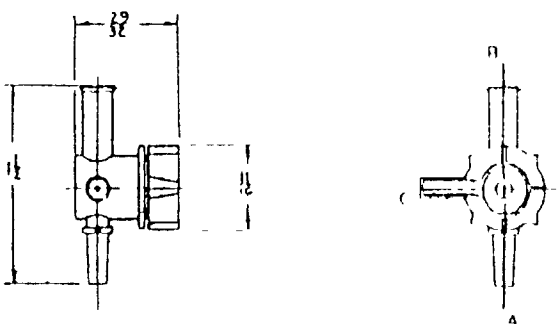

STYLE 3

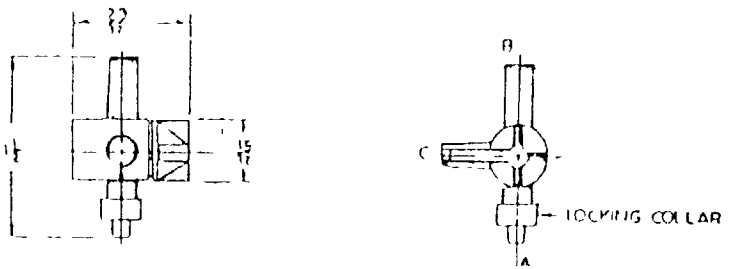

STYLE 4

NOTES.

A MALE LUER SLIP CONE (NOZZLE) CONNECTOR IN ACCORDANCE WITH ISO STANDARD 594

B FEMALE CONE (SOCKET) LUER LOCK CONNECTOR IN ACCORDANCE WITH ISO STANDARD 594.


C FEMALE CONE (SOCKET) LUER SLIP CONNECTOR IN ACCORDANCE WITH ISO STANDARD 594

ALL OUTLINE DIMENSIONS SHOWN ARE FOR REFERENCE PURPOSES ONLY, AND ARE IN INCHES

NSN 6515 00 726 7195

FIGURE 1 STOPCOCK, INTRAVENOUS, THERAPY

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

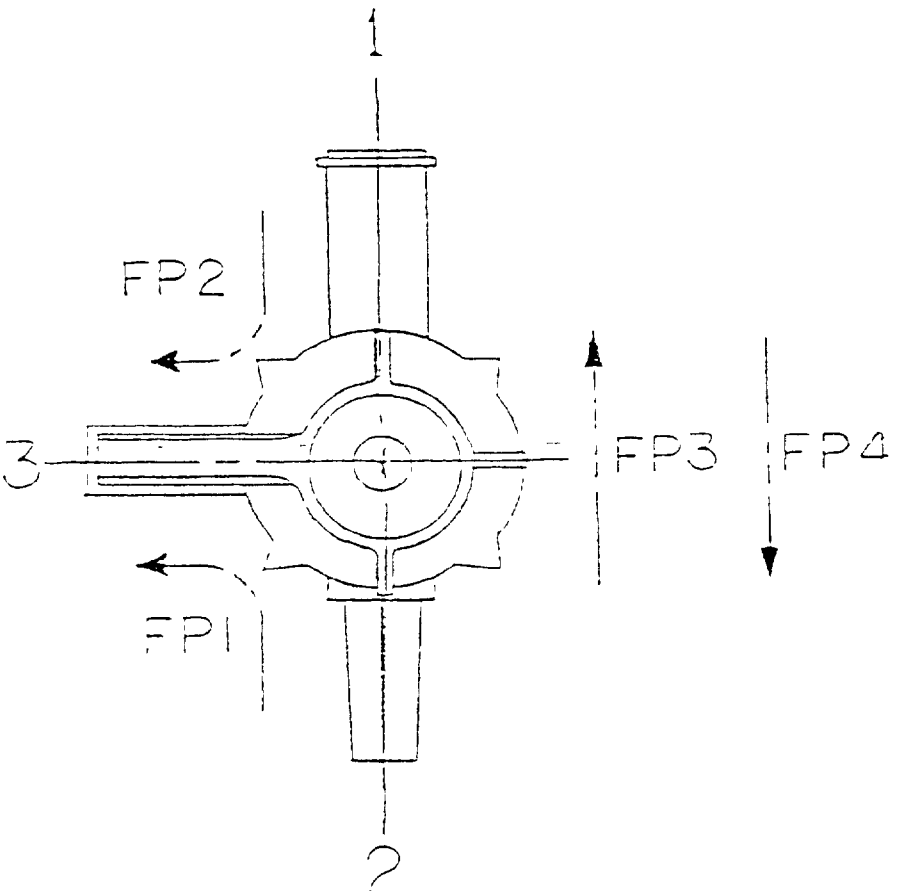

NSN 5E 1E-00-926-9 195

FIGURE 2 FLUID PATHS OF STOPCOCK

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54686	8 January 1993

3. DOCUMENT TITLE
STOPCOCK, INTRAVENOUS THERAPY

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON
c. ADDRESS (Include Zip Code)	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous editions are obsolete — 198/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.