INCH-POUND

A-A-54814
12 February 1993

COMMERCIAL ITEM DESCRIPTION

MASK, ORONASAL, Plastic, Disposable

The General Service Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-M-37553 which is cancelled.

This Commercial Item Description covers one type of disposable, plastic oronasal mask with tube and inlet connector for the purpose of administrating oxygen.

Salient Characteristic.

General. The mask shall consist of essentially five components, that is the facepiece, turret tubing connector, tubing, nipple connector and the elastic strap. The facepiece shall be made of pliable plastic with a rotatable turret tubing connector attached. The tubing connector shall be permanently attached to a length plastic tubing not less than 60 inches. The other end of the tubing shall have a female connector for attachment to the standard nipple of a regulator from an oxygen supply. An adjustable elastic head band shall be used to hold the mask to wearer's head without aid.

Material. Plastic used for the facepiece shall be transparent or translucent flexible polyethylene. The turret and the female connector shall be made of rigid polyvinyl chloride. The tubing shall be made of medical grade polyvinyl chloride.

Style, design and dimensions. The complete mask shall be in accordance with Figures 1 and 2 for style, design and dimensions.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Mask. The mask shall be designed to be usable on a wide variety of facial shapes, and sizes and to cover the oronasal area to the chin or under the chin, not just below the lower lip. A plastic tubing connector shall be present on the mask at a location corresponding to the zone beneath the nose and near the mouth of the wearer. An exhaust port about one half inch in diameter shall be present in the mask or as an alternate, six 1/8 inch diameter holes shall be placed in a circle on each side of the mask.

Tubing. The tubing shall have a minimum tensile strength of 1900 pounds per square inch (psi) and ultimate elongation of 225 percent when tested in accordance with ASTM D-412 test method.

Elastic headband. The free end of the band shall be either dipped in rubber cement, or have shoelace type ends to prevent fraying.

Security of mask-tube assembly. The tubing attachment to the mask shall not come apart with a minimum of two pound pull test.

Workmanship. The mask shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG) One package containing fifty individually packaged masks, as specified, constitutes one unit. The individual package of masks shall be a suitable container capable of maintaining cleanliness of contents until manually opened. Complete and detailed instructions for use shall be supplied with each unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in specification where such inspection are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one one mask as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one mask. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-00-888-6122	MASK, ORONASAL, Plastic, Disposable, 50s

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5436
Location: c:\word\seto\maskcid1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

FIGURE 1. MASK, OXYGEN, PASTIC, DISPOSABLE

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:38Z
Check the source to verify that this is the currentversion before use.

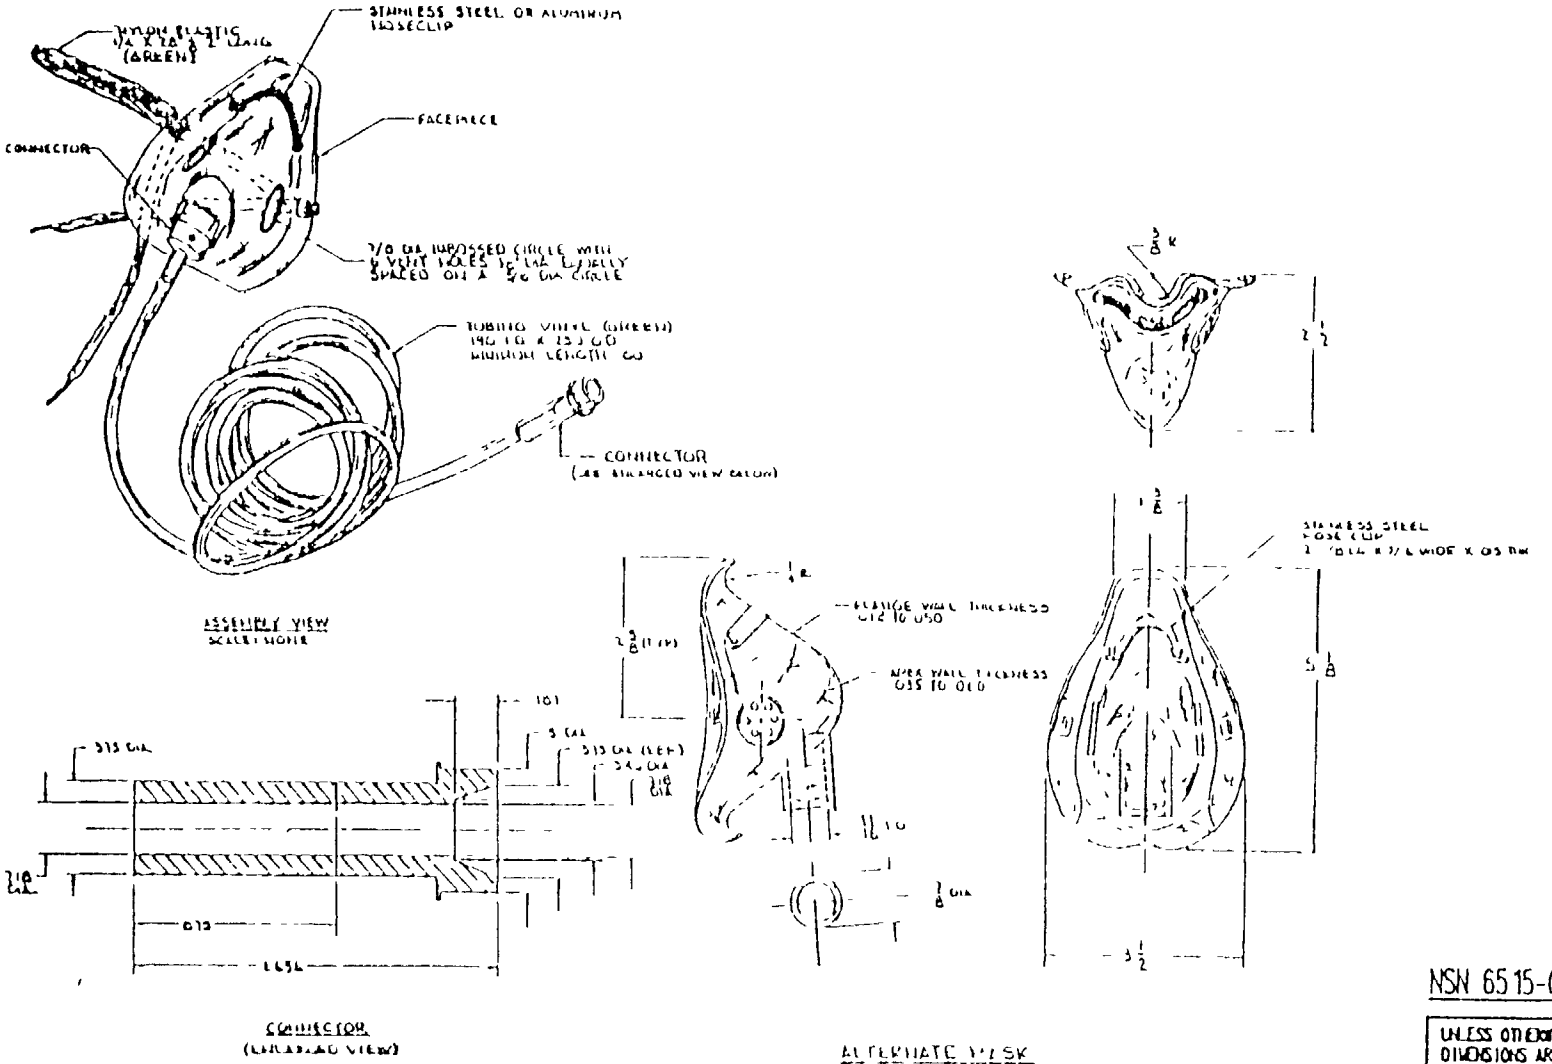

CONNECTOR
(EXPANDED VIEW)

NSN 6515-00-888-6122

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ON:	
FRACTIONS	
UNDER 1"	± 1/16
1" AND OVER	± 1/8
DECIMALS	
.X	± .1
.XX	± .02
.XXX	± .005

FIGURE 2 MASK, OXYGEN, PLASTIC, DISPOSABLE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
	A-A-54814	12 February 1993

3 DOCUMENT TITLE

MASK, ORONASAL, Plastic, Disposable

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)
	e DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial / (2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215)7372870 / 444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403 Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous editions are obsolete — 198/29

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.