INCH-POUND

A-A-54815
26 February 1993

COMMERCIAL ITEM DESCRIPTION

RETRACTOR, NERVE ROOT, HOLSHER

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-R-42010A which is cancelled.

This Commercial Item Description covers two sizes of nerve root retractors suitable for use during neurosurgical operating procedures.

Salient characteristics:

General. The nerve root retractor shall be of the Holsher design and suitable for use in neurosurgical and orthopedic spinal surgical procedures. The retractor shall be of the following sizes:

SIZE	DESCRIPTION
1	7 mm Tip
2	13 mm Tip

Material. The nerve root retractor shall be fabricated from class 4 martensitic corrosion-resistant steel in accordance with ASTM F899. As an alternate, the retractor handle shall be manufactured from class 3 austenitic corrosion-resistant steel in accordance with ASTM F899.

Hardness. The nerve root retractor shall have a Rockwell hardness (HRC) 38 to 45 for class 4 material and a Rockwell hardness (HRB) 80 to 95 for class 3 (alternate) material when tested for hardness in accordance with ASTM E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM E140.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:38Z
Check the source to verify that this is the current version before use.

Style, design and dimensions. The nerve root retractor shall be in accordance with Figure 1 for style, design and dimensions.

Finish. The nerve root retractor shall have a mirror, satin, or matte finish.

Passivation. The nerve root retractor shall be properly passivated.

Corrosion resistance. The nerve root retractor shall show no evidence of corrosion plating or copper when tested for corrosion resistance in accordance with ASTM F1089.

Identification marking. The nerve root retractor shall be legibly marked with contractor's name or registered trademark, and the work "stainless". Foreign manufactured retractors shall bear the name of the country of origin.

Workmanship. The nerve root retractor shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One nerve root retractor, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 1.0 (percent defective) and an inspection level of II. The unit of product for test purposes shall be one nerve root retractor.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests (dimensional) shall be conducted in accordance with MIL-STD-105, with an AQL of 1.0 (percent defective) and an inspection level of S-2. The unit of product for test purposes shall be one nerve root retractor.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor Certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered material. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NSN	Item Identification	Size
6515-01-164-8856	RETRACTOR, NERVE ROOT, HOLSHER, 8-1/2 Inches Long, 1/4 Inch Tip.	1
6515-01-164-8855	RETRACTOR, NERVE ROOT, HOLSHER, 8-1/2 Inches Long, 1/2 Inch Tip.	2

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:38Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5241

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

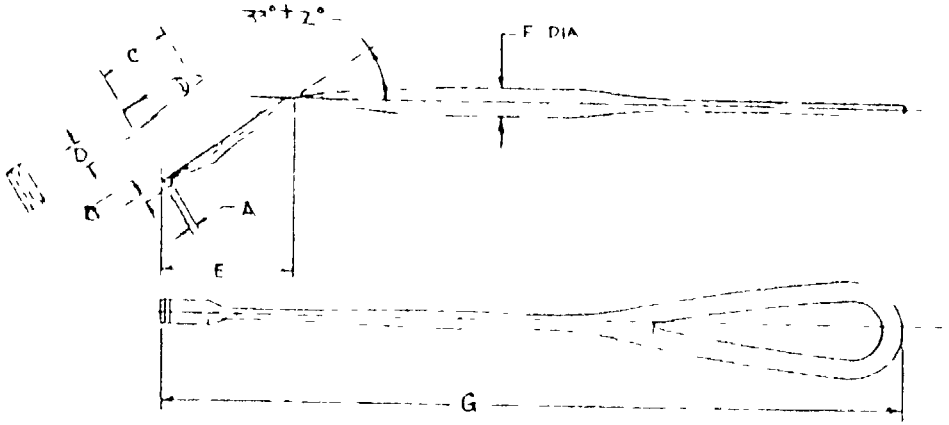

NSN	SIZE	A	B	C	D	E (cm)	F	G (cm)
6515-01-164-8856	1	1 10	4 50	25 40	7 0	4 5	4 8	21 5
6515-01-164-8855	2	1 10	7 00	28 57	13 0	4 5	4 8	21 5
TOLERANCE		± 0 25	± 0 25	± 0 25	± 0 8	± 0 3cm	± 0 8	± 0 6cm

NOTE

1 AS AN ALTERNATE THE SHANK OF THE RETRACTOR MAY BE ROUND OR OCTAGONAL.

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN MILLIMETERS

FIGURE 1 RETRACTOR, NERVE ROOT, HOLSHER

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER: A-A-54815	2. DOCUMENT DATE (YYMMDD): 26 February 1993

3. DOCUMENT TITLE: RETRACTOR, NERVE ROOT, HOLSHER

4. NATURE OF CHANGE (*Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.*)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. [illegible]	b. ORGANIZATION
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable) 7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON
c. ADDRESS (Include Zip Code)	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous editions are obsolete. 190

Source: https://assist.dla.mil - Downloaded: 2020-10-26T09:38Z
Check the source to verify that this is the current version before use.