INCH-POUND

A-A-54827
12 April 1993

COMMERCIAL ITEM DESCRIPTION

NEEDLE, BIOPSY, DISPOSABLE

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-N-36930, which is cancelled.

This Commercial Item Description covers a sterile, disposable biopsy needle with a 20 mm specimen notch in this obturator.

Salient characteristics:

General. The needle shall consist of a cannula, obturator and a protective needle sheath.

Material. The cannula and obturator shall be fabricated from Class 3 Type 304 stainless steel in accordance with ASTM F899. The cannula hub and the obturator hub shall be fabricated from rigid plastic. The protective sheath shall be fabricated from semi-transparent flexible plastic.

Style and design. The biopsy needles shall be suitable for obtaining biopsy samples. The cannula shall be a 14 gauge needle designed to fit and reciprocate within the cannula. The style, design and dimensions shall be in accordance with Figures 1 and 2.

Non toxic, pyrogen-free and sterile. The needle shall be non toxic and pyrogen free when tested in accordance with United States Pharmacopeia (USP). The needle shall be tested for sterility in accordance with USP or AAMI requirements. Sterility assurance level shall be 0.0001.

Workmanship. The needle shall be free from defects which detract from its appearance or impair its serviceability.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Unit. Each (EA). One needle, packaged in a suitable peel-open type container capable of maintaining the sterility of contents unless package is damaged or opened, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one needle as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one needle. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commerical Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

NOTE: The following National Stock Numbers and their respective Item Identifications are covered by this document:

National Stock Numbers	Item Identifications
6515-00-104-8390	NEEDLE, BIOPSY, DISPOSABLE, 14 gauge, 6 inch
6515-00-487-6781	NEEDLE, BIOPSY, DISPOSABLE, 14 gauge, 4-1/2 inch

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:39Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS

Document No. 6015-5507
Location: C:\MIL-STD\FILE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

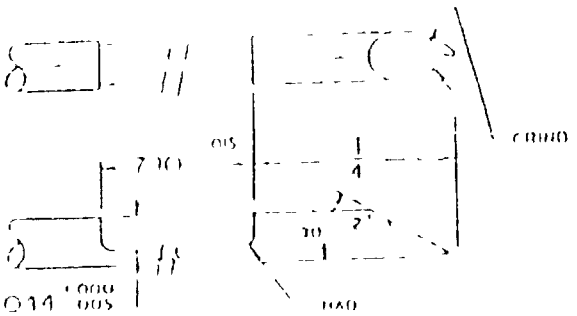


OBTURATOR TIP DETAIL

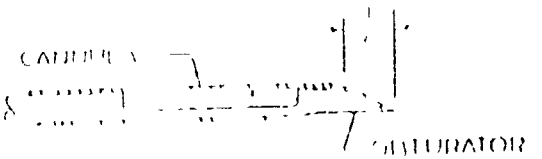

DETAIL F

ENLARGED VIEW OF TIP OF BIOPSY NEEDLE SHOWING OBTURATOR IN FULLY RETRACTED POSITION

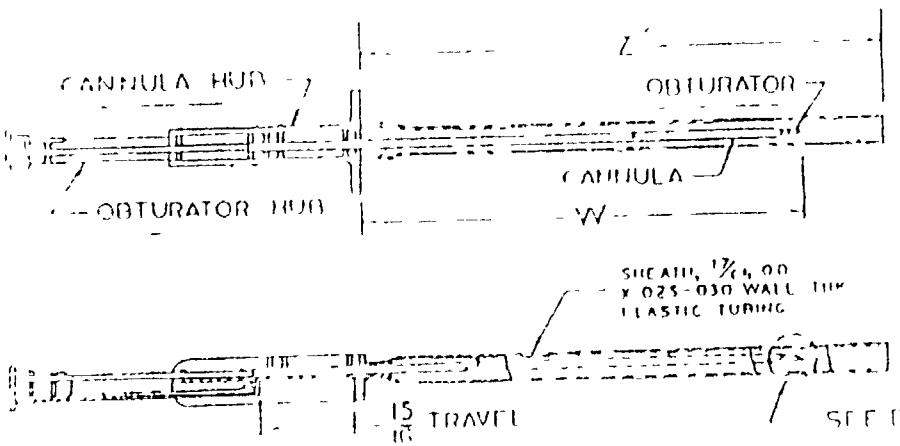

BIOPSY NEEDLE ASSEMBLY

SCHEDULE OF DIMENSIONS


NSN	SIZE	DIM W	DIM X	DIM Y	DIM Z
6515 00 304 8300	6"	6 1/8	2 11/16 ± 1/32	7 3/16 ± 1/32	7 1/2
6515 00 487 8282	4 1/2"	4 1/2 - 1/8	2 1/4 ± 1/32	5 1/16 - 1/32	6

NOTES


1. UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES AND TOLERANCES ON FRACTIONS SHALL BE ± 1/64.
2. TOLERANCES ON DIMENSIONS MARKED NOMINAL SHALL BE IN ACCORDANCE WITH ACCEPTED COMMERCIAL PRACTICE.
3. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY SYMMETRY, AND FIRST QUALITY WORKMANSHIP.


FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T09:39Z
Check the source to verify that this is the current version before use.

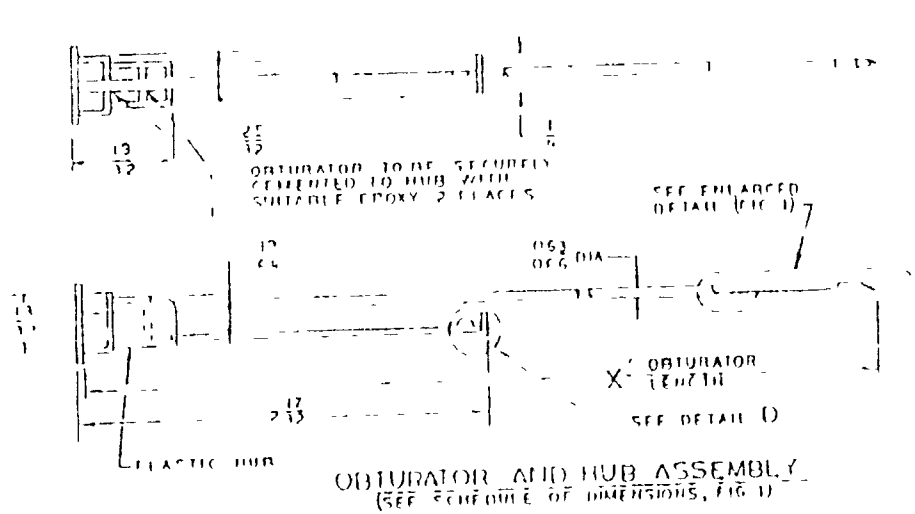



OBTURATOR AND HUB ASSEMBLY
(SEE SCHEDULE OF DIMENSIONS, FIG 1)




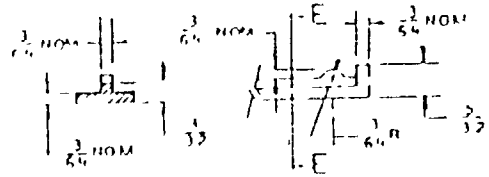


SECTION E-E DETAIL D

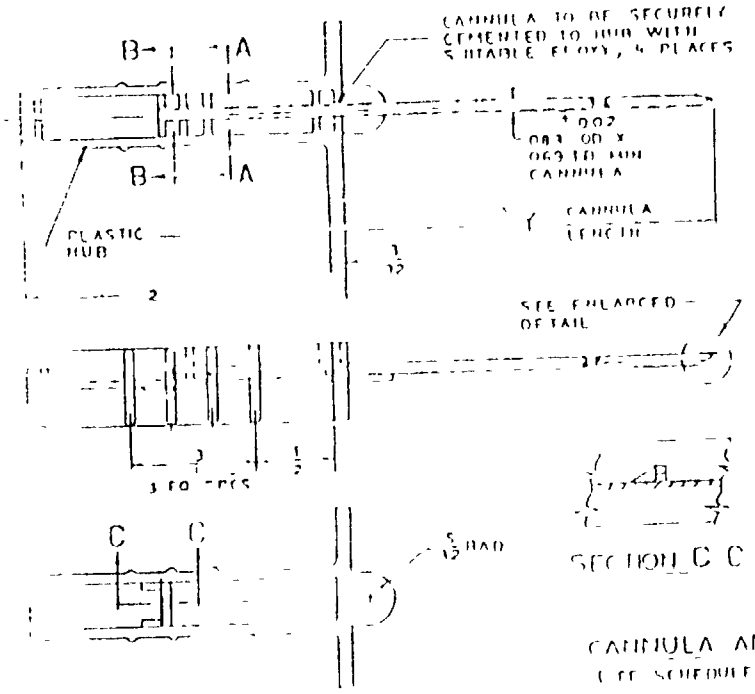




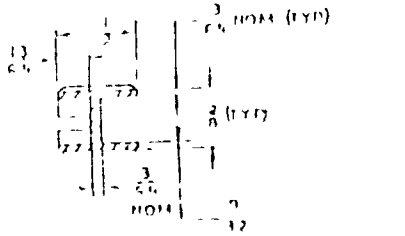

SECTION A-A (TYP 3 PLCS)



SECTION B-B

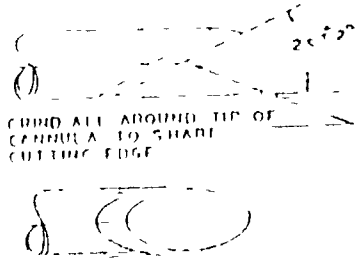

CANNULA TIP DETAIL

SECTION C C

CANNULA AND HUB ASSEMBLY
(SEE SCHEDULE OF DIMENSIONS FIG 1)

FIGURE 2

A-A-54827

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54827	12 April 1992

3. DOCUMENT TITLE

NEEDLE, BIOPSY, DISPOSABLE

4. NATURE OF CHANGE (*Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.*)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215)7372670	444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 *Previous editions are obsolete* 1982/1

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:39Z
Check the source to verify that this is the current version before use.