INCH-POUND

A-A-54828
12 March 1993

COMMERCIAL ITEM DESCRIPTION

SYRINGE, HYPODERMIC,
Angiographic Injector

The General Services Administration has authorized the use of this Commercial Item Description.

This Commercial Item Description covers a sterile, disposable 130 milliliter (ml) syringe for use during angiographic procedures.

Salient characteristics:

Material. The syringe barrel and plunger shall be fabricated from polypropylene which meets the United States Pharmaceutical (USP) requirements for Class IV plastics. The interior of the barrel shall be lightly coated with an inert pharmaceutical or medical grade silicone lubricant. The plunger tip shall be fabricated from a pharmaceutical grade rubber or neoprene which meets the USP requirements for Elastomeric Closures for Injections.

Style, design and dimension. The syringe shall have a Luer slip tip in accordance with ISO 594. The hub of the syringe shall have a Luer lock nut of the Linden Design which is proximal to the tip, 3/4 ± 1/16 inch in length, and suitable for accepting and securing in place, by means of a push and turn motion, the proximal nubbed end of catheter, needle or connector tube used during angiographic procedures.

The inside of the barrel shall have a smooth, uniform surface, free from pits, grind marks, bubbles, flash or other imperfections. The plunger shall glide freely through the barrel while maintaining a fluid-tight fit. The plunger tip and barrel shall both be beveled and form a flush fit at zero volume. The barrel shall be transparent and the plunger tip shall have two visible rings touching the sides of the barrel.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

The style, design and dimension shall be in accordance with Figure 1.

Leakage test. The water pressure test system shall have a water pressure gauge and rubber plug. A needle shall be secured to the Luer tip of the syringe by applying it with a 5 pound axial force and while maintaining this compressive stress twisting the needle hub 45 degrees relative to the Luer tip. The needle of the hypodermic shall be inserted into the plug. The syringe shall be tested for liquid leakage at the syringe piston and syringe nozzle under compression and during aspiration in accordance with ISO 7886.

Sterility, pyrogenicity, toxicity. The syringe shall be nonpyrogenic and nontoxic in accordance with the USP. The syringe shall be sterile in accordance with USP or Association for the Advancement of Medical Instrumentation (AAMI) requirements. Sterility assurance level shall be 0.0001.

Workmanship. The syringe shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing fifty individually packaged sterile syringes, as specified, constitutes one unit. The individual package shall be a sealed peel-open type container capable of maintaining sterility of contents unless the package is damaged or opened.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspection are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one syringe as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one syringe. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-01-023-0929	SYRINGE, HYPODERMIC, Angiographic Injector, Disposable, 130 ml, 50's

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5523
Location: c:\word\doc\levin\syrin2cd

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

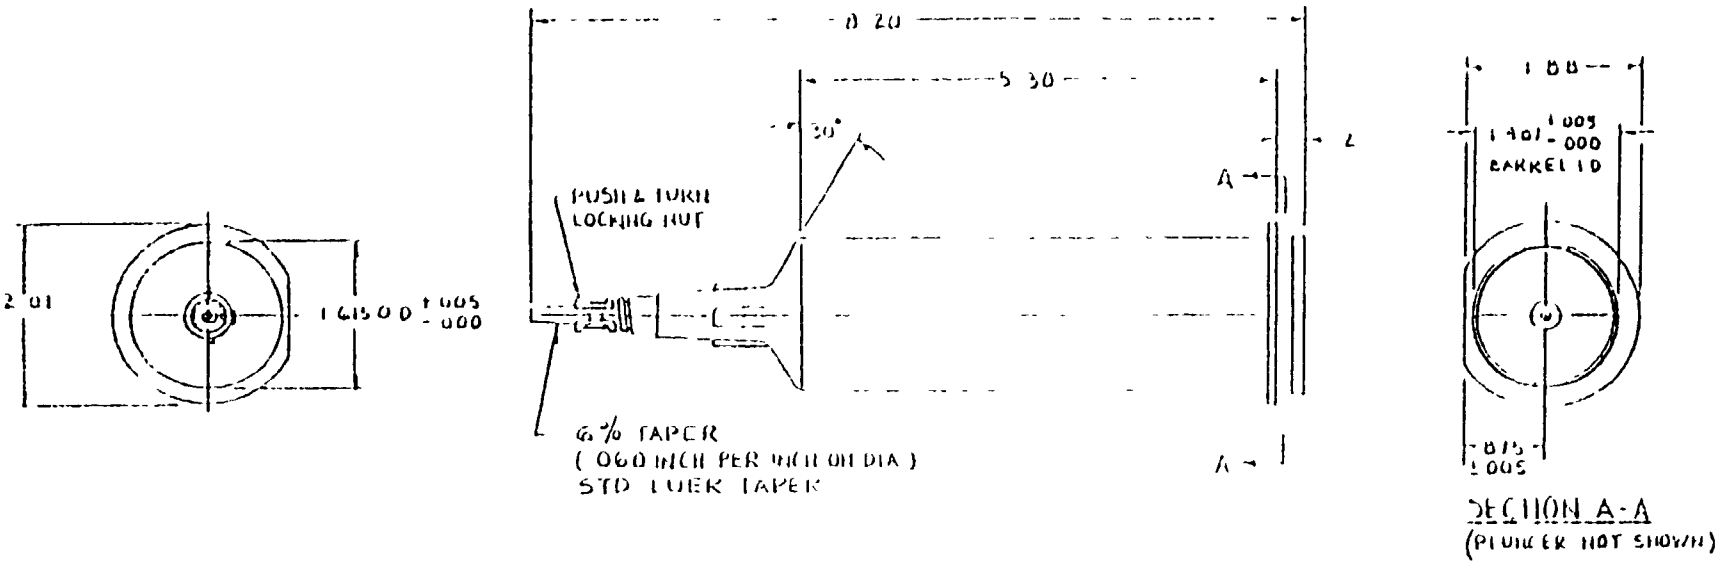

NSN 6515-01-023-0929

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
±	± .01	± 0° 31'

4-A-54525

FIGURE 1 SYRINGE, HYPODERMIC, ANGIOGRAPHIC INJECTOR

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
	A-A-51630A	12 March 1993

3 DOCUMENT TITLE

BLOOD SAMPLE, COLLECTING SET

4 NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)*

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code)	
Defense Personnel Support Center ATTN: DPSC-MSE	(1) Commercial (215)7372870	(2) AUTOVON 444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403 Falls Church VA 22041 3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.