INCH-POUND

A-A-54835/2
8 October 1993

COMMERCIAL ITEM DESCRIPTION

RONGEUR, KERRISON,
40 Degree Upbite

The General Services Administration has authorized the use of this Commercial Item Description Sheet.

The complete requirements for procuring Kerrison rongeurs shall consist of this document and the issue in effect of Commercial Item Description A-A-54835.

Salient characteristics:

Style, design and dimensions. This specification covers the following style and class of Kerrison rongeur:

Style II - 40 degrees upbite

Class 1 - 8 inch shaft

The rongeur shall be in accordance with Figure 1.

Notes:

1. Intended use: Rongeurs of the Kerrison design covered in this Commercial Item Description Sheet are intended to be used in laminectomy procedures.

2. Copies of Commercial Item Description A-A-54835 may be obtained by writing the Defense Printing Service Detachment Office; Bldg 4D; DoD-SSP; 700 Robbins Avenue; Philadelphia, PA; 19222-5094.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

3. National Stock Numbers, Item Identifications and Classes:

National Stock Number	Item Identifications	Class
6515-01-139-8264	RONGEUR, KERRISON, 3 mm 40 Degree Upbite, 8 inch Straight Shaft	1
6515-01-139-8265	RONGEUR, KERRISON, 5 mm 40 Degree Upbite, 8 inch Straight Shaft	1

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5615
Location: c:\word\doc\david\rongeur2\sg

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

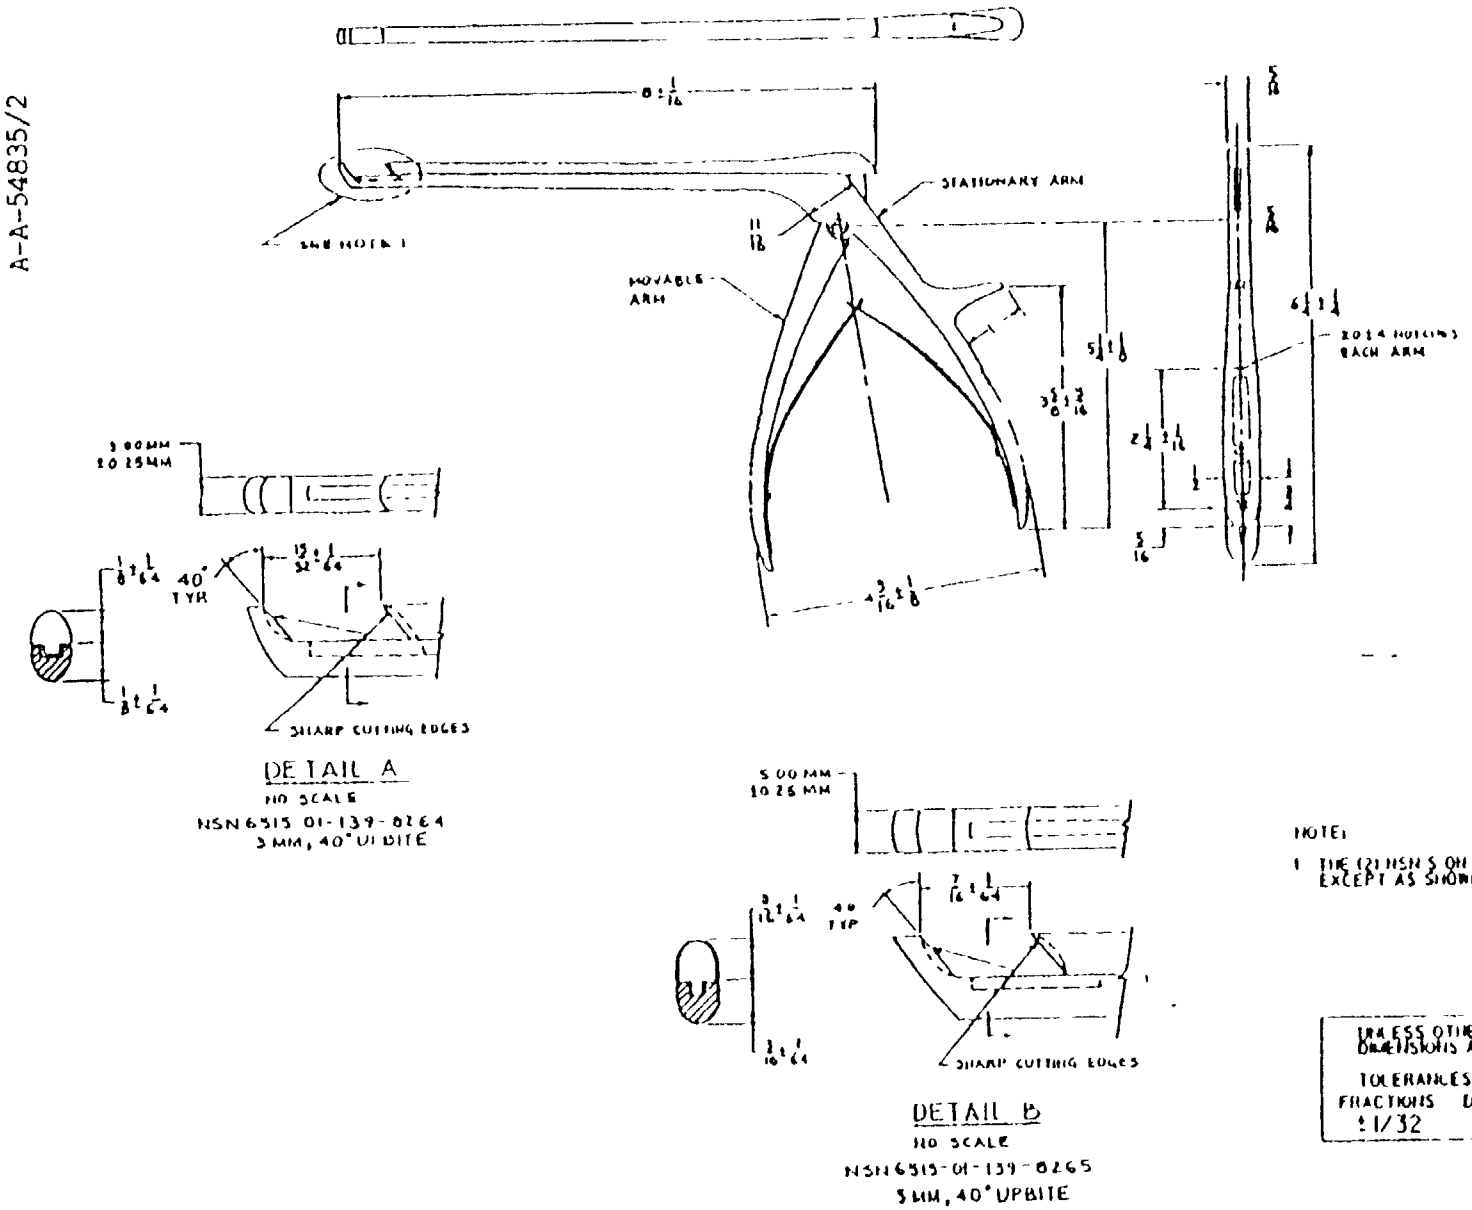


FIGURE 1 RONGEUR, KERRISON, 8 INCH

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54835/2	2 DOCUMENT DATE (YYMMDD) 931008

3 DOCUMENT TITLE
RONGEUR, KERRISON, 40 Degree Upbite

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)

5 REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a NAME Defense Personnel Support Center ATTN: DPSC-MSE	b TELEPHONE (Include Area Code) (1) Commercial (215)7372870	(2) AUTOVON 444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.