INCH-POUND

A-A-54837
12 April 1993

COMMERCIAL ITEM DESCRIPTION

SYRINGE, IRRIGATING, Glass

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Federal Specification GG-S-931, which is cancelled.

This Commercial Item Description covers a bulb type glass irrigating syringes.

Salient characteristics:

Classification. The syringe shall be of the following types:

TYPE I - Tapered Tip
TYPE II - Cone Tip (rubber)
TYPE III - Tapered Tip with removable tip

Material. The syringe shall be fabricated from borosilicate glass. The bulb and removable tip shall be fabricated from inert medical grade rubber or inert medical grade neoprene.

Style and design. All the syringes shall be a bulb-type with a glass barrel. The Type I syringe shall have tapered glass tip. The Type II syringe shall have a rubber cone tip. The Type III syringe shall have a tapered glass tip with a removable rubber tip. The bulb shall form a leakproof seal with the syringe barrel. The bulb shall be capable of repeated sterilizations without any determental effects. The bulb shall be easily compressed and shall return to its original configuration without any permanent distortion. The style and design of the syringe shall be in accordance with Figure 1. Each syringe shall be packaged in an individual container that shall protect the syringe during shipment and storage.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Marking. The capacity and the manufacturer's name or registered trademark shall be permanently marked on the syringe.

Workmanship. The syringe shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One syringe of the type and ounce specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one syringe as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one syringe. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commerical Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

NOTE: The following National Stock Numbers and their respective Item Identifications is covered by this document:

NATIONAL STOCK NUMBERS	ITEM IDENTIFICATIONS	TYPES
6515-00-379-4200	SYRINGE, IRRIGATING, Glass, 1/2 ounce	I
6515-00-379-4300	SYRINGE, IRRIGATING, Glass, 1 ounce	I
6515-00-379-4400	SYRINGE, IRRIGATING, Glass, 3 ounce	I
6515-00-379-5600	SYRINGE, IRRIGATING, Ear, Glass, 1 ounce	II
6515-00-379-6820	SYRINGE, IRRIGATING, Glass, 4 ounce	III

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS


Project No. 6515-5554
Location: C:\MARK\SYRINGE3\D

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

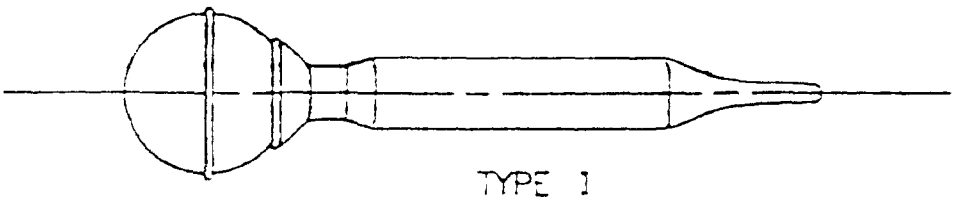


TYPE I

NSN 6515-00-379-4200
6515-00-379-4300
6515-00-379-4400

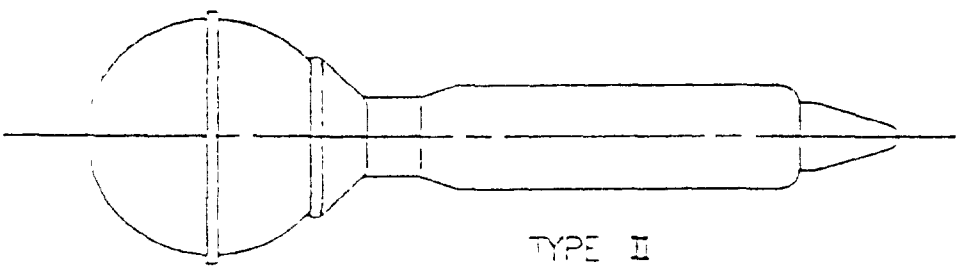

TYPE II

NSN 6515-00-379-5600

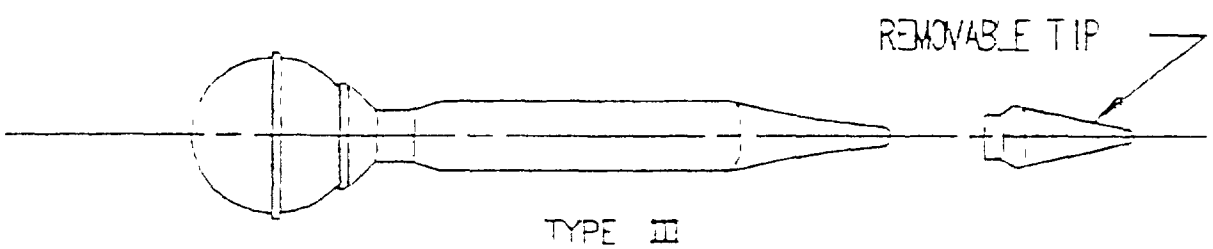

TYPE III

NSN 6515-00-379-6820

FIGURE 1 SYRINGE, GLASS, WITH BULB

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

RECOMMEND A CHANGE:	1. DOCUMENT NUMBER: A-A-54837	2. DOCUMENT DATE (YYMMDD): 12 April 1993

3. DOCUMENT TITLE: SYRINGE, IRRIGATING, Glass

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	c. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	d. DATE SUBMITTED (YYMMDD)

7. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215)7372870	444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.