MILITARY SPECIFICATION

CONNECTORS, ELECTRICAL, PLUGS, TIP (TEST POINT PLUG, BANANA PLUG) GENERAL SPECIFICATION FOR


This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers the general requirements for test point plugs and banana plugs for use in electrical and electronic equipment. (See 6.1.) As used in this specification, the term "connectors" shall include test point plugs and banana plugs.

1.2 Classification. Connectors covered by this specification shall be single-contact or multiple-contact connectors, as specified (see 3.1).

1.2.1 Military part number. The military part number shall consist of the letter "M", the basic number of the specification sheet, and an assigned dash number (see 3.1), as shown in the following:



2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

L-P-394	- Plastic Molding Material, Polypropylene, Injection and Extrusion
L-P-410	- Plastic, Polyamide (Nylon), Rigid: Rods, Tubes, Flats, Molded and Cast Parts.
L-P-1183	- Plastic Molding Material, Acrylonitrile-butadiene-styrene (Abs) Rigid
QQ-B-750	- Bronze, Phosphor; Bar, Plate, Rod, Sheet, Strip, Flat Wire, and Structural and Special Shaped Sections.
QQ-C-530	- Copper-Beryllium Alloy Bar, Rod and Wire (Copper Alloy Number 172).
QQ-C-533	- Copper-Beryllium Alloy Strip, (Copper Alloy Numbers 170 and 172).
QQ-N-290	- Nickel Plating (Eletrodeposited).
QQ-P-35	- Passivation Treatments for Austenitic, Ferritic, and Martensitic Corrosion-Resisting Steel (Fastening Devices).

MILITARY

MIL-M-14	- Molding Plastics and Molded Plastic Parts, Thermosetting.
MIL-T-10727	- Tin Plating; Electrodeposited or Hot-Dipped, for Ferrous and Nonferrous Metals.
MIL-C-14550	- Copper Plating, (Electrodeposited).
MIL-I-17214	- Indicator, Permeability; Low-Mu (Go -No Go).
MIL-P-19468	- Plastic Rods, Polytetrafluoroethylene, Molded and Extruded.
MIL-P-19833	- Plastic Molding Material and Plastic Molded Parts, Glass Fiber Filled, Diallyl Phthalate Resin.
MIL-C-39024	- Connector, Electrical, Jacks, Tip (Test Point, Panel or Printed Wiring Type), General Specification for
MIL-G-45204	- Gold Plating, Electrodeposited.
MIL-C-45662	- Calibration System Requirements.
MIL-C-55330	- Connectors, Preparation for Delivery of.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Commander, Naval Electronic Systems Command, ATTN: ELEX 5043, Department of the Navy, Washington, DC 20360, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

(See Supplement 1 for list of associated specification sheets.)

STANDARDS

FEDERAL

FED-STD-H28 - Screw Thread Standards for Federal Services
FED-STD-406 - Plastic, Methods of Testing.
FED-STD-595 - Colors.

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-202 - Test Methods for Electronic and Electrical Component Parts.
MIL-STD-889 - Dissimilar Metals.
MIL-STD-1344 - Test Methods for Electrical Connectors.

(Copies of specifications, standards, drawings, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Specification sheets. The individual item requirements shall be as specified herein and in accordance with the applicable specification sheets. In the event of any conflict between requirements of this specification and the specification sheets, the latter shall govern.

3.2 First article. Connectors furnished under this specification shall be products which have passed the first article inspection of 4.4 (see 6.3).

3.3 Materials. Materials shall be as specified herein; however, when a definite material is not specified, a material shall be used which will enable the connectors to meet the performance requirements of this specification. Acceptance or approval of any constituent material shall not be construed as a guaranty of the acceptance of the finished product.

3.3.1 Metal parts.

3.3.1.1 Nonmagnetic materials. All parts shall be made from materials which are classed as nonmagnetic.

3.3.1.2 Dissimilar metals. Where dissimilar metals are used in intimate contact with each other protection against electrolysis and corrosion shall be provided. Dissimilar metals shall be as defined in MIL-STD-889. Dissimilar metals such as brass, copper, or steel (except corrosion-resisting steel, passivated in accordance with QQ-P-35) shall not be used in intimate contact with aluminum or aluminum alloy.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

3.3.1.3 Metals and finishes. All exposed metal parts, except electric contacts, terminals, and corrosion-resisting steel parts shall be nickel-plated in accordance with class 1, type 2, of QQ-N-290. Steel parts shall be passivated in accordance with QQ-P-35.

3.3.1.4 Contacts. Contacts and contact tabs shall be made of copper-beryllium in accordance with QQ-C-530 or QQ-C-533, or (when specified, see 3.1) phosphor bronze per QQ-B-750. Contacts shall be gold plated in accordance with type II, grade C, class 1 of MIL-G-45204. Silver underplate shall not be used.

3.3.1.5 Terminals. Soldering terminals shall be made of a copper alloy material, and shall be gold plated in accordance with type II, grade C, of MIL-G-45204 with an 0.0002-inch minimum thickness underplate of either copper, class 3 of MIL-C-14550, or nickel, or shall be tin plated in accordance with type I of MIL-T-10727, 0.0004-inch thick with an 0.0002-inch minimum thickness underplate of copper in accordance with class 3 of MIL-C-14550. Silver underplate shall not be used.

3.3.2 Plastic parts. Plastic parts shall be made of type GDI-30F of MIL-P-19833, type SDG-F of MIL-M-14, MIL-P-19468, L-P-410, L-P-394 or L-P-1183 unless otherwise specified (see 3.1). The color of the insulated portions shall be black no 17038 or red no 11136 in accordance with FED-STD-595, as specified (see 3.1).

3.3.2.1 Flammability. Plastic materials shall be limited to those certified by their manufacturers as self-extinguishing in accordance with method 2021, 2022, or 2023 of FED-STD-406.

3.3.3 Threaded parts. Screw threads for threaded parts shall conform to FED-STD-H28, and shall be as specified (see 3.1).

3.4 Design, construction, and physical dimensions. Connectors shall be of the design, construction, and physical dimensions specified (see 3.1). Unless otherwise specified (see 3.1), connectors shall have an operating temperature range of -65° to +50°C.

3.4.1 Contacts. Contacts shall be of the design, construction and physical dimensions specified (see 3.1).

3.4.1.1 Contact identification. Contact positions on multiple-contact connectors shall be permanently identified by legible letters or numerals, as specified (see 3.1), molded or stamped on the front and rear face of the connector body. Marking shall be arranged to avoid confusion between contacts.

3.4.1.2 Contact arrangement. The center-to-center distance between contacts shall be as specified (see 3.1).

3.4.1.3 Contact finish. Contact finish shall be smooth, free of shear lines, tear out or scratches, and shall show no signs of porosity or surface cracks.

3.4.1.4 Contact current rating. The current rating of contacts shall be as shown in table I, as specified (see 3.1).

TABLE I. Contact current rating.

Contact diameter	Current rating (maximum)
inch	amperes
.040	3
.080	5
.150 - .170	8

3.4.2 Cable mounting hardware. Screws, clamps, brackets, or similar means for mounting the cable shall be furnished, when specified (see 3.1).

3.5 Performance.

3.5.1 Permeability. When connectors are tested as specified in 4.6.3, the relative magnetic permeability shall be less than 2.0.

3.5.2 Contact resistance. When connectors are tested as specified in 4.6.4, the voltage drop shall be not greater than 20 millivolts, unless otherwise specified (see 3.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

3.5.3 Insulation resistance. When measured as specified in 4.6.5, the insulation resistance shall be 5,000 megohms or greater.

3.5.4 Dielectric withstanding voltage. When tested as specified in 4.6.6, connectors shall withstand the test voltage specified (see 3.1) with no evidence of flashover.

3.5.5 Thermal shock. When tested as specified in 4.6.7, connectors shall show no visual evidence of physical damage.

3.5.6 Shock (specified pulse). When tested as specified in 4.6.8, connectors shall show no visual evidence of mechanical damage, loosening of parts or rupturing of dielectric materials. When specified (see 3.1), there shall be no loss of electrical continuity in excess of 10 microseconds.

3.5.7 Vibration. When connectors are tested as specified in 4.6.9 , there shall be no loss of electrical continuity in excess of 10 microseconds during the test. After the test, connectors shall meet the following requirements:

Visual examination - - - - - - - - - -	There shall be no cracking, breaking, or loosening of parts or other evidence of physical damage.
Contact resistance (when specified see 3.1) - - - - - - - - - - - - - -	Shall be as specified in 3.5.2.

3.5.8 Humidity (steady state). When tested as specified in 4.6.10, connectors shall show no visual evidence of physical damage and the insulation resistance shall exceed 1,000 megohms.

3.5.9 Salt spray (corrosion). When connectors are tested as specified in 4.6.11, there shall be no exposure of the basis metal. After the test, the contact resistance shall be as specified in 3.5.2, unless otherwise specified (see 3.1).

3.6 Identification marking. Connectors shall be marked in accordance with method I of MIL-STD-1285, with the complete part number, manufacturer's name or trademark, and, when specified (see 3.1), the date and source code. Marking shall be located on the connector so that it will be visible after installation, unless this is impossible because of space limitations. In such cases, required marking shall be applied to an envelope, bag, box, or other intermediate container suitable for shelf storage.

3.7 Workmanship. Connectors shall be processed in such a manner as to be uniform in quality and shall be free from pits, cracks, rough edges, and other defects that will affect life, serviceability, or appearance.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Test equipment and inspection facilities. Test and measuring equipment and inspection facilities of sufficient accuracy, quality and quantity to permit performance of the required inspection shall be established and maintained by the contractor. The establishment and maintenance of a calibration system to control the accuracy of the measuring and test equipment shall be in accordance with MIL-C-45662.

4.2 Classification of inspections. The inspections specified herein are classified as follows:

a. First article inspection (see 4.4).
b. Quality conformance inspection (see 4.5).

4.3 Inspection conditions. Unless otherwise specified herein, all inspections shall be performed in accordance with the test conditions specified in the "GENERAL REQUIREMENTS" of MIL-STD-1344.

Source: https://assist.dla.mil -- Downloaded: 202610-20T20:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

4.4 First article inspection. First article inspection shall be performed by the contractor, after award of contract and prior to production, at a location acceptable to the Government. First article inspection shall be performed on sample units which have been produced with equipment and procedures normally used in production. First article approval is valid only on the contract under which it is granted, unless extended by the Government to other contracts.

4.4.1 Sample size. 8 connectors shall be subjected to first article inspection.

4.4.2 Inspection routine. The sample shall be subjected to the inspections specified in table II, in the order shown. All sample units shall be subjected to the inspections of group I. The sample shall then be divided equally into two groups of four units each, and subjected to the inspections for their particular group.

4.4.3 Failures. One or more failures shall be cause for refusal to grant lot approval.

TABLE II. First article inspection.

Examination or test	Requirement paragraph	Test paragraph
Group I (all specimens)		
Visual and mechanical examination	3.1, 3.3, 3.4, 3.6, and 3.7	4.6.2
Permeability	3.5.1	4.6.3
Group II (4 specimens)		
Contact resistance	3.5.2	4.6.4
Insulation resistance	3.5.3	4.6.5
Dielectric withstanding voltage	3.5.4	4.6.6
Salt spray (corrosion)	3.5.9	4.6.11
Visual and mechanical	3.1, 3.3, 3.4, 3.6 and 3.7	4.6.2
Group III (4 specimens)		
Thermal shock	3.5.5	4.6.7
Shock (specified pulse)	3.5.6	4.6.8
Vibration	3.5.7	4.6.9
Humidity (steady state)	3.5.8	4.6.10
Visual and mechanical	3.1, 3.3, 3.4, 3.6 and 3.7	4.6.2

4.5 Quality conformance inspection.

4.5.1 Inspection of product for delivery. Inspection of product for delivery shall consist of groups A and B inspections.

4.5.2 Inspection lot. An inspection lot, as far as practicable, shall consist of all connectors of the same basic type, size, and terminal style (if applicable), produced under essentially the same conditions, and offered for inspection at one time. When a connector has different colors of insulation, an inspection lot may include any quantity and variety of colors provided that the units are otherwise mechanically and dimensionally identical.

4.5.2.1 Group A inspection. Group A inspection shall consist of the examination and test specified in table III, and shall be made on the same set of sample units, in the order shown.

TABLE III. Group A inspection.

Examination or test	Requirement paragraph	Test paragraph	AQL (percent defective)	
			Major	Minor
Visual and mechanical examination	3.1, 3.3, 3.4 3.6, and 3.7	4.6.2	1.0	4.0
Permeability	3.5.1	4.6.3		

4.5.2.1.1 Sampling plan. Statistical sampling and inspection shall be in accordance with MIL-STD-105 for general inspection level II. The acceptable quality level (AQL) shall be as specified in table III. Major and minor defects shall be as defined in MIL-STD-105.

Source: https://assist.dla.mil -- Downloaded: 202640-20T20:53Z
Check the source to verify that this is the currentversion before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

4.5.2.1.2 Rejected lots. If an inspection lot is rejected, the contractor may rework it to correct the defects, or screen out the defective units, and resubmit for reinspection. Resubmitted lots shall be inspected using tightened inspection and shall not thereafter be tendered for acceptance unless the former rejection or requirement of correction is disclosed. Such lots shall be separate from new lots, and shall be clearly identified as reinspected lots.

4.5.2.2 Group B inspection. Group B inspection shall consist of the test specified in table IV, in the order shown, and shall be made on sample units which have been subjected to and have passed group A inspection.

TABLE IV. Group B inspection.

Test	Requirement paragraph	Test paragraph
Contact resistance	3.5.2	4.6.4
Insulation resistance	3.5.3	4.6.5
Dielectric withstanding voltage	3.5.4	4.6.6

4.5.2.2.1 Sampling plan. The sampling plan shall be in accordance with MIL-STD-105 for special inspection level S-4. The sample size shall be based on the inspection lot size from which the sample was selected for group A inspection. The AQL shall be 2.5 percent defective.

4.5.2.2.2 Rejected lots. If an inspection lot is rejected, the contractor may rework it to correct the defects, or screen out the defective units, and resubmit for reinspection. Resubmitted lots shall be inspected using tightened inspection and shall not thereafter be tendered for acceptance unless the former rejection or requirement of correction is disclosed. Such lots shall be separate from new lots, and shall be clearly identified as reinspected lots.

4.5.2.2.3 Disposition of sample units. Sample units which have been subjected to group B inspection shall not be delivered on the contract or purchase order.

4.5.3 Inspection of preparation for delivery. Sample packages and packs and the inspection of the preservation-packaging, packing and marking for shipment and storage shall be in accordance with the requirements of MIL-C-55330.

4.6 Methods of examination and test.

4.6.1 Test point receptacles. Test point receptacles used for test purposes shall be in accordance with MIL-C-39024 or as specified (see 3.1).

4.6.2 Visual and mechanical examination. Connectors shall be examined to verify that the design, construction, physical dimensions, marking, and workmanship are in accordance with the applicable requirements (see 3.1, 3.3, 3.4, 3.6, and 3.7).

4.6.3 Permeability (see 3.5.1). The permeability of all metal parts shall be measured with an indicator conforming to MIL-I-17214.

4.6.4 Contact resistance (see 3.5.2). Connectors shall be tested in accordance with method 307 of MIL-STD-202. The following details and exception shall apply:

a. Method of connection - In accordance with figure 1. Measurements shall be made after the temperature of the wire has stabilized.
b. Test current - As specified in table I.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

c. Points of measurement - Across each mated test probe and connector between the two points indicated "X" "X" on figure 1.
d. Number of activations prior to measurement - Not applicable.
e. Number of test activations - Not applicable.
f. Number of measurements per activation - Not applicable.


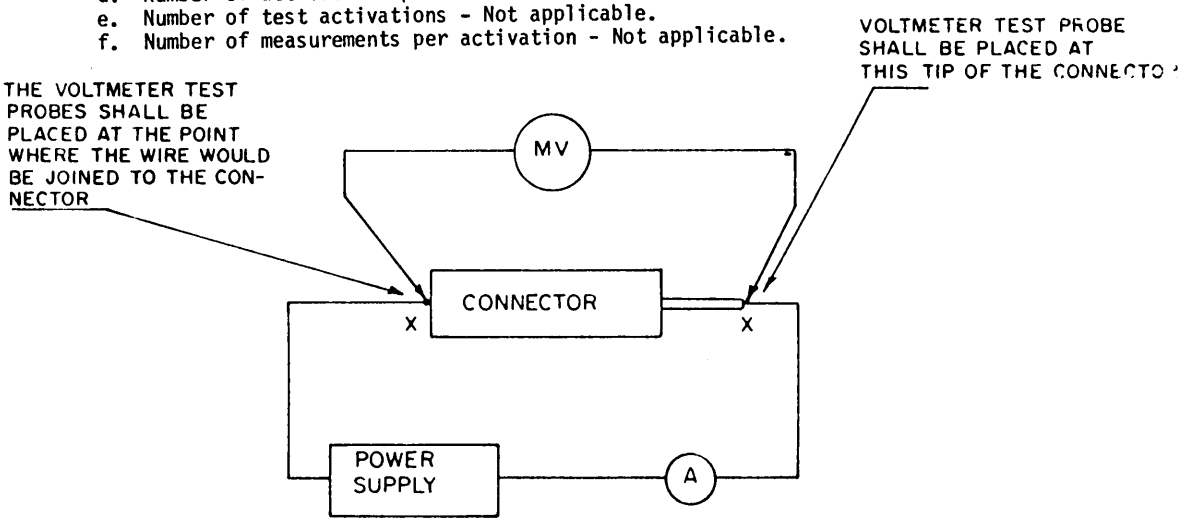


FIGURE 1. Resistance of contacts (potential drop).

4.6.5 Insulation resistance (see 3.5.3). Connectors shall be tested in accordance with method 3003 of MIL-STD-1344 (any number of contacts may be tested simultaneously). The following details and exceptions shall apply:

a. Magnitude of test voltage - 100 volts ±10 percent. On multiple-contact connectors, the voltage shall be applied between all contacts alternately connected.
b. Special conditions - In accordance with figure 2, when specified (see 3.1).
c. Points of measurement - Between all contacts and the panel or test mount, and between all adjacent contacts.
d. Electrification time - Not to exceed 1 minute.
e. Test condition letter - A of method 302, MIL-STD-202.

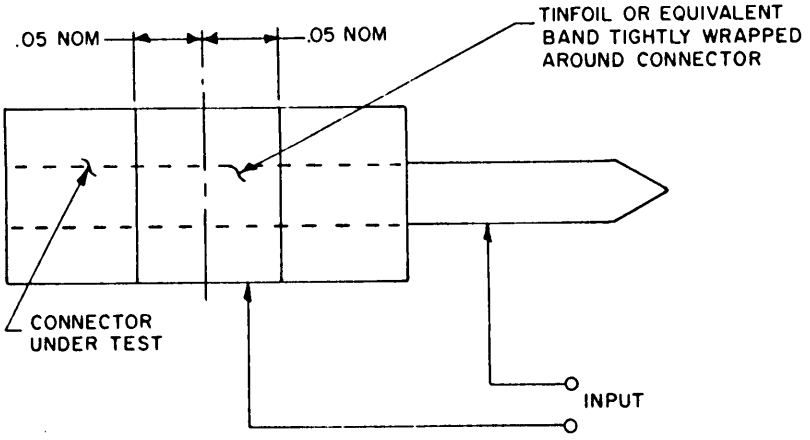

NOTES:
1. Meters, bridges or other apparatus, when required, shall be incorporated in the circuit.
2. Thickness of the conductive band (e.g. tinfoil) shall be such that it can withstand the applied voltage.

FIGURE 2. Test circuit for dielectric withstanding voltage and insulation resistance tests.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

4.6.6 Dielectric withstanding voltage (see 3.5.4). Connectors shall be tested in accordance with method 3001 of MIL-STD-1344. The following details shall apply:

a. Special conditions - In accordance with figure 2, when specified (see 3.1).
b. Magnitude of test voltage - As specified (see 3.1).
c. Duration of application of test voltage - For a period of 1 minute, unless otherwise specified (see 3.1).
d. Points of application of test voltage - Between current-carrying parts and ground, unless otherwise specified (see 3.1). On multiple-contact connectors, the voltage shall be applied between all contacts alternately connected.

4.6.7 Thermal shock (see 3.5.5). Connectors shall be tested in accordance with method 1003 of MIL-STD-1344. The following details shall apply:

a. Test condition letter - B of method 107, MIL-STD-202 (or C, when specified (see 3.1)).
b. Examination after test - Connectors shall be visually examined for evidence of physical damage.

4.6.8 Shock (specified pulse)(see 3.5.6). Connectors, when inserted into the approved mating connector (see 3.1) shall be tested in accordance with method 2004 of MIL-STD-1344. The following details and exception shall apply:

a. Mounting method - By normal mounting means (see 4.6.1).
b. Test condition letter - I of method 213, MIL-STD-202.
c. Measurements during shock test - Connectors shall be monitored for electrical continuity both during and after the test. Loss of continuity for a period of longer than 10 microseconds constitutes a failure. All wiring shall be in accordance with 4.6.1.

4.6.9 Vibration (see 3.5.7). Connectors shall be tested in accordance with method 2005 of MIL-STD-1344. The following details shall apply:

a. Test condition number I.
b. Measurement during test - Connectors shall be monitored for electrical continuity during the test. Equipment shall be sufficiently sensitive to detect any interruption with a duration of 10 microseconds.
c. Tests after vibration - Contact resistance shall be measured as specified in 4.6.4.

4.6.10 Humidity (steady state) (see 3.5.8). Connectors shall be tested in accordance with method 1002 of MIL-STD-1344. The following details shall apply:

a. Test-condition letter - B of method 103, MIL-STD-202.
b. Final measurements - Insulation resistance shall be measured as specified in 4.6.5.

4.6.11 Salt spray (corrosion)(see 3.5.9). Connectors shall be tested in accordance with method 1001 of MIL-STD-1344. The following details shall apply:

a. Test-condition letter - B of method 101, MIL-STD-202.
b. Measurements after exposure - Immediately after exposure, connectors shall be washed with tap water and allowed to dry for 6 hours maximum in a circulating air oven at a temperature of 38° ±3°C. After drying contact resistance shall be measured as specified in 4.6.4.

5. PACKAGING

5.1 Packaging requirements. The requirements for packaging shall be in accordance with MIL-C-55330.

6. NOTES

6.1 Intended use. The test point connectors covered by this specification are primarily for use in airborne, ground support, and shipboard electrical and electronic equipment, for test purposes only. They are not intended for use during equipment operation.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

6.2 Ordering data. Procurement document should specify the following:

a. Title, number, and date of this specification.
b. Title, number, and date of the application specification sheet, and the complete part number.
c. Levels of preservation, packaging and packing, and applicable marking (see section 5).

6.3 First article. When a first article is required, it shall be tested and approved under the appropriate provisions of 7-104.55 of the Armed Services Procurement Regulation. The first article should be (a preproduction sample), (a first production item) (a sample selected from the first lot of production items) (or it may be a standard production item from the contractor's current inventory as specified in 4.2.1). The first article should consist of (one), (two), etc. unit(s). The contracting officer should include specific instructions in all procurement instruments, regarding arrangements for examinations, test and approval of the first article.

Custodians:
Army - CR
Navy - EC
Air Force - 85

Review activities:
Army - ME
Navy -
Air Force - 11, 17, 99
DLA - ES

User activities:
Army - MI, AR
Navy - AS, YD, MC, CG, OS, SH
Air Force - 14, 19

Preparing activity:
Navy - EC

Agent:
DLA - ES

(Project 5935-3054)

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE: MIL-C-28901

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*.

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

S/N 0102-014-1802

Source: https://assist.dla.mil -- Downloaded: 202640-20T20:53Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T20:53Z
Check the source to verify that this is the current version before use.