# COMMERCIAL ITEM DESCRIPTION

## CHUCK AND KEY, BONE PIN (Jacobs)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a Jacobs chuck with a handle, and the key for the chuck. The chuck is suitable for insertion and withdrawal of bone pins and wires in orthopedic, hand, and podiatry procedures.

Salient characteristics:

Style and design. Style, design and dimensions of the chuck and key shall be in accordance with Figure 1.

Components. Components of the drill shall be in accordance with the following:

Handle. The handle shall be aluminum and have a length of 4 inches (nominally) and a diameter of 3/4 inch (nominally). Handle shall be free from burrs, have no sharp edges, and shall be attached to the shaft.

Shaft. The shaft shall connect the handle to the chuck. The shaft shall be fabricated of Class 3 or Class 4 corrosion-resistant steel in accordance with ASTM Designation F899 and shall have a Rockwell Hardness C Scale (HRC) of 25, minimum.

Chuck. The chuck shall be a 3-jaw No. 1BM Jacobs chuck capable of accepting bone pins and wires having diameters up to and including 1/4 inch. Chuck shall be permanently secured to the shaft. Chuck shall be fabricated of Class 4 martensitic corrosion-resistant steel in accordance with ASTM Designation F899 and shall have a Rockwell Hardness C Scale (HRC) 38, minimum. The finish on the chuck shall be mirror or mirror satin. The chuck shall be marked "stainless".

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Chuck key. The chuck key shall be a No. 1M Jacobs chuck key. It shall be able to open and close jaws of the chuck completely. The chuck key shall be fabricated of Class 4 martensitic corrosion-resistant steel in accordance with ASTM Designation F899 and shall have a Rockwell Hardness C Scale (HRC) 33, minimum. The chuck key shall be marked "stainless".

Passivation. The chuck and key shall be properly passivated.

Sterilization. The chuck and key shall be capable of withstanding repeated sterilization via steam, ethylene oxide, or long term, 10 hour soaking in cold sterilization solution. The chuck and key shall show no evidence of corrosion when autoclaved as follows:

> Clean chuck and key and place in autoclave. Autoclave at 270 ± 5 degrees F for a minimum of 5 minutes. Upon removal from autoclave, examine entire surface area of the chuck and key for evidence of corrosion.

Workmanship. The chuck and key shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One chuck and key, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.



Source: https://assist.dla.mil -- Downloaded: 202640-26T09:22Z
Check the source to verify that this is the current version before use.

Responsibility for compliance. All items must meet all requirements. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in this specification shall not relieve the contractor of the responsibility of assuring that all products or supplies submitted to the Government for acceptance comply with all requirements of the contract. Sampling in quality conformance does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to acceptance of defective material.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. The acceptable quality level (AQL) shall be 0.65 for an inspection level of S-2. The unit of product for test purposes shall be one chuck and key.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.



Source: https://assist.dla.mil -- Downloaded: 202610-26T09:22Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

| NSN | ITEM IDENTIFICATION |
|---|---|
| 6515-01-125-3242 | CHUCK AND KEY, BONE PIN, Jacobs, 3-1/2 Inch (88 mm) |

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 47337

Project No. 6515-4153



Source: https://assist.dla.mil -- Downloaded: 202640-26T09:22Z
Check the source to verify that this is the current version before use.

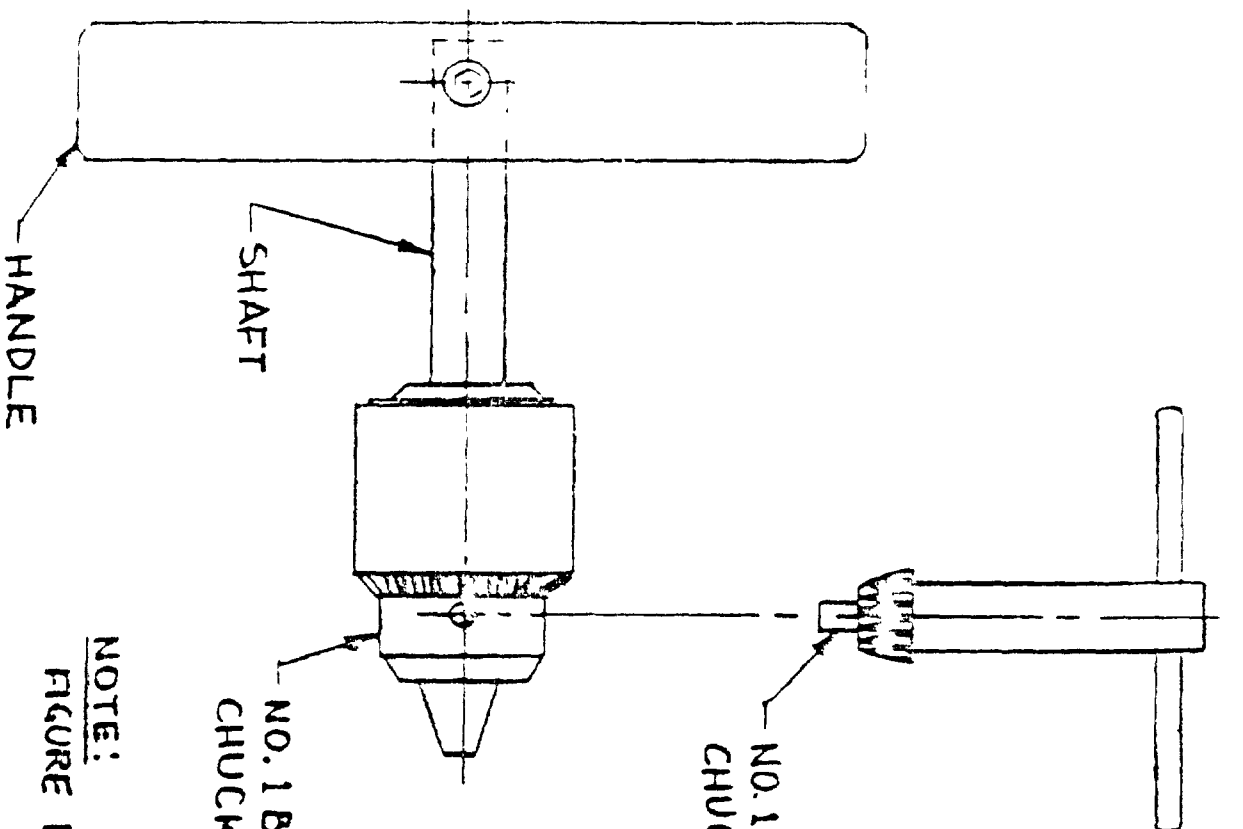



FIGURE 1 CHUCK AND KEY, BONE PIN

NOTE: FIGURE FOR STYLE AND DESIGN ONLY.



Source: https://assist.dla.mil -- Downloaded: 202610-26T09:22Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

*(See Instructions - Reverse Side)*

| 1. DOCUMENT NUMBER | 2. DOCUMENT TITLE |
|---|---|
| A-A-53605 | CHUCK AND KEY, BONE PIN (Jacobs) |

| 3a. NAME OF SUBMITTING ORGANIZATION | 4. TYPE OF ORGANIZATION *(Mark one)* |
|---|---|
| | ☐ VENDOR |
| b. ADDRESS *(Street, City, State, ZIP Code)* | ☐ USER |
| | ☐ MANUFACTURER |
| | ☐ OTHER *(Specify)* |

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

| 7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional | b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional |
|---|---|
| c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional | 8. DATE OF SUBMISSION *(YYMMDD)* |

Source: https://assist.dla.mil -- Downloaded: 2026/0-26T09:22Z
Check the source to verify that this is the current version before use.

**INSTRUCTIONS** In a continuing effort to make our standardization documents better the DoD provides this form for use in submitting comments and suggestions for improvements All users of military standardization documents are invited to pr suggestions This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)* mailed In block 5, be as specific as possible about particular problem areas such as wording which required interpretation was too rigid restrictive loose ambiguous or was incompatible and give proposed wording changes which would alleviate the problems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered

NOTE This form may not be used to request copies of documents nor to request waivers, deviations, or clarification of specification requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

*(Fold along this line)*

*Fold along this line)*

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

**BUSINESS REPLY MAIL**
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN DPSC - RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.