COMMERCIAL ITEM DESCRIPTION

INTRAVENOUS INJECTION CASSETTE SET

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers an intravenous injection cassette set suitable for delivering IV solutions during patient care.

Salient characteristics:

General. Shall be a closed system, sterile, disposable, intravenous injection cassette set, with an infusion pump syringe chamber cassette, an insertion spike, two Y-injection sites, a flexible drip chamber, a roller flow clamp, a male needle Luer adapter, end protectors and 100 ± 5 inches of plastic tubing. The intravenous injection cassette set shall be vented or non-vented, as specified (Note 1). The intravenous injection cassette set shall be compatible with an infusion pump (Note 2).

Materials. The intravenous injection cassette set shall be fabricated of suitable plastics which meet the requirements of the USP for Class II plastics. Tubing and drip chamber shall be fabricated of clear polyvinylchloride.

Style and design. The distal end of the device shall have a tapered insertion spike, capable of piercing an intravenous fluid container and a 15-20 ml drip chamber with a drop forming drip cannula. Cannula and drip chamber shall be leakproof. Cassette shall snap firmly into the infusion pump. Cassette shall have a syringe pump to deliver prescribed volume of fluid determined by the pump setting. Cassette shall not leak while maintaining a closed, sterile system. The intravenous injection cassette set shall have 28 (± 3) inches of clear tubing between the insertion spike and the cassette, and 72 (± 3) inches of clear tubing between the cassette and the proximal end. Both sections of tubing shall have one needle injection site. A roller flow clamp shall be located immediately below the drip chamber. The clamp shall not drift more than 4 drops/minute from the pump set rate after a period of one minute under normal handling. The roller clamp wheel shall not separate from the clamp housing during typical usage or stress.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Non-vented Intravenous Injection Cassette: Shall be suitable for plastic and vented glass solution containers. Shall be in accordance with Figures 1 and 2.

Vented Intravenous Injection Cassette: Shall be suitable for non-vented glass solution container. Shall be in accordance with Figures 1 and 2, with the inclusion of an air inlet vent on the insertion spike. The air inlet vent shall have a ball check valve to vent the solution container during the administration of solution. The air inlet vent opening shall be capped with a removable and replaceable porous bacterial retentive air filter.

Sterility. The intravenous injection cassette set shall be sterile in accordance with USP or AAMI guidelines.

Pyrogenicity and toxicity. The intravenous injection cassette set shall be non-pyrogenic and non-toxic in accordance with the USP.

Drop test. The intravenous injection cassette set shall be tested at 72 ± 5° Fahrenheit (F), using water at a rate of 100 ± 5 drops per minute. The number of drops required to deliver 5 milliliters (ml) shall be counted, and the drops per ml calculated. The number of drops per ml shall range from 15 to 20.

Piercing device (spike) durability test. The piercing device shall be immersed for 4 hours in a solution of USP dextrose and sodium chloride. The piercing device shall be removed from the solution and immediately inserted into a standard solution container (See Note 3). The piercing device shall not loosen, become damaged, or permit leakage after insertion.

Security of roller in clamp body. The roller clamp shall be removed from the set together with a piece of tubing approximately one inch longer than the clamp body. The tubing shall be present in the roller clamp in its normal position with a 1/2 inch length extending from each end of the roller clamp. The clamp shall be held vertically, with the large end down, over a supporting gap so that the roller, if forced out of the body, is free to fall. A polished steel rod is applied to the top of the roller, so that the roller is able to rotate in the course of the test, and the vertical downward force required to separate the roller from the clamp body is measured. The roller shall withstand a 3.65 kilogram load without being separated from the clamp body (See Figure 3).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Pump compatibility and leakage test. The intravenous injection cassette set shall be tested for compatibility with the infusion pump (See Note 2). The cassette shall seat firmly onto the pump and allow variable flow without leakage ranging from 1 ml/hr to 299 ml/hr.

Instructions. Each intravenous injection cassette set shall be provided with complete instructions for use.

Workmanship. The intravenous injection cassette set shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing twenty sterile intravenous injection cassette sets, each set individually packaged in a sealed container as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for Inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be level S-3 and acceptance number zero, in accordance with MIL-STD-105. The unit of product for test purposes shall be one intravenous injection cassette set.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE 1: The following National Stock Number is covered by this document.

NSN	ITEM IDENTIFICATION
6515-01-156-2898	INTRAVENOUS INJECTION CASSETTE SET, Non-Vented, With Flexible Drip Chamber, Closed System, Disposable, 20's

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

NSN	ITEM IDENTIFICATION
6515-01-153-5745	INTRAVENOUS INJECTION CASSETTE SET, Vented, with Flexible Drip Chamber, Closed System, Disposable, 20's

NOTE 2: The intravenous injection cassette set shall be compatible with a 6 volt, Battery Operated, Portable, Volumetric, Intravenous Infusion Pump (NSN 6515-01-025-8839).

NOTE 3: The intravenous injection cassette set shall be compatible with a 250 ml container of Type I, Size 2, Strength 1, 5 percent USP, Dextrose Injection (NSN 6505-00-975-0604).

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4366

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.



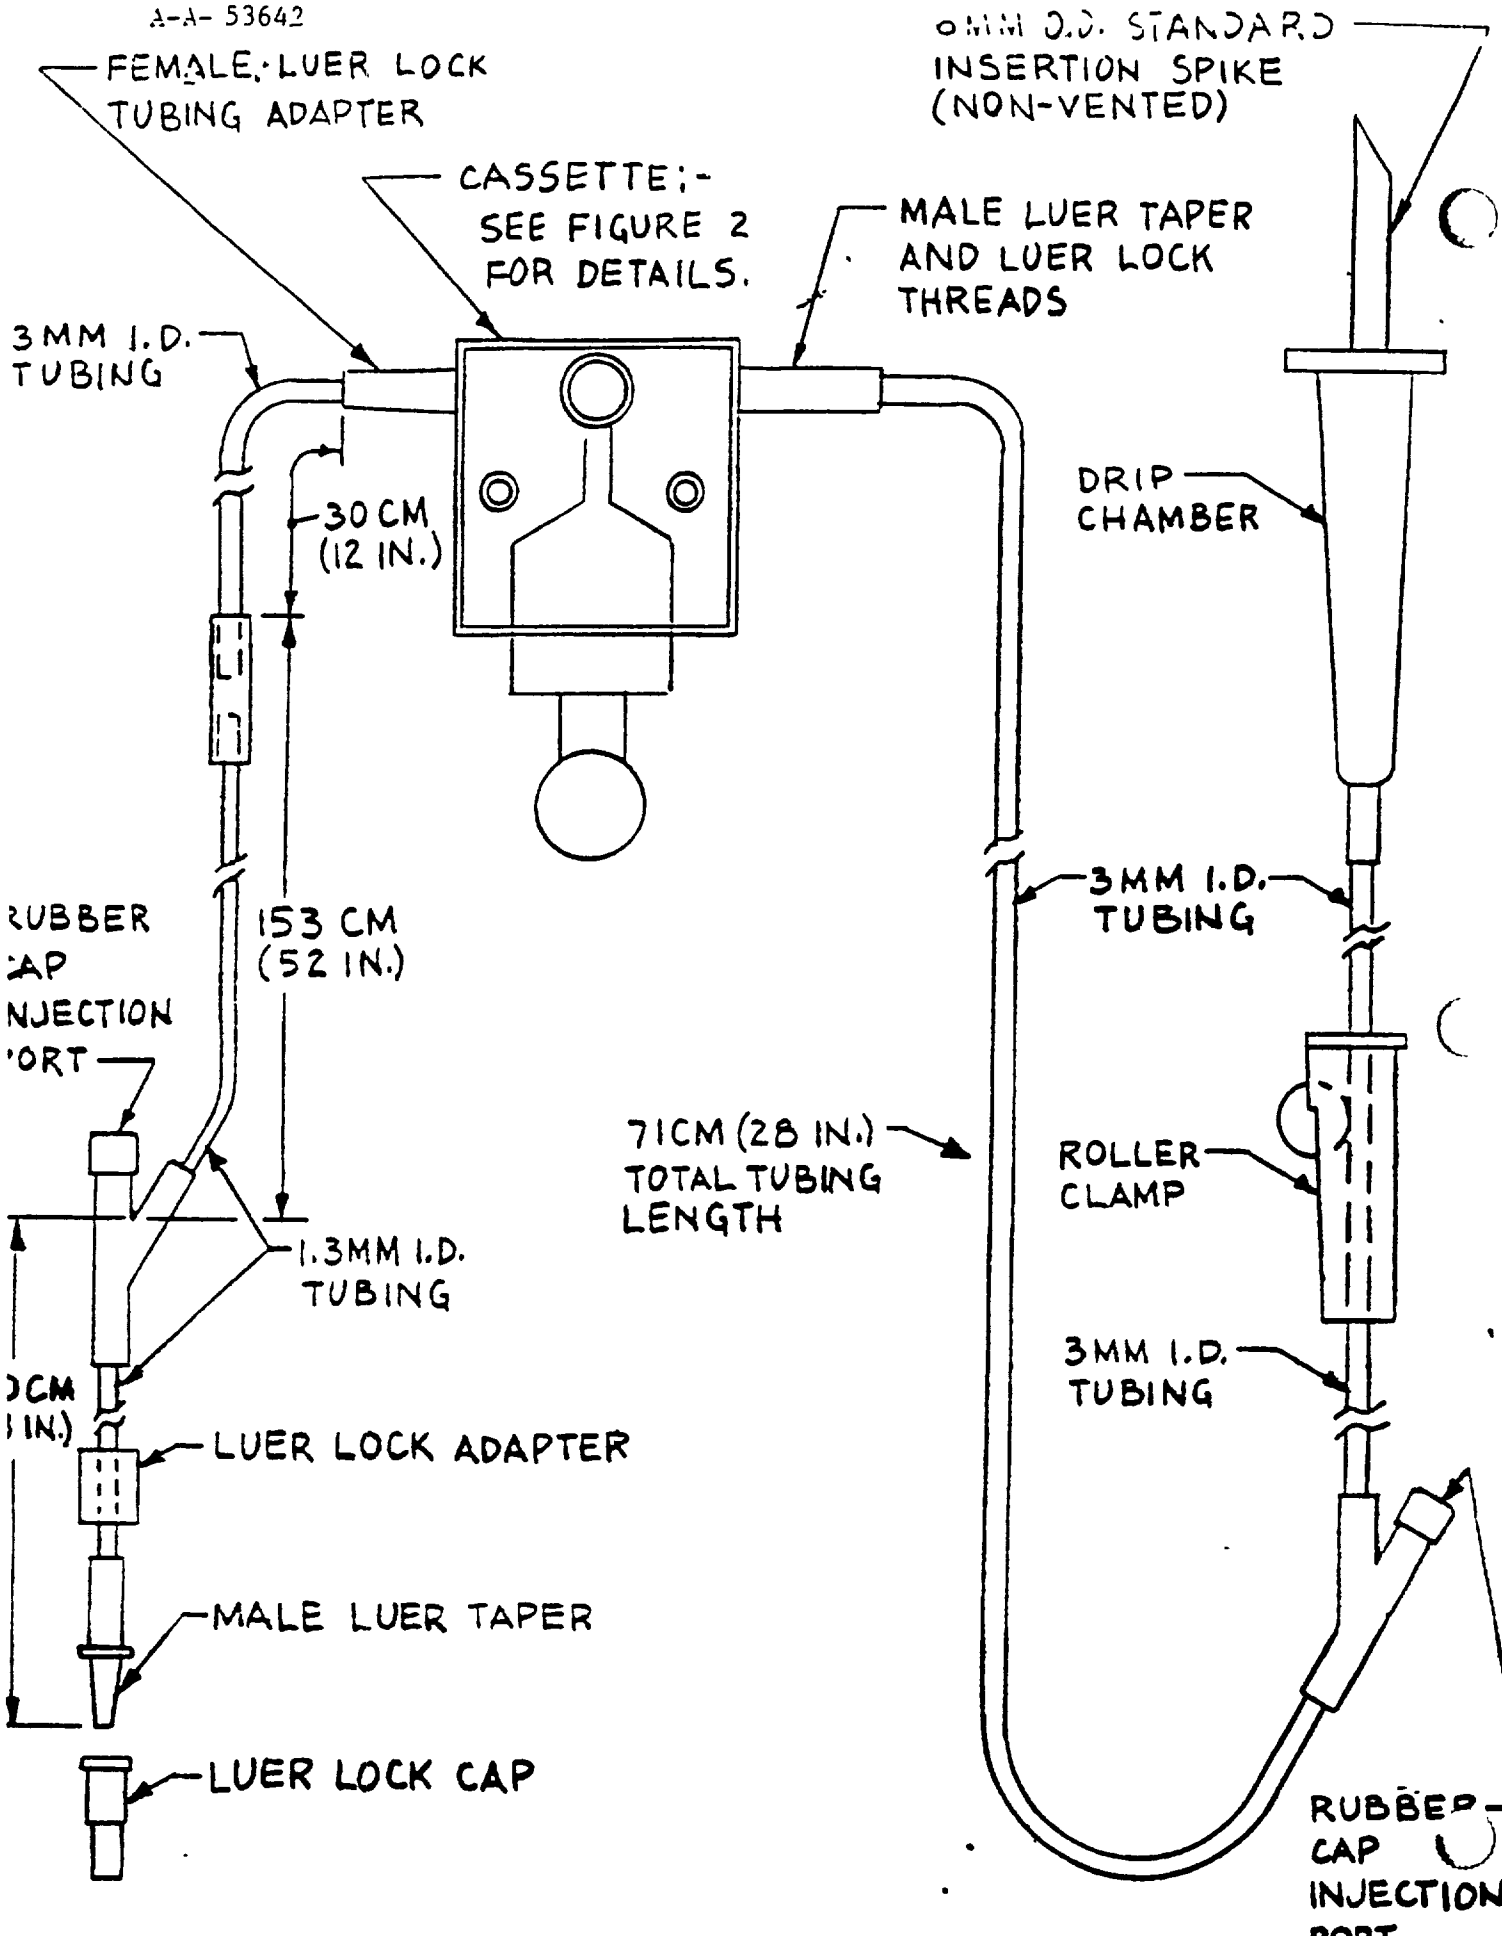


FIGURE 1 INTRAVENOUS INJECTION CASSETTE SET

Source: https://assist.dla.mil -- Downloaded: 2020-10-20T00:22Z
Check the source to verify that this is the current version before use.

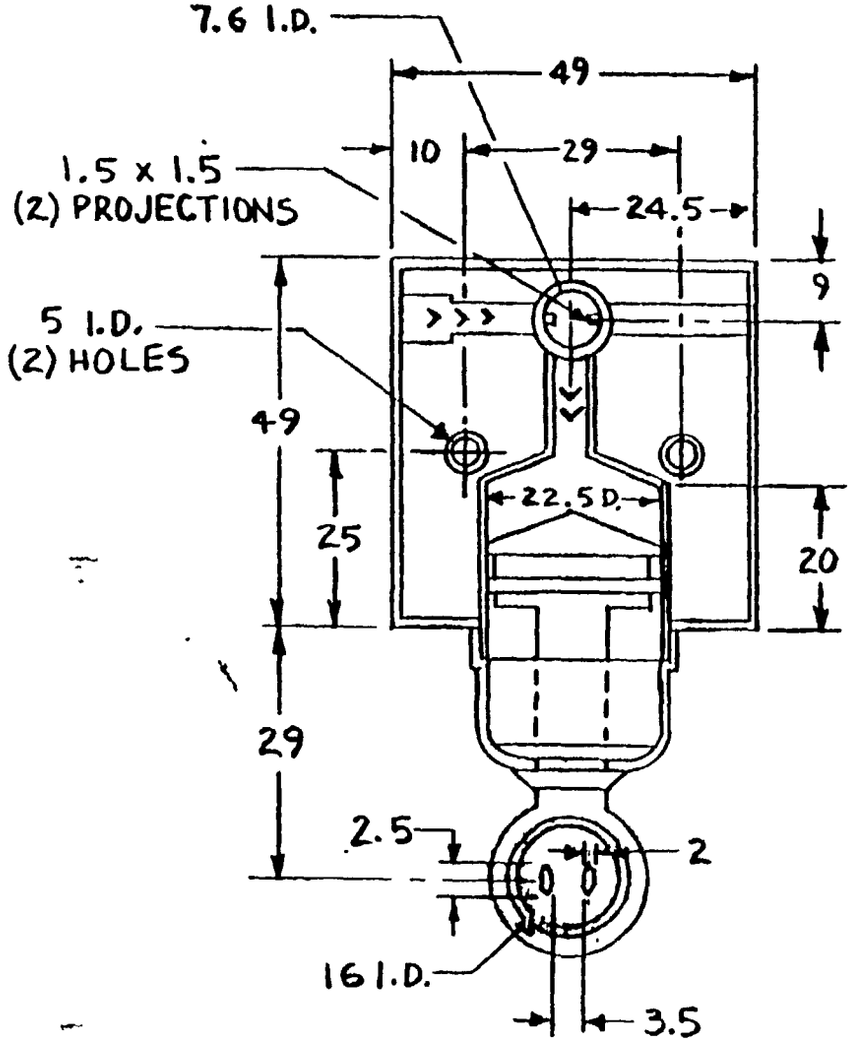

INTAKE
FROM CONTAINER

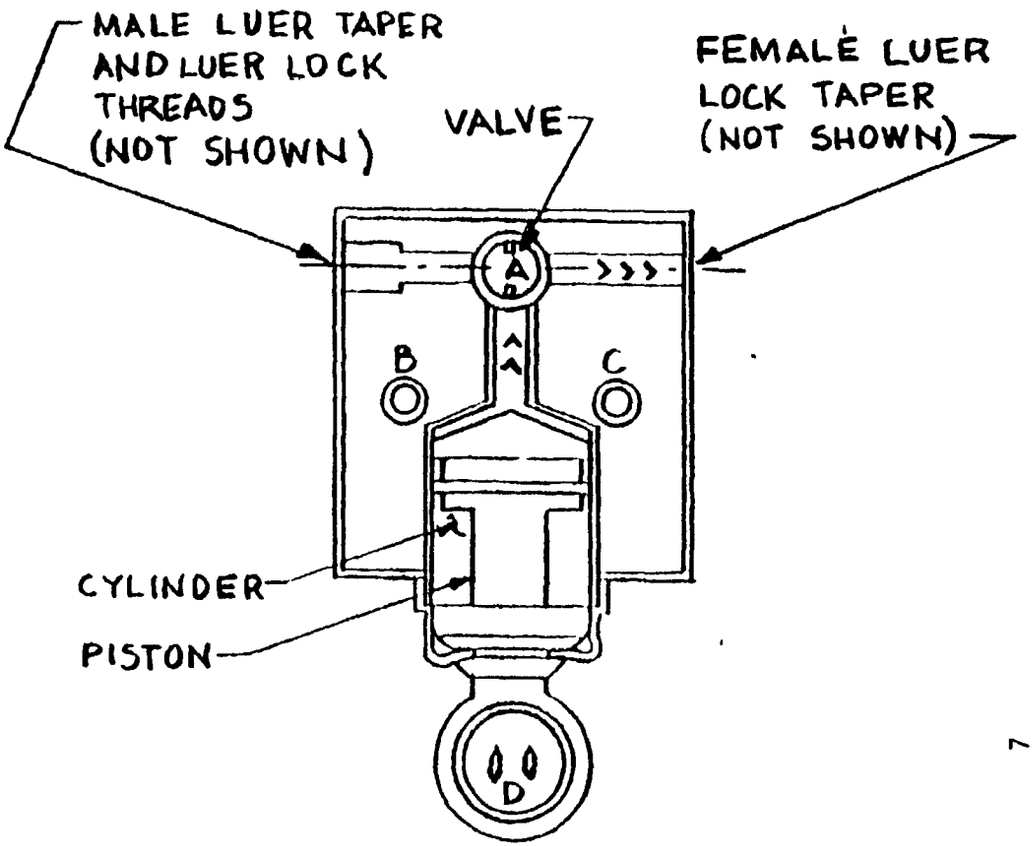


INFUSION
TO PATIENT

NOTES:
1. CYLINDER STROKE VOLUME IS 3.5 CC.
2. PUMP (NSN 6515-01-025-8839) CONNECTS TO CASSETTE AT A, B, C AND D.

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN MILLIMETERS.
TOLERANCES
BELOW 10MM = ±0.5MM
10MM AND ABOVE = ±1MM

FIGURE 2 CASSETTE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

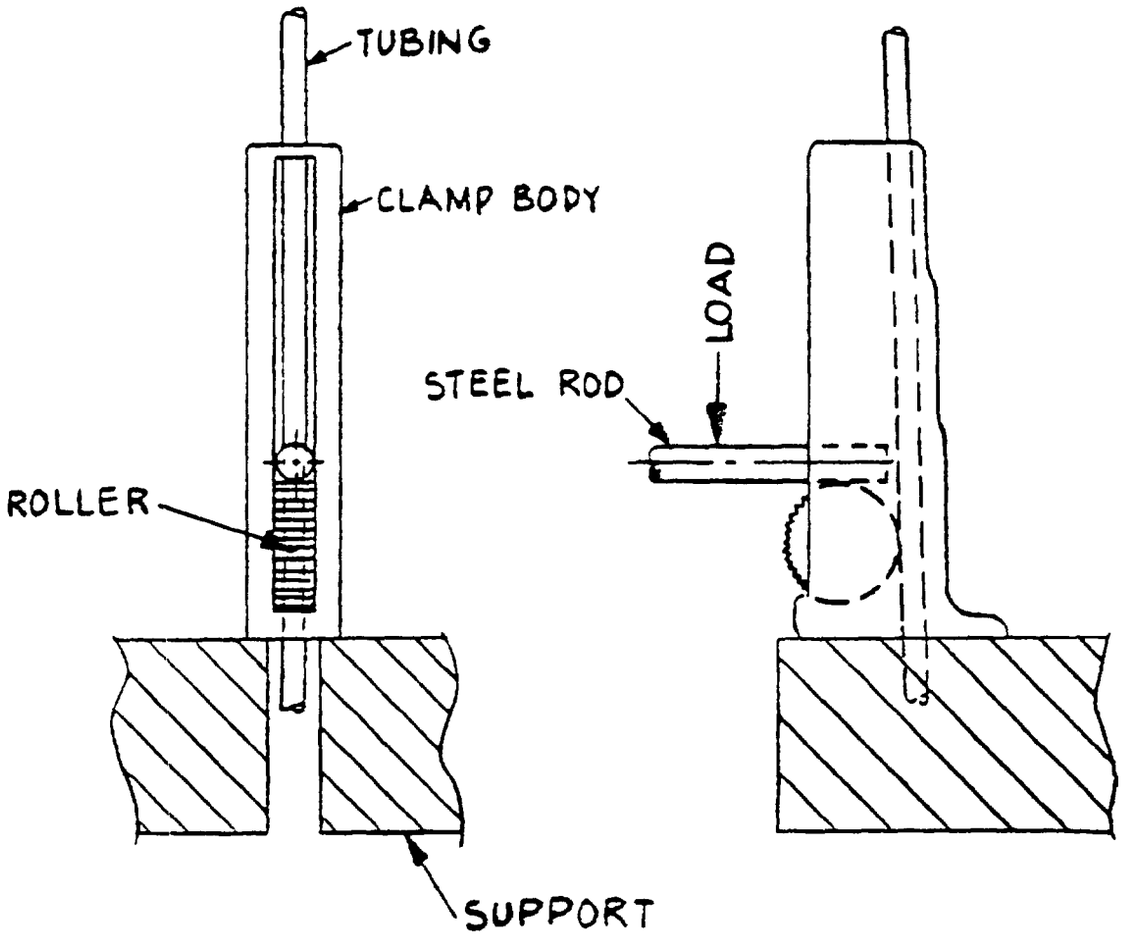

METHOD OF APPLYING LOAD TO ROLLER

FIGURE 3

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-53642	INTRAVENOUS INJECTION CASSETTE SET

3a. NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.