A-A-53658
24 August 1988

COMMERCIAL ITEM DESCRIPTION

CARRIER, BRONCHOSCOPIC SPONGE (Jackson Extra-Heavy)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a Jackson design bronchoscopic sponge carrier.

Salient characteristics:

Style and design. Shall be a bronchoscopic sponge carrier. Style and design of the carrier shall conform to Figures 1,2, and 3. The style and design specified herein shall be known as the "Extra-Heavy Jackson Design".

Performance. The carrier shall hold 12-ply gauze bronchoscopic sponges used with 5 mm through 9 mm bronchoscopes. The carrier's jaws shall open when the handle is turned clockwise and close when the handle is turned counterclockwise.

Materials. Each carrier component shall be fabricated from the material specified in Table 1. All grades of stainless steel specified herein shall comply with ASTM Designation F899.

Table 1 - Materials of Construction.

Component	Material
Handle	Type 303 Stainless Steel
Reducing Bushing	Same as above
Threaded Bushing	Same as above
Main Shaft	Type 410 Stainless Steel
Jaw Blades	Type 430 Stainless Steel
Body Tube	Monel 400
Locking Tube	Same as above
Threaded Tube	Nickel-Silver

AMSC/NA FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Hardness. The hardness of each carrier component shall be as specified in Table 2. Each carrier component shall be tested for hardness. Hardness testing shall be performed in accordance with ASTM Designation E18.

Table 2 - Component Hardnesses

Component	Hardness
Handle	HRB 90 - HRB 110
Reducing Bushing	Same as above
Threaded Bushing	Same as above
Main Shaft	HRC 38 - HRC 42
Jaw Blades	HRC 38 - HRC 48
Body Tube	HRB 63.6 - HRC 23.2
Locking Tube	Same as above
Threaded Tube	HRB 87 - HRB 91

Corrosion-resistance. The corrosion-resistance requirements for the carrier's components are as follows:

All carrier components fabricated from 300 series corrosion-resisting (stainless) steel shall pass the boil-test specified in ASTM Designation F1089.

All carrier components fabricated from 400 series corrosion-resisting (stainless) steel shall pass the copper-sulphate test and boil-test specified in ASTM Designation F1089.

Passivation. All corrosion-resisting (stainless) steel carrier components shall be passivated to resist corrosion.

Finish. All carrier components shall have a bright, smooth finish, except where knurling is indicated in Figure 1.

Workmanship. The fully assembled sponge carrier shall be free from defects that detract from its appearance or impair its serviceability.

Unit. Each (EA). One carrier, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 at Level S-2, AQL 0.65%. The unit of product for tests purposes shall be one carrier.

Sample carriers shall be inspected for workmanship, style and design, and performance. Carriers shall be disassembled and inspected for finish, hardness, and corrosion-resistance.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-8374	CARRIER, BRONCHOSCOPIC SPONGE, JACKSON, EXTRA-HEAVY, 23-1/2 Inches (cm)

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 51092 Project No. 6515-3450

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

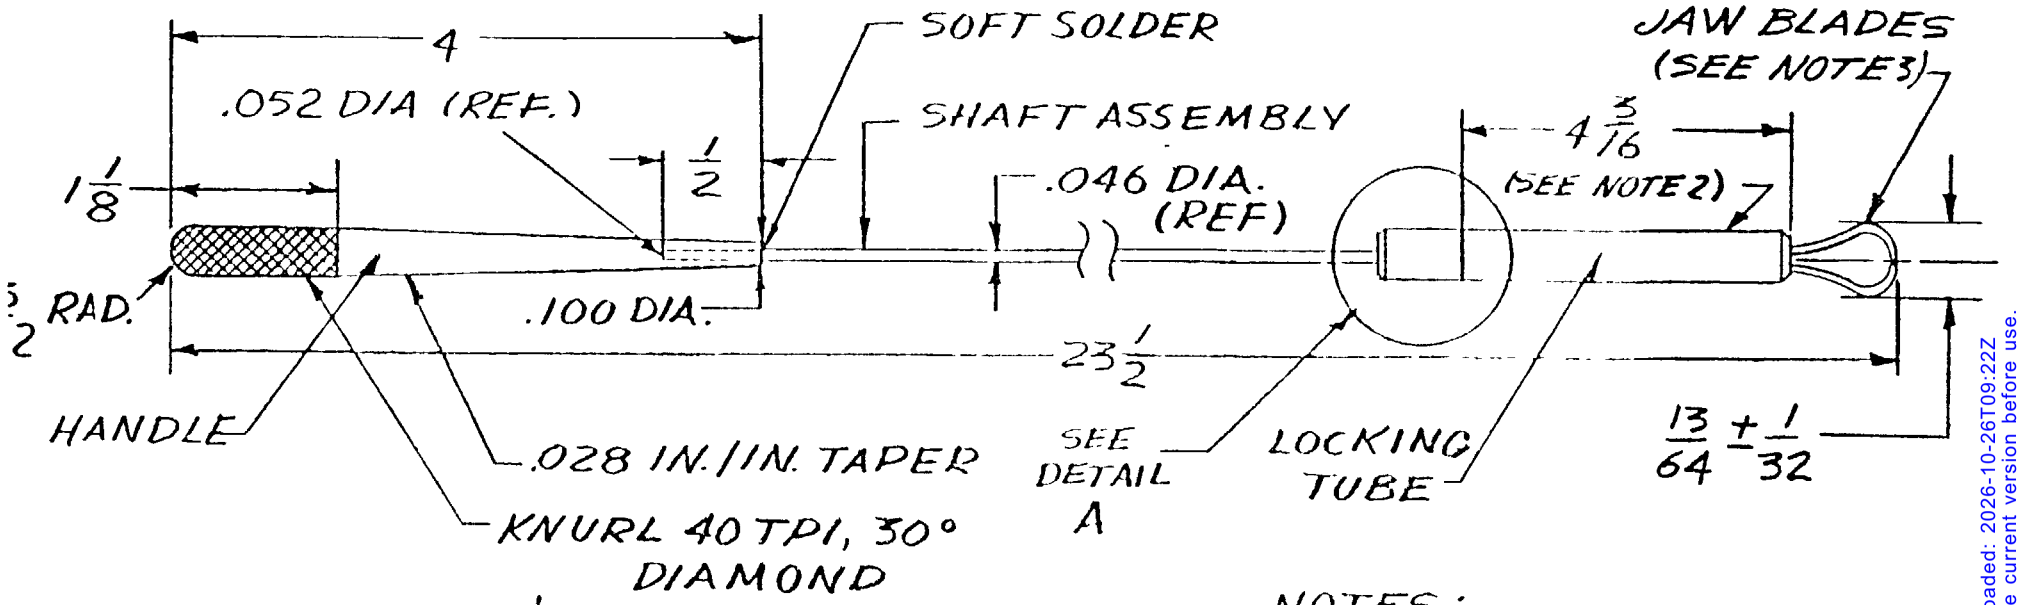

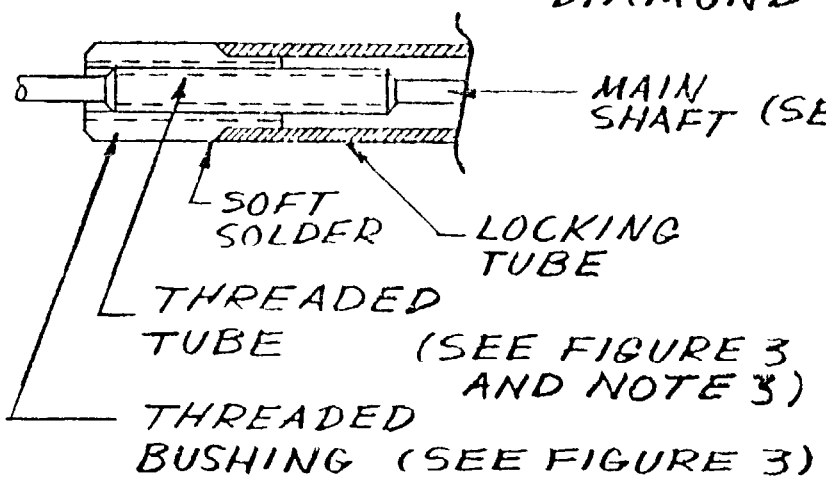

DETAIL A


NOTES:

1. UNLESS OTHERWISE SPECIFIED TOLERANCES SHALL BE AS FOLLOWS:
   A. FRACTIONS: ± 1/64
   B. DECIMALS: ±.005
2. DIMENSIONS FOR LOCKING TUBE SHALL BE .135 OD BY .125 ID. BOTH ENDS SHALL HAVE .010 × 60° CHAMFER.
3. JAW BLADES, MAIN SHAFT AND THREADED TUBE COMPRISE SHAFT ASSEMBLY PER FIG. 2

A-A-53658

FIGURE 1. CARRIER, BRONCHOSCOPIC SPONGE, JACKSON, EXTRA-HEAVY

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

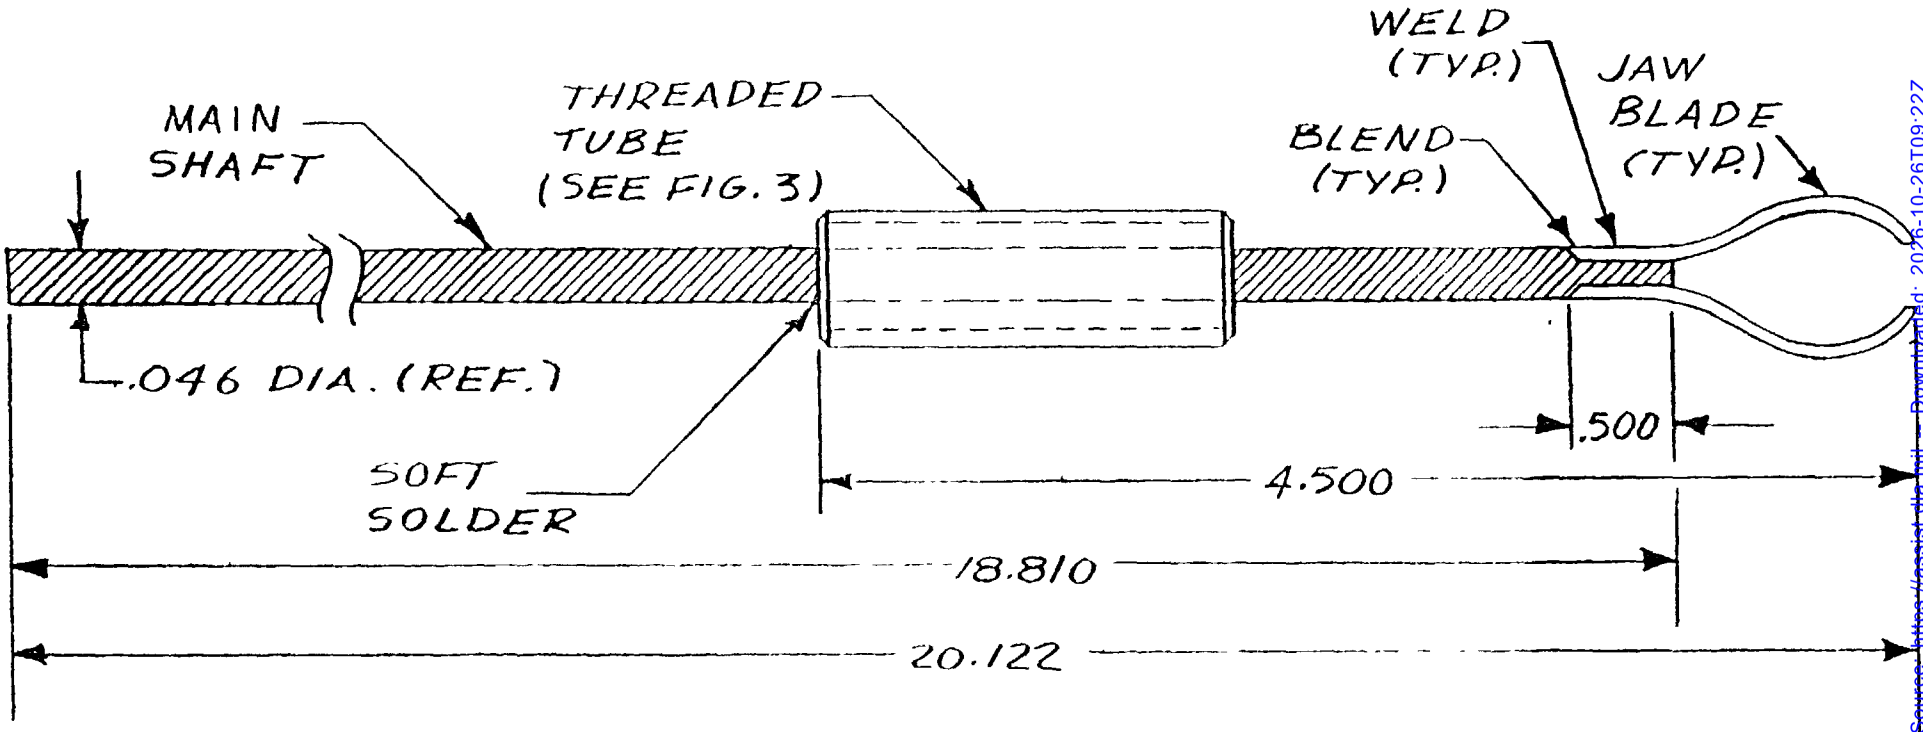


NOTE:

1. UNLESS OTHERWISE SPECIFIED TOLERANCES SHALL BE ± .005
2. ON FIG.'S 1, 2 & 3 ALL DIMS. ARE IN INCHES.

FIGURE 2 SHAFT ASSEMBLY, BROCHOSCOPIC SPONGE CARRIER

Source: https://assist.dla.mil — Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.


THREADED BUSHING

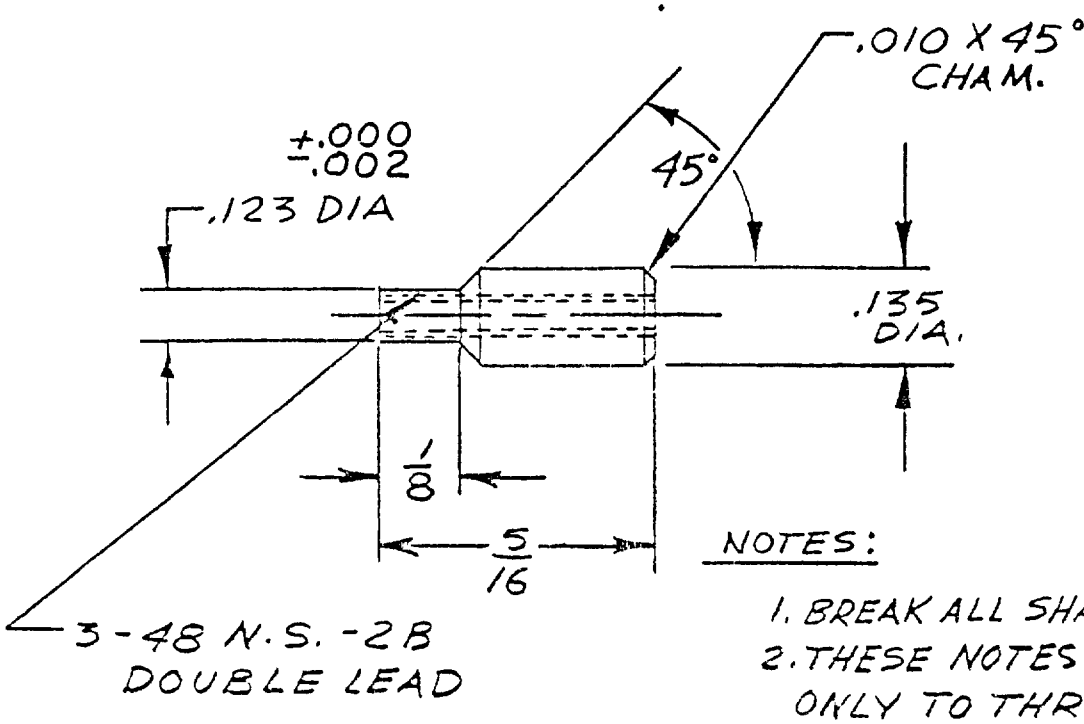

NOTES:

1. BREAK ALL SHARP EDGES
2. THESE NOTES APPLY ONLY TO THREADED BUSHING.

THREADED TUBE

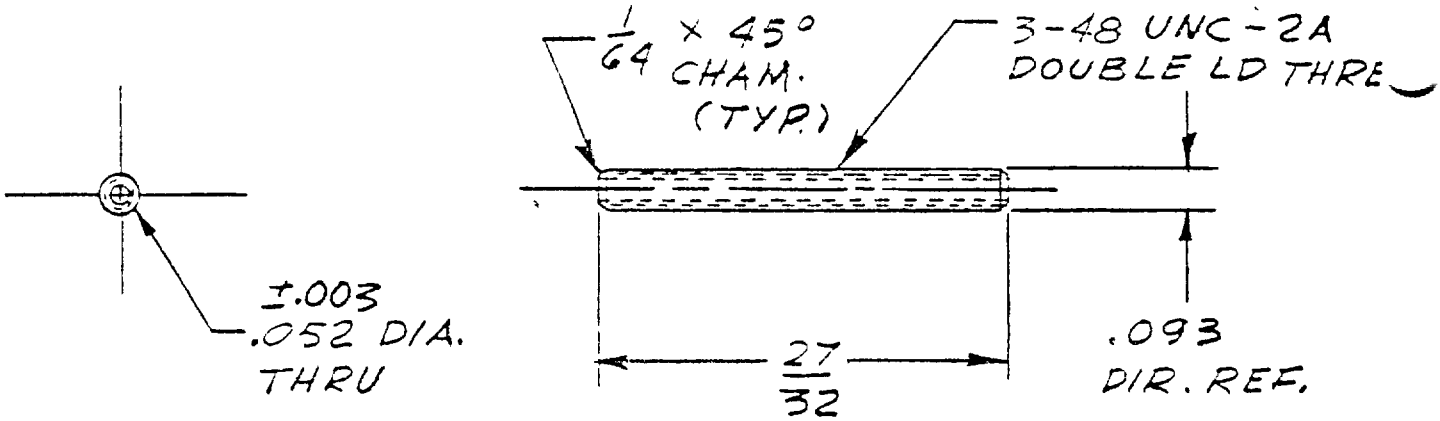

NOTE:

1. FOR BOTH THREADED TUBE AND BUSHING, TOLERANCES ARE AS FOLLOWS:
   - A. FRACTIONS: ±1/64
   - B. DECIMALS: ±.005
   - C. ANGLES: ±1/2°

NOTES:

1. THREAD DIM.
   - .0946 / .0990 MAJ. DIM.
   - .0833 PITCH
   - .0855 DIA.
2. THESE NOTES APPLY ONLY TO THREADED TUBE

FIGURE 3 THREADED BUSHING AND THREADED TUBE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-53658	CARRIER, BRONCHOSCOPIC SPONGE (Jackson Extra-H

3a. NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark on*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street, City, State ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Inclu Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.