A-A-53840/3
10 May 1990

COMMERCIAL ITEM DESCRIPTION SHEET

HOOK, TYRELL

The General Services Administration has authorized the use of this Commercial Item Description Sheet as a replacement for Military Specification MIL-H-37004 which is cancelled.

The complete requirements for procuring hooks shall consist of this document and the issue in effect of Commercial Item Description A-A-53840.

Salient characteristics:

Style, design and dimensions. This specification covers the following neurosurgical hooks:

Style 1- Blunt Point Iris
Style 2- Sharp Point Iris

The hooks shall be in accordance with Figure 1.

Notes:

a. Intended use: Neurosurgical hooks of the Tyrell design covered in this Commerical Item Description Sheet are intended for aiding in neurosurgical procedures on the eye.

b. Copies of Commercial Item Description A-A-53840 may be obtained by writing Standardization Documents Order Desk, Building 4D, 700 Robbins Avenue, Phialdelphia, PA 19111-5094

c. National Stock Number and Item Identification

NSN	Item Indentification
6515-00-342-3100	HOOK, IRIS, Blunt, Tyrell, Style 1
6515-00-342-3300	HOOK, IRIS, Sharp, Tyrell, Style 2

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:25Z
Check the source to verify that this is the current version before use.

A-A- 53840/3

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4660

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:25Z
Check the source to verify that this is the current version before use.

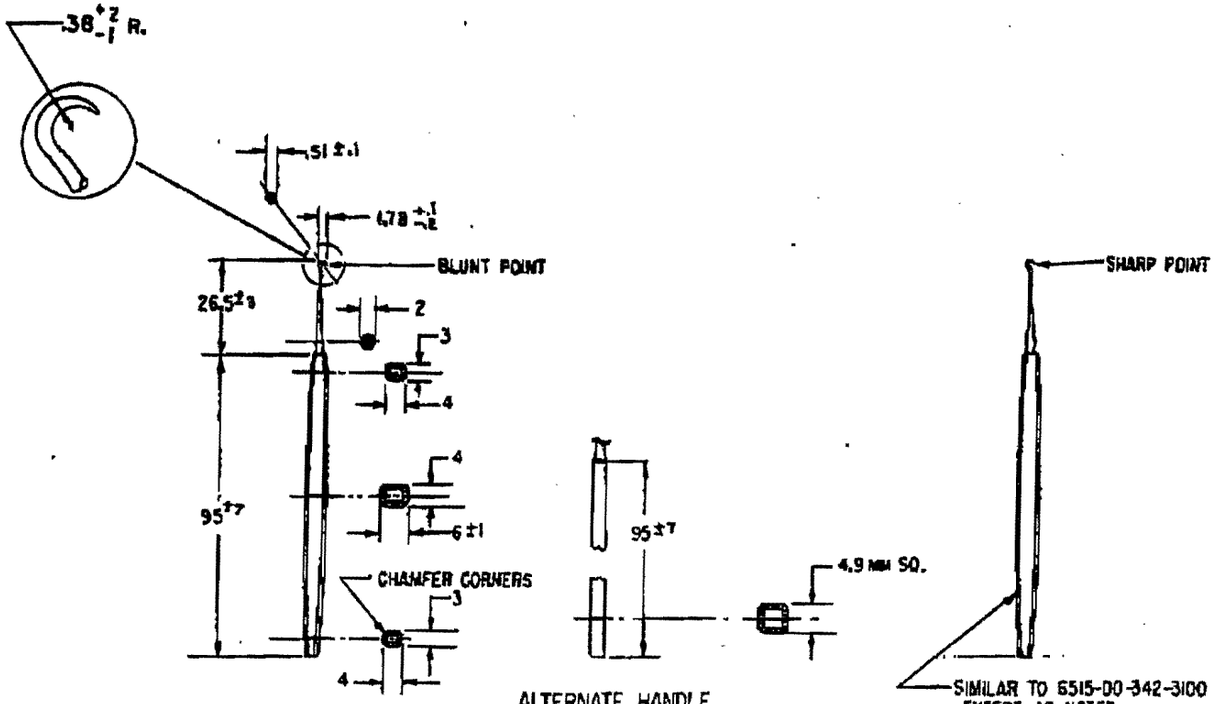

ALTERNATE HANDLE

HOOK, IRIS, BLUNT, TYRELL
NSN 6515-00-342-3100
STYLE 1

HOOK, IRIS, SHARP, TYRELL
NSN 6515-00-342-3300
STYLE 2

NOTES

1 UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN MILLIMETERS AND TOLERANCES ARE AS FOLLOWS: ALL DIMENSIONS UP TO 5 MM. ± .5

2 TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY, AND FIRST QUALITY WORKMANSHIP

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:25Z
Check the source to verify that this is the current version before use.