A-A-53857
30 May 1989

COMMERCIAL ITEM DESCRIPTION

PAD, OPERATING TABLE

Two Sections

The General Services Administration has authorized the use of this Commercial Item Description.

This Commercial Item Description covers a two-section operating table pad, suitable for use with the folding-type operating and dressing table.

Salient characteristics:

The operating table pad shall be supplied in two sections and shall be suitable for use with the folding type operating and dressing table built into shipboard battle dressing stations. The two-section pad shall be of the design shown in figure 1.

The head section shall consist of a fire-resistant polyurethane foam at least 1 inch thick, 41-1/2 inches plus or minus 1/2 inch long by 19 inches plus or minus 1/2 inch wide, suitably covered with a snugly fitting, black, electrically conductive rubber material of box construction with inside seams, which meets the requirements of Underwriters' Laboratories, Inc. The head end of the conductive cover shall have a durable slide fastener closure to permit easy insertion and removal of the pad. The head end of the cover shall be legibly and permanently labeled "HEAD SECTION-HEAD END". Four durable web ties, each a minimum of 16 inches long and 1 inch wide, shall be securely sewn into the top seam of the conductive cover. The ties shall be attached two on each side of the head section, one approximately 11-1/2 inches from the head end and the other approximately 6 inches from the perineal end.

The leg section shall consist of a fire-resistant polyurethane foam pad at least one inch thick, 30 inches plus or minus 1/2 inch long by 19 inches plus or minus 1/2 inch wide, suitably covered with a snugly fitting, black, electrically conductive

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:26Z
Check the source to verify that this is the current version before use.

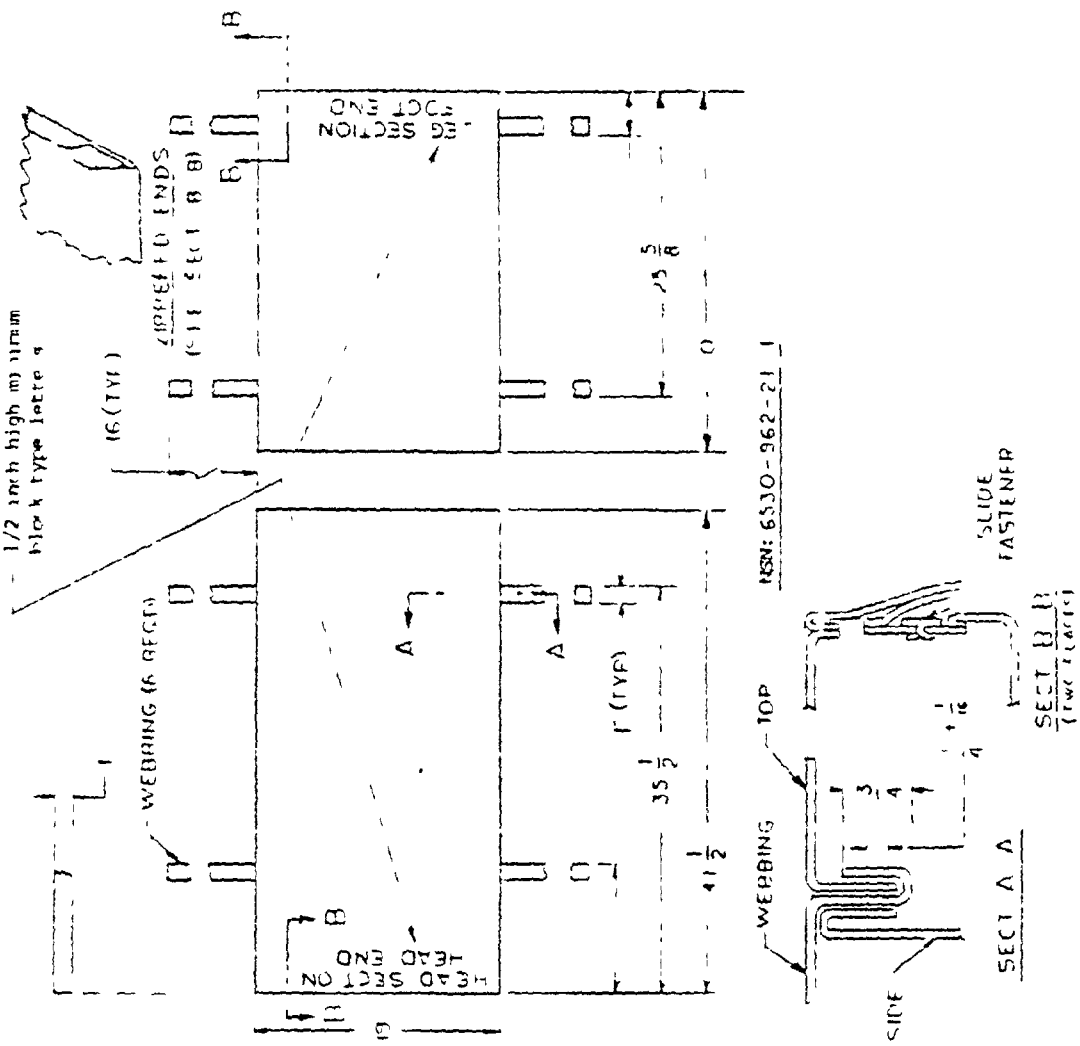


FIGURE 1. Operating table pad.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:26Z
Check the source to verify that this is the current version before use.

rubber material of box construction with inside seams, which meets the requirements of Underwriters' Laboratories, Inc. The foot end of the conductive cover shall have a durable slide fastener closure to permit easy insertion and removal of the pad. The foot end of the cover shall be permanently and legibly labelled "LEG SECTION-FOOT END". Four durable web ties, each a minimum of 16 inches long and 1 inch wide, shall be securely sewn into the top seam of the conductive cover. The ties shall be attached two on each side of the leg section, one approximately 4-3/8 inches (11.10 cm) from the head end and the other approximately 2 inches (3.08 cm) from the foot end.

The polyurethane foam shall be of uniform cellular construction with 40 to 55 cells per inch and a density of 2 pounds per cubic foot, plus or minus 10 percent. A load of 40 to 55 pounds shall produce a 25 percent indentation. The deflection for a 60 to 100 pound load shall be 65 percent. Elongation shall be 350 to 600 percent. Resilience shall be a ball rebound of 25 to 40 percent.

The rubber material shall be a cotton or synthetic cloth rubber coated on both sides. The coated cloth shall have a thickness between 0.013 inch and 0.018 inch, with a breaking strength of 50 pounds minimum. The coated cloth shall meet the requirements for Reduction of Electrostatic Hazard-Table Covers and Sheeting, as specified in National Fire Protection Association (NFPA) No. 99, Health Care Facilities Anesthetics.

The slide fastener shall be a slide interlocking, non-separating, non-reversible fastener without lock. The fastener shall have a bridge type top stop and a closed bottom stop with a single slider arrangement. The fastener shall be of sufficient length to permit easy removal of the rubber cover. The slide fastener shall be securely attached with double stitching.

The web ties shall be of woven heavyweight cotton, 1 inch wide, weighing not less than 1.33 ounces per linear yard with a minimum breaking strength of 550 pounds. The ties shall be water repellent, mildew resistant, and dyed black. The exposed raw ends of the webbing straps shall be suitably finished or contained to prevent unraveling.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:26Z
Check the source to verify that this is the current version before use.

All stitching shall be machine stitching conforming to type 301 (stitch formed with two threads: one needle thread and one bobbin thread. A loop of the needle thread shall be passed through the material to be sewn and interlaced with the bobbin thread. The needle thread shall be pulled back so that the interlacing shall be midway between surfaces of the materials being sewn). There shall be a minimum of eight stitches per inch.

Workmanship. The operating table pad shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One pad, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:26Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 4.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one operating table pad, as specified in this description.

Defects.

Any component of pad is missing, broken, or otherwise unusable.

Pad is not made of polyurethane foam.

Exposed ends of the webbing straps are not contained to prevent unraveling.

Slide fasteners are not securely fastened and free moving.

Rubber cover does not fit over the inner pad smoothly and neatly.

Identification marking of head section and foot section is not complete, permanent, or legible.

Stitching is not the correct type.

Stitching is not machine stitching with a minimum of eight stitches per inch.

Sampling for tests. Sampling for tests (dimensional) shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-2. The unit of product for test purposes shall be one operating table pad.

a. First article. Where a first article sample is required, all tests shall be performed on that unit.

b. Acceptance testing. When a first article sample has not been required, one unit shall be subjected to the performance test specified herein. If a test article sample has successfully passed all tests, performance test shall not be required at acceptance.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:26Z
Check the source to verify that this is the current version before use.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6530-00-962-2121

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:26Z
Check the source to verify that this is the current version before use.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6530-2063

Location:
CID/PAD/OPERATING/TABLE/H13-32

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:26Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-53857	PAD, OPERATING TABLE, Two Sections

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*.

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:26Z
Check the source to verify that this is the current version before use.

DD FORM 1426

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge (DO NOT STAPLE), and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s), or to amend contractual requirements.

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4968 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:26Z
Check the source to verify that this is the current version before use.