MIL-D-0051082D(MU)
15 April 1969
USED IN LIEU OF
MIL-D-51082C
29 December 1966

MILITARY SPECIFICATION

DETECTOR TUBES, CHEMICAL AGENT

This limited coordination Military specification has been prepared by Edgewood Arsenal based upon currently available technical information, but it has not been approved for promulgation as a coordinated revision of *Military Specification MIL-D-51082C. It is subject* to modification. However, pending its promulgation as a coordinated Military specification, it may be used in procurement.

1. SCOPE

1.1 Scope. This specification covers detection tube assemblies consisting of clips of tubes for sampling and detecting chemical agents.

1.2 Classification. The tubes shall be of the following types:

Type I - Mustard and G-agent (H and G) detector.
Type II - Hydrogen cyanide (AC) detector.
Type III - Phosgene (CG) detector.
Type IV - Arsenicals (L and ED) detector.
Type V - Arsenical (L) detector.
Type VI - CN-BBC detector.
Type VII - Sampling tube.

2. APPLICABLE DOCUMENTS

2.1 Government documents. The following documents of the issue in effect on date of invitation for bids or request for proposal form a part of this specification to the extent specified herein.

SPECIFICATIONS

MILITARY

MIL-S-14374 - Silica Gel, Iron Free.
MIL-P-50014 - Packet, Sodium Pyrophosphate Peroxide.
MIL-T-51023 - Tablets, Compound 34.

FSC 6665

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

STANDARDS

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.
MIL-STD-414 - Sampling Procedures and Tables for Inspection by Variables for Percent Defective.

DRAWINGS

US ARMY MUNITIONS COMMAND

EDGEWOOD ARSENAL

C5-77-387 - Clips, Detector Tube.
C5-77-784 - Dispenser, Filled.
C5-77-820 - Clips, Detector Tube.
D5-77-446 - Tubes, Detector.
IL 136-41-780 - Dilution Apparatus, Toxic Gas, Q5.
DL 136-14-360 - Apparatus, Airflow Resistance, Q34.

(Copies of specifications, standards, drawings, and publications required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

UNIFORM CLASSIFICATION COMMITTEE

Uniform Freight Classification

(Application for copies of these ratings, rules and regulations should be addressed to Uniform Classification Committee, 202 Union Station, 516 West Jackson Boulevard, Chicago, Illinois 60606.)

MUNSELL COLOR COMPANY, INC.

Munsell Book of Colors

(Application for copies of this book should be addressed to the Munsell Color Company, Inc., Baltimore, Maryland 21203.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

AMERICAN SOCIETY FOR TESTING AND MATERIALS

ASTM Standards

D1193-66 - Reagent Water.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, Pennsylvania 19103.)

3. REQUIREMENTS

3.1 Materials and components.

3.1.1 Materials. All materials cited on Drawing D5-77-446 and on subsidiary drawings shall conform to the specifications listed thereon or to the specific characteristics set forth on the drawings.

3.1.2 Components. All components of the detector tubes shall conform to the specifications and drawings listed on Drawing D5-77-446.

3.2 Manufacture and assembly. The detector tubes shall be manufactured in accordance with Drawing D5-77-446 and assembled in accordance with Drawing C5-77-387, C5-77-784, or C5-77-820, as applicable (see 6.2).

3.2.1 Gels. Silica gel conforming to MIL-S-14374 shall be used and impregnated where indicated (see 6.4):

Tube type	Material
I	DB3 Mercuric cyanide
II	Cupric sulfate p,p'-Tetramethyldiaminodiphenylmethane Salicylic acid Dye (see 6.7)
III	p-Dimethylaminobenzaldehyde N-Phenyl-1-naphthylamine Thiourea
IV	Ammonium molybdate Zinc sulfate
V	Cupric nitrate Potassium iodide
VI	m-Dinitrobenzene
VII	Silica gel (not impregnated)

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

Impregnated gels shall be no older than 120 days when sealed into detector tubes (all type tubes except type VII). Sealed tubes shall be no older than 120 days when the three year expiration date is stamped on the kit.

3.2.2 Charcoal. Forty to sixty mesh activated charcoal shall be used in type II tubes (see 6.5).

3.3 Leakage. The detector tubes shall not leak when tested in accordance with 4.4.4.1.

3.4 Airflow resistance. The detector tubes of all types shall have an airflow resistance of 40 to 70 millimeters (mm) of water. As an exception, type II detector tubes for the M18A2 detector kit only (Drawing C5-77-820) shall have an airflow resistance of 40 to 95 mm of water. Test for airflow resistance shall be conducted in accordance with 4.4.4.2.

3.5 Volatile matter. The volatile content of the gels and the charcoal in the detector tubes shall conform to table I when tested in accordance with 4.4.4.3.

Table I. Volatile matter

Tube type	Percent
I, IV, V	5.0 max
II Gel	15.0 max
Charcoal	14.0 min
III, VI	10.0 max
VII	3.0 max

3.6 Stability. Before and after aging the detector tubes for two weeks at 65° + 2°C, the gel layer shall comply with the designated colors in table II when tested in accordance with 4.4.4.4. The Munsell Book of Colors shall be used in determining the color.

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

Table II. Munsell colors

Tube type	Hue	Value	Chroma
I, V, VI, VII	Neutral	9,9.5	0
II	5.0 R	9	0.5
	10 R	9	1
	5.0 YR	9	1
	10 YR	9	1,2
	2.5 Y	9	1,2
	5.0 Y	9	0.5,1,2
	7.5 Y	9	1,2
	5.0 GY	8,9	1
	5.0 G	9	0.5
III	5.0 Y	9	10,12,14
	5.0 Y	8	8,10,12
	7.5 Y	8,9	8,10
IV	7.5 Y	9	3,4,6,8
	10 Y	8	6,8
	2.5 GY	8	4,6
	2.5 GY	9	4

3.7 Sensitivity. Before and after aging for two weeks at 65° + 2°C, the detector tubes shall comply with the requirements of table III when tested in accordance with 4.4.4.5.

Table III. Sensitivity

Tube type	Requirement
Blanks for I, IV, V, VI	2.5Y to 7.5Y 9/3 (max)
I (H)	blue or purple-blue ring in 15 sec
I, VII (G)	yellow ring in 30 sec
II	blue ring immediately
III	green color immediately
IV	blue or blue-green ring in 15 sec
V	red-brown ring in 15 sec
VI	pink or magenta ring in 15 sec

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

3.8 Score breakage. When tested in accordance with 4.4.4.6, the tubes shall break along the score mark without splintering when subjected to a maximum load of 950 grams (g). The tubes shall not break when subjected to a load of 400 g. When broken by hand, at least 60 percent of the tube shall break cleanly around the score mark and the remaining portion shall not have protrusions exceeding 1/32 inch.

3.9 Preproduction. Prior to the start of regular production, a preproduction lot of detector tubes shall be produced for examination and test in accordance with 4.3.

3.10 Workmanship. The detector tubes shall not be cracked, chipped, or broken. They shall be free from foreign matter and uniform in thickness with sealed ends which are smoothly rounded.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection.

4.1.1 Supplier's responsibility. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to specified requirements.

4.1.2 Objective evidence. The supplier shall provide objective evidence acceptable to the contracting officer that the requirements of 3.1, 3.2 and section 5 for which specific inspection has not been provided in this specification have been satisfied.

4.2 Classification of inspections. The inspection requirements specified herein are classified as follows:

(a) Preproduction inspection (see 4.3)
(b) Quality conformance inspection (see 4.4)

4.3 Preproduction inspection.

4.3.1 Lotting. A preproduction lot of 300 of each type of detector tube shall be manufactured using the same methods, materials, equipment and processes as will be used during regular production (see 4.4.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

4.3.2 Sampling.

4.3.2.1 For examination and nondestructive test. Sampling for each type of detector tube shall be conducted in accordance with MIL-STD-105. For leakage test, level S-4 shall be used.

4.3.2.2 For destructive tests. Sampling for each type of detector tube shall be conducted in accordance with table IV.

4.3.3 Inspection procedure.

4.3.3.1 For examination and nondestructive test. The sample detector tubes of each type shall be examined for all requirements of the applicable drawings, the classification of defects and MIL-STD-105. Test shall be conducted in accordance with 4.4.4.1 and table IV.

4.3.3.2 For destructive tests. Sample detector tubes of each type shall be tested in accordance with 4.4.4.2 through 4.4.4.6 and table IV.

4.3.4 Acceptance/rejection criteria. The preproduction sample shall meet the requirements of 4.3.3.1 and, when tested in accordance with 4.4.4, shall comply with the acceptance numbers listed in table IV to be acceptable.

4.4 Quality conformance inspection.

4.4.1 Lotting. A lot shall consist of the tubes of the same type assembled into the same size clip by one manufacturer from the same materials and under essentially the same manufacturing conditions. However, one lot of tubes shall contain no more than one lot of gel and shall have been filled within five consecutive working days. All tubes shall be sealed the same day they are filled.

4.4.2 Sampling.

4.4.2.1 For examination and nondestructive test. Sampling shall be conducted in accordance with MIL-STD-105. For leakage test, level S-4 shall be used.

4.4.2.2 For destructive tests. Sampling shall be conducted in accordance with table IV.

4.4.3 Inspection procedure.

4.4.3.1 For examination and nondestructive test. Sample detector tubes of each type shall be examined in accordance with the classification of defects and MIL-STD-105. Tests shall be conducted in accordance with 4.4.4.1 and table IV.

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

4.4.3.2 For destructive tests. Sample detector tubes of each type shall be tested in accordance with 4.4.4.2 through 4.4.4.6 and table IV.

Table IV. Sampling plan

Requirement	Sample Size	Acceptance number	Test paragraph
Leakage	MIL-STD-105, level S-4	AQL 1.0 percent defective	4.4.4.1
Airflow resistance			4.4.4.2
Dwg C5-77-784	MIL-STD-105, level S-4	AQL 2.5 percent defective	
Dwg C5-77-820	MIL-STD-105, level S-4	AQL 2.5 percent defective	
Dwg C5-77-387	MIL-STD-414	AQL 0.1 percent variability unknown, standard deviation method, double specification limit.	
Volatile matter	48 tubes (for lot size of 10,000 and under)	0 defective	4.4.4.3
	96 tubes (for lot size over 10,000)	1 defective	4.4.4.3
Stability and sensitivity	50 tubes *	3 defectives	4.4.4.4, 4.4.4.5
Score breakage			
a. machine break	MIL-STD-105, level S-4	AQL 2.5 percent defective	4.4.4.6(a)
b. hand break	MIL-STD-105, level S-4	AQL 2.5 percent defective	4.4.4.6(b)

*Twenty-five tubes shall be tested for stability aged, and sensitivity aged. Twenty-five tubes shall be tested for stability unaged and sensitivity unaged.

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

4.4.3.3 Classification of defects.

(a) Tubes, detector, assembly and detail (Drawing D5-77-446).

Categories		Defects
Critical:		None defined
Major:	AQL	1.0 percent defective
101		Component missing or incorrectly assembled
102		Gel length
103		Length of charcoal (type II only)
104		Scored line missing, incomplete or incorrectly located
105		Workmanship (3.10)
Minor:	AQL	2.5 percent defective
201		Overall tube length
202		Color bands missing or incorrectly located
203		Paint sticky or tubes stuck together

(b) Clips, detector tube (Drawing C5-77-387).

Categories		Defects
Critical:		None defined
Major:	AQL	1.0 percent defective
101		Number of tubes
102		Marking incorrect or missing
103		Workmanship (3.10)

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

(c) Dispenser, filled (Drawing C5-77-784).

Categories	Defects
Critical:	None defined
Major:	AQL 1.0 percent defective
101	Number of tubes
102	Marking incorrect or missing
103	Workmanship (3.10)

(d) Clips, detector tube (Drawing C5-77-820).

Categories	Defects
Critical:	None defined
Major:	AQL 1.0 percent defective
101	Number of tubes
102	Marking incorrect or missing
103	Workmanship (3.10)

4.4.4 Tests. Water in accordance with ASTM D1193 and reagent grade chemicals shall be used throughout the tests, which shall be conducted as follows:

4.4.4.1 Leakage. Place the tubes in a vacuum desiccator and apply a vacuum of 5 inches of mercury. Close the stopcock and maintain the vacuum for 30 minutes. At the end of this period, draw in sufficient colored water (0.1 g 3,3'-dibromothymolsulfonphthalein and 8.0 milliters (ml) N/50 sodium hydroxide per 2.5 liters) to cover the tubes. Release the vacuum. Wait 5 minutes and examine each tube for evidence of water penetration.

4.4.4.2 Airflow resistance. Determine the airflow resistance of each tube with Q34 (Drawing DL 136-14-360) and a flow rate of 100 ml per minute.

4.4.4.3 Volatile matter. Remove the gel from 16 tubes. Composite and weigh to the nearest milligram (mg) in a tared weighing bottle. Dry in an oven at 150° ± 5°C for 3 hours ± 5 minutes. Determine the loss in weight. Perform the test on each group of 16 tubes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

4.4.4.4 Stability. Examine the gel layer of each tube and record its hue, value, and chroma. Continue as directed in 4.4.4.5.

4.4.4.5 Sensitivity. Determine sensitivity using a flow rate of 1 liter per minute and an exposure time of 30 to 60 seconds (see 6.3).

(a) Apparatus and reagents.

Dilution Apparatus, Toxic Gas, Q5, (Drawing IL 136-41-780)
Sodium hydroxide solution - 8.5 + 0.5%
Compound 34-pyrophosphate peroxide solution:
2.5 mg compound 34 - MIL-T-51023
200 mg sodium pyrophosphate peroxide - MIL-P-50014
8 ml water.

(b) Blank. Select 8 tubes at random from the sample. Break off the ends of each tube and add 2 drops of sodium hydroxide solution to each tube. After two minutes, determine the Munsell color of the gel layer.

(c) Type I. Use half of the tubes for each test.

(1) Sensitivity to mustard. Break off the ends of each tube and expose the gel to 0.5 microgram (µg) H. Remove the tube from the apparatus, wait 2 minutes, then add 2 drops of sodium hydroxide solution. Examine the gel layer. Record the color and reaction time.

(2) Sensitivity to G-agent. Break off the ends of each tube and expose the gel to 1.0 µg GB. Remove the tube from the apparatus and add 2 drops of compound 34-pyrophosphate peroxide solution. Examine the gel layer. Record the color and reaction time.

(d) Type II. Break off the ends of each tube and expose the gel to 8.0 µg AC. Remove the tube from the apparatus and examine the gel layer. Record the color and reaction time.

(e) Type III. Break off the ends of each tube and expose the gel to 12.0 µg CG. Remove the tube from the apparatus and examine the gel layer. Record the color and reaction time.

(f) Type IV. Break off the ends of each tube and expose the gel to 10.0 µg L. Remove the tube from the apparatus and add 2 drops of sodium hydroxide solution. Examine the gel layer. Record the color and reaction time.

(g) Type V. Break off the ends of each tube and expose the gel to 10.0 µg CN. Remove the tube from the apparatus and add 2 drops of sodium hydroxide solution. Examine the gel layer. Record the color and reaction time.

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

(h) Type VI. Break off the ends of each tube and expose the gel to 12.0 µg CN. Remove the tube from the apparatus and add 2 drops of sodium hydroxide solution. Examine the gel layer. Record the color and reaction time.

(i) Type VII. Determine the sensitivity in accordance with 4.4.4.5(c)(2).

4.4.4.6 Score breakage.

(a) Machine breakage. Determine the score breakage on each end of the tubes using the apparatus shown in figure 1.

(b) Hand breakage. Break both ends of the tubes at the score mark by hand. Observe for compliance with 3.8.

5. PREPARATION FOR DELIVERY

5.1 Packaging, level C. The detector tube assemblies of the same type and size shall be packaged to provide adequate protection against corrosion, deterioration, and damage from the supply source to the first receiving activity for immediate use.

5.2 Packing, level C. Detector tube assemblies, packaged as specified in 5.1, shall be packed to insure carrier acceptance and safe delivery to the first domestic destination. Containers shall be in compliance with Uniform Freight Classification rules or the regulations of other common carriers applicable to the mode of transportation.

5.3 Marking. In addition to any special marking required by the contract or order, unit packages, intermediate packages, and shipping containers shall be marked in accordance with MIL-STD-129.

5.4 Repair part. When type I and VII detector tubes are procured for storage and issue as a repair part, preservation, packaging, packing and marking shall be as specified on the packaging data sheet which is identified by the Federal Stock Number.

6. NOTES

6.1 Intended use. The items covered by this specification are intended for use in the sampling and detection of chemical agents.

6.2 Ordering data. Procurement documents should specify the following:

(a) The title, number, and date of this specification.
(b) The applicable assembly drawing.
(c) Preproduction.

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

(NOTES FOR FIG. 1)

1. METHOD OF OPERATION


THE DETECTOR TUBE IS INSERTED IN THE TUBE HOLDER (G) UNTIL THE SCRIBED MARK IS LINED UP WITH THE POINTER (A). THE LEVER ARM IS GRADUALLY LOWERED ONTO THE DETECTOR TUBE, MAKING CONTACT AT POINT (E).

2. DESIGN OF TEST DEVICE

THE DEVICE IS SO DESIGNED THAT THE MOVABLE WEIGHT WHEN PLACED ON 2 SELECTED POSITIONS WILL PRODUCE THE 2 REQUIRED LOADS AS SPECIFIED ON THE TUBE AT POINT (E). ANY COMBINATION OF LEVER ARM LENGTH AND WEIGHT THAT WILL PRODUCE THE REQUIRED LOADS IS ACCEPTABLE. THE LEVER ARM SHALL BE PARALLEL TO THE BASE WHEN TOUCHING THE TUBE JUST BEFORE THE FULL LOAD IS APPLIED.

3. CALIBRATION OF TEST DEVICE

THE TEST DEVICE MAY BE CALIBRATED BY MOVING THE WEIGHT SO THAT THE REQUIRED LOAD IS PRODUCED ON THE SPRING SCALE PLACED AT (E). THE POSITION OF THE WEIGHT SHOULD BE PERMANENTLY MARKED. REPEAT THE CALIBRATION PROCEDURE FOR THE SECOND REQUIRED LOAD.

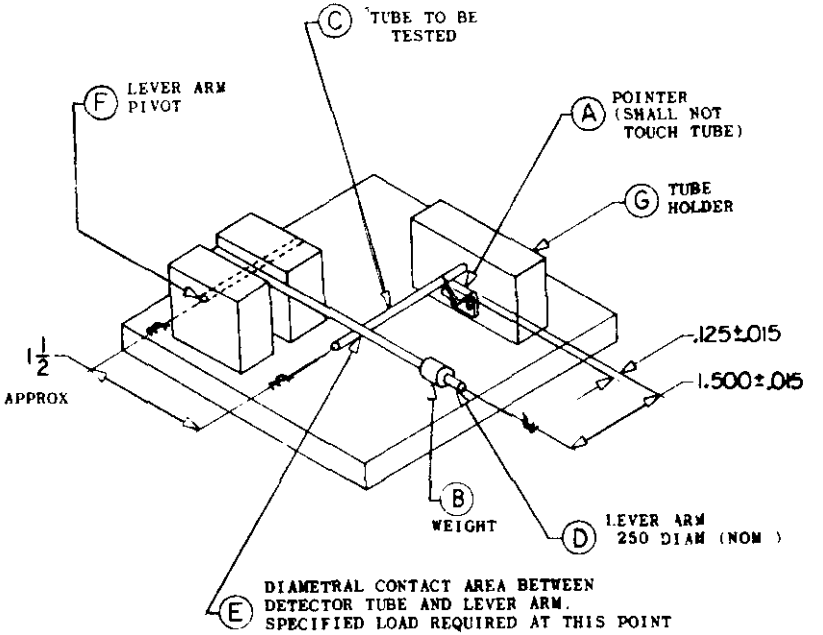

CALIBRATION

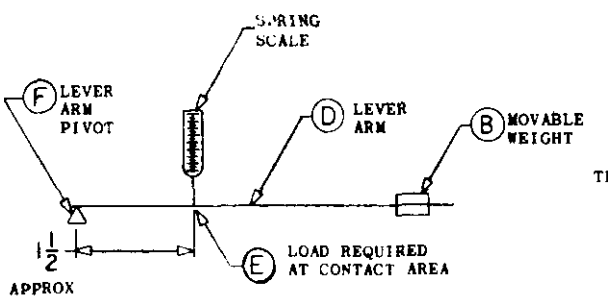


Figure 1
TEST DEVICE, BREAKING POINT DETECTOR TUBES

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

(1) Time allowed for supplier submission of samples for Government test and evaluation after award of contract.
(2) Name and address of test facility and shipping instructions when testing is performed by the Government.
(3) Time required for the Government to notify the supplier whether or not to proceed with production.

6.3 Precautions. Special care must be exercised in the handling of mustard, G-agents, hydrogen cyanide, phosgene, arsenicals, and chloroacetophenone. Tests involving any of these substances should be conducted in a well-ventilated fume hood. A protective mask and rubber gloves should be used when necessary. If any agent (either in pure form or in solution) spills on the clothing or skin, the affected area should be washed immediately and thoroughly with cold, soapy water.

6.4 Manufacture and protection of gels and unsealed tubes. Edgewood Arsenal Directive No. 631 gives suggested methods for preparing impregnated gels. All gels and unsealed tubes containing gels should be protected from organic vapors, such as those emanating from lacquer, paint, cement, and solvents. Testing of unsealed tubes should be conducted as rapidly as possible. This should be done in an air-conditioned room low in humidity and free from dust and organic vapors.

6.5 Charcoal. Before use, the charcoal should be dried in 1/2 inch layers at 150° + 5°C for 24 hours, cooled in a closed container, humidified with 0.4 ml of distilled water per gram of charcoal, blended until free of lumps, and stored in a closed container for 35 hours.

6.6 Significant places. For the purpose of determining conformance with this specification, an observed or calculated value shall be rounded off "to the nearest unit" in the last right-hand place of figures used in expressing the limiting value, in accordance with the rounding-off method of the Recommended Practices For Designating Significant Places in Specified Limiting Values (ASTM E29).

6.7 Suggested source: Dye, DuPont TLA #35 has been found to be satisfactory.

6.8 International interest. Certain provisions of this specification are the subject of international standardization agreement ABCA-ARMY-STD-94. When amendment, revision, or cancellation of this specification is proposed which will affect or violate the international agreement concerned, the preparing activity will take appropriate reconciliation action through international standardization channels including departmental standardization offices, if required.

Custodians:

Army - MU

Preparing activity:

Army - MU (EA)

International interest (see section 6)

Project No. 6665-A242

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

(NOTES FOR FIG. 1)

1 METHOD OF OPERATION


THE DETECTOR TUBE IS INSERTED IN THE TUBE HOLDER (G) UNTIL THE SCRIBED MARK IS LINED UP WITH THE POINTER (A). THE LEVER ARM IS GRADUALLY LOWERED ONTO THE DETECTOR TUBE, MAKING CONTACT AT POINT (E).

2. DESIGN OF TEST DEVICE

THE DEVICE IS SO DESIGNED THAT THE MOVABLE WEIGHT WHEN PLACED ON 2 SELECTED POSITIONS WILL PRODUCE THE 2 REQUIRED LOADS AS SPECIFIED ON THE TUBE AT POINT (E). ANY COMBINATION OF LEVER ARM LENGTH AND WEIGHT THAT WILL PRODUCE THE REQUIRED LOADS IS ACCEPTABLE. THE LEVER ARM SHALL BE PARALLEL TO THE BASE WHEN TOUCHING THE TUBE JUST BEFORE THE FULL LOAD IS APPLIED.

3. CALIBRATION OF TEST DEVICE

THE TEST DEVICE MAY BE CALIBRATED BY MOVING THE WEIGHT SO THAT THE REQUIRED LOAD IS PRODUCED ON THE SPRING SCALE PLACED AT (E). THE POSITION OF THE WEIGHT SHOULD BE PERMANENTLY MARKED. REPEAT THE CALIBRATION PROCEDURE FOR THE SECOND REQUIRED LOAD.

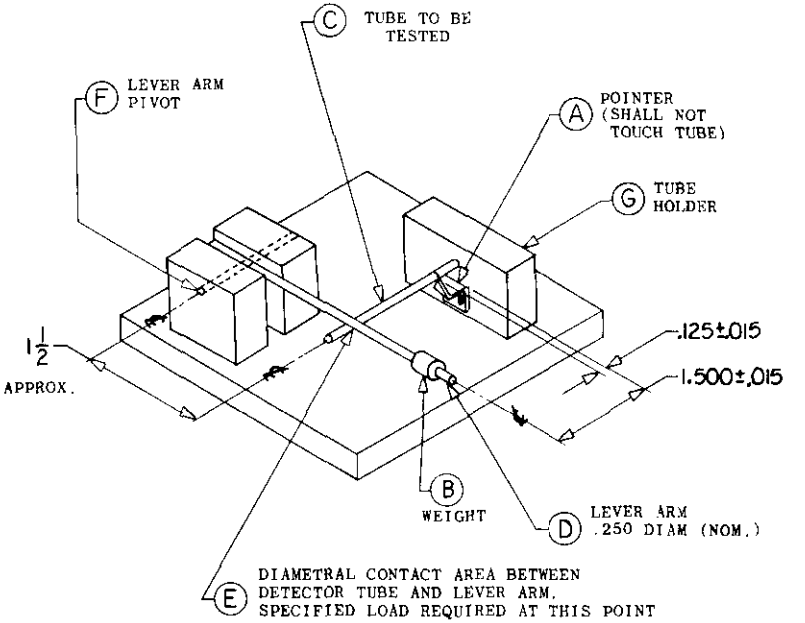

CALIBRATION:

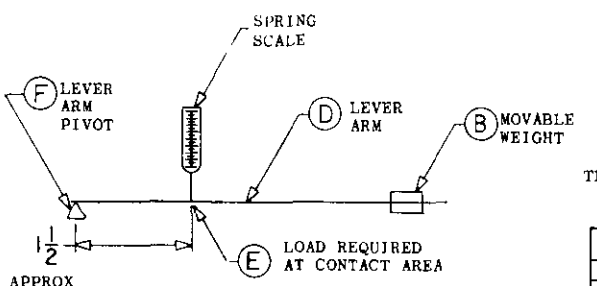


Figure 1
TEST DEVICE, BREAKING POINT, DETECTOR TUBES

PART OF SPEC	CHEMICAL CORPS SPECIFICATION FIGURE
MIL-D-51082	
	DATE 19 OCT 64 / B18-60-1015

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

FOLD

POSTAGE AND FEES PAID

OFFICIAL BUSINESS

Commanding Officer
Edgewood Arsenal
ATTN: SMUEA-QAES
Edgewood Arsenal, Maryland 21010

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.

TO DETACH FORM T ON THIS LINE

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)* | DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 64 WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-22T20:50Z
Check the source to verify that this is the current version before use.