COMMERCIAL ITEM DESCRIPTION

TUBE, COLON, SURGICAL (Disposable)

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-T-36264A.

This commercial item description covers a colon tube suitable for irrigation of the human colon.

Salient characteristics:

Material. The colon tube shall be fabricated from flexible polyvinyl chloride suitable for the intended purpose.

Toxicity. The colon tube shall be non-toxic when tested as specified in American Society for Testing and Materials (ASTM) F749, Method B.

Pyrogenicity. The colon tube shall be non-pyrogenic when tested as specified in the latest edition of the United States Pharmacopeia (USP).

Style and design. Style and design of the colon tube shall conform to Figure 1 (colon tube with fitted connector). As an alternate, colon tube style and design may conform to Figure 2 (colon tube with integral connector). The proximal connector (integral or fitted) shall be suitable for effecting a connection between the tube and any size 28 French tube. The fitted connector shall not separate from the colon tube when subjected to a 15 lb. tensile load. The colon tube shall be size 28 French. All edges on the tube and connector shall be suitably dulled or rounded.

Sterility. The colon tube, if supplied sterile, shall pass the sterility test specified in the latest edition of the United States Pharmacopeia (USP).

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

AMSC N/A

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:55Z
Check the source to verify that this is the current version before use.

Thermal stability. The colon tube, if supplied non-sterile, shall pass the thermal stability test listed below.

Thermal stability test. Sample colon tubes will be subjected to cyclic steam autoclaving at 250 ± 5° F, 15 ± 1 psig. A total of 10 cycles, 30 minutes ± seconds per cycle, must be used. After each cycle, the colon tube will be examined for any sign of brittleness, blistering, swelling, peeling, or cracking.

Workmanship. The colon tube shall be free from any defects that detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing 50 individually packaged colon tubes, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one colon tube.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-00-064-0951	Tube, Colon, Surgical, Disposable, 28 Fr, 50s

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:55Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITY

VA-OSS

44546

Project No. 6515-3336

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.

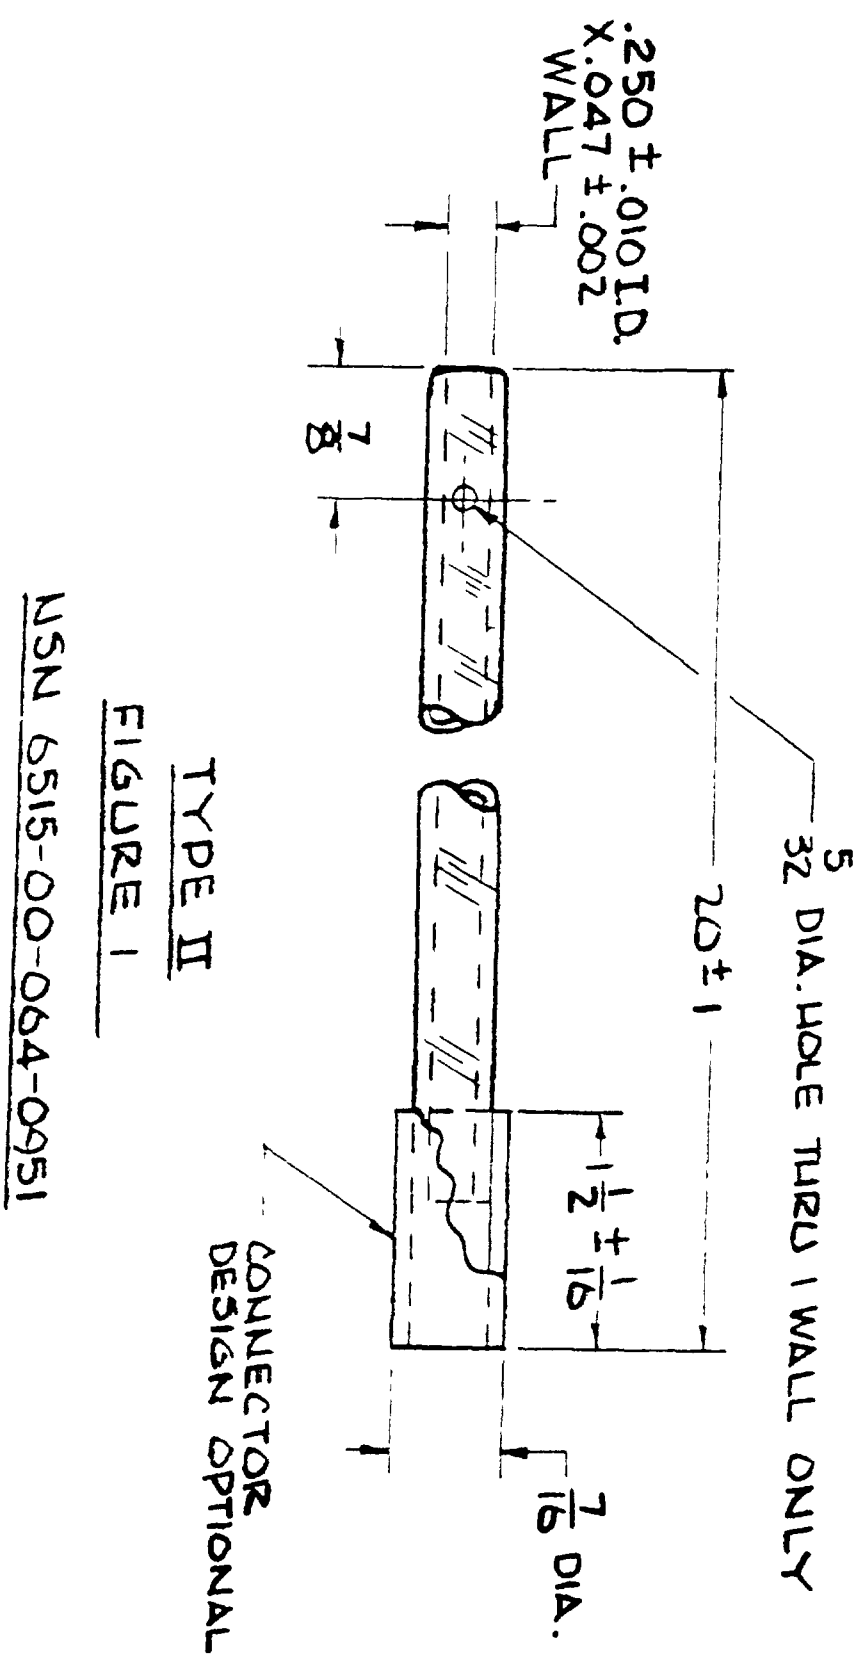


TYPE II

FIGURE 1

NSN 6515-00-064-0951

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.

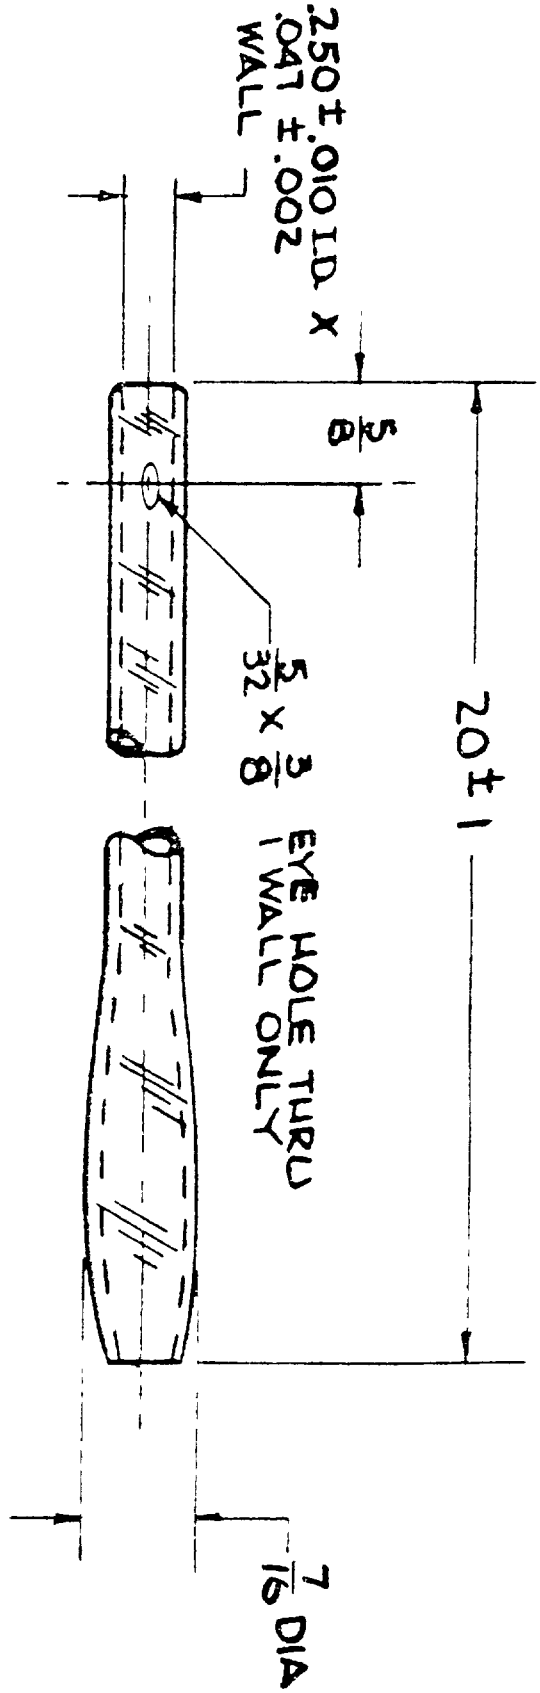

TYPE I

FIGURE 2

NSN 6515-01-064-0951

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.