INCH-POUND

A-A-54623
30 April 1992

COMMERCIAL ITEM DESCRIPTION

MASK, TRACHEOSTOMY, Plastic, Disposable

The General Services Administrations has authorized the use of this commercial item description.

This commercial item description covers one type of disposable, plastic tracheostomy, mask suitable for tracheostomy and laryngectomy patient requiring administration of oxygen, air, or aspiration.

Salient Characteristic.

General. The tracheostomy mask shall consist of a pliable plastic mask, a rigid plastic elbow, and an adjustable elastic neckband, all preassembled.

Material. Plastic used for the mask proper shall be transparent and of a natural color. As an alternate, the mask may be of a non-dermatitic, green transparent polyvinyl chloride.

Elbow plastic. Plastic used for the elbow shall be of rigid, clear, transparent styrene acrylic nitrile.

Style, design and dimensions. The complete mask shall be in accordance with Figure 1 for style, design and dimensions.

Mask. The mask shall be anatomically contoured to fit the human neck. Edges of the mask in contact with the neck shall be curved or rolled to provide a smooth comfortable fit. The mask shall be constructed to retain the rigid elbow securely and shall have wings to accept the neckband. One wing shall have a male strap fastener component permanently to the outside of the wing. The other wing shall have a perforation to hold the neckband securely after adjustment. As an alternate, the elastic band may be attached to the wings by removable ball and clip fastener. Buckles shall be provided to permit adjustment of the neck band in a secure manner.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Elbow. The rigid plastic elbow shall be securely retained in the center of the pliable mask and shall be capable of 360 degree rotation. The elbow shall have a front hole in the center to permit aspiration of the patient without removal of the mask. The front hole shall be between 7/16 and 9/16 inch in diameter. The right angle inlet tubing adapter of the elbow shall have an approximate minimum length of 5/8 inch and shall have a 13/16 inch outside diameter and nominal 3/4 inch inside diameter to provide an airtight fit when connected to corrugated plastic tubing with an elastic plastic end of 3/4 inch inside diameter.

Neckband. The adjustable elastic neckband shall be 18 to 30 inches long. One end of the band shall be inserted through the perforated mask wing from the underside and shall have a metal clip attached to the external end of the band to prevent accidental removal from the mask wing. The other end shall be fitted with an appropriate female snap fastener component to mate with the male component on the mask wing.

Instructions. The tracheostomy mask shall be complete with instructions for use.

Workmanship. The mask and elbow shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package. (PG) One package containing fifty (50) tracheostomy masks, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract of purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination and testing. Examination shall be conducted on the mask in accordance with commercial practice. The sampling for examination shall be in accordance with commercial practice.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-00-915-4141	MASK, TRACHEOSTOMY, Plastic, Disposable, 50

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5330
Location:\word\seto\mask


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

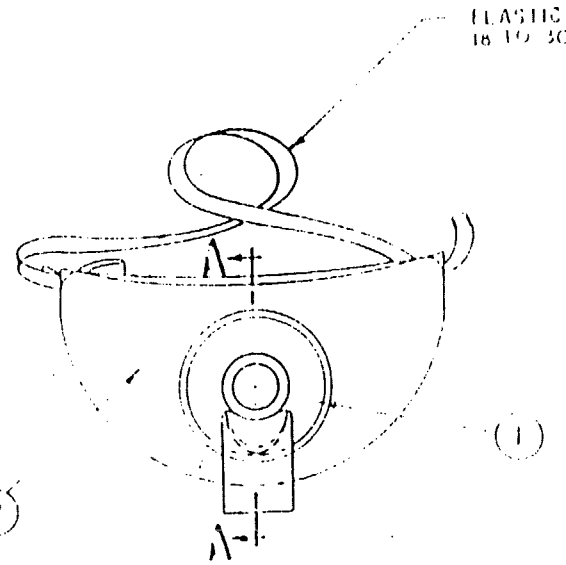

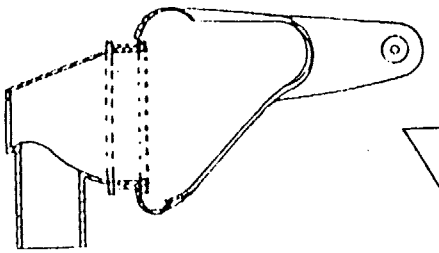

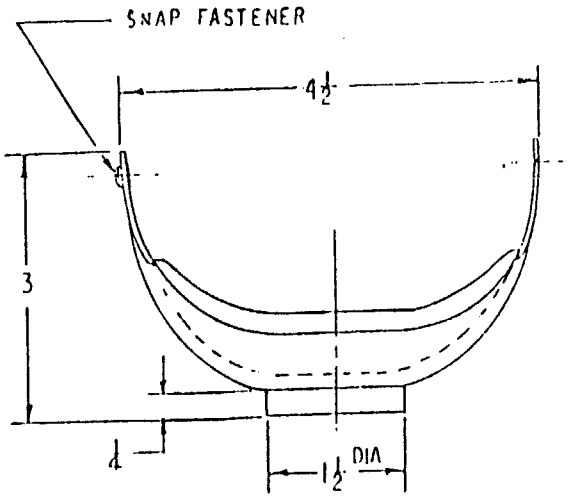

② MASK

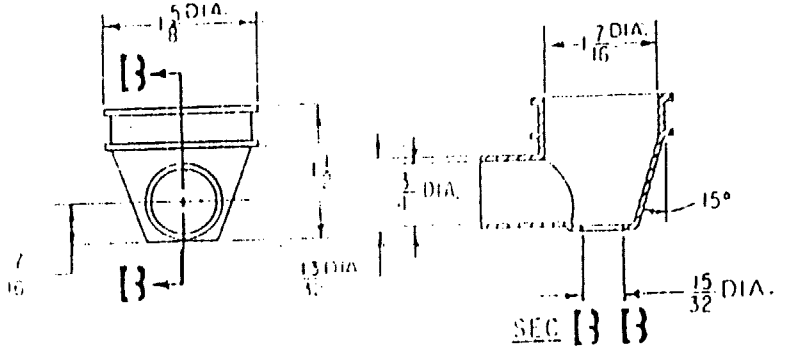

① TURRET

NSN 6515-00-915-4141

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES

FIGURE 1 TRACHEOTOMY MASK, DISPOSABLE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54623	30 April 1992

3. DOCUMENT TITLE

MASK, TRACHEOSTOMY, Plastic, Disposable

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code)	
Defense Personnel Support Center ATTN: DPSC-MSE	(1) Commercial (215)737-2870	(2) AUTOVON 444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.