INCH-POUND

A-A-54673
15 June 1992

COMMERCIAL ITEM DESCRIPTION

DRAIN, SURGICAL, Rubber, Whistle Tip, Right Angle, 13 Inches Long, 3-1/2 Inch Leg

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-D-36847 which is cancelled.

This commercial item description covers right angle rubber surgical drains with whistle tips and one eye, for use in surgical procedures.

Salient characteristics:

Classification. This specification covers the following sizes of surgical drains:

Size 40 French
Size 45 French

The specific size drain to be provided for each stock number is indicated under notes..

General. The drain shall be molded or dip formed in one piece to have one long leg and one short leg at right angles to the long leg. The short leg shall have a whistle tip and an eye.

Material. Material of the drain shall be fabricated of high grade rubber latex free from coloring matter or fillers.

Style, design and dimensions. The surgical drains shall be in accordance with Figure 1 for style, design and dimensions. The French Size and inside diameter shall be measured at the proximal end (on short leg) of the drain.

Pyrogens, safety and biological tests. The drain shall meet the United States Pharmacopeia (USP) requirements for pyrogens, safety and Class IV biological tests.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Physical properties. The drains shall have a tensile strength of 4500 psi and ultimate elongation of 750 percent when tested in accordance with ASTM D412 Tension Testing of Vulcanized Rubber.

Sterilization. The drain shall show no signs of deterioration after steam autoclaving for 20 minutes at 250°F and 15 psig.

Resistance to aging. The tensile strength and ultimate elongation of the surgical drains shall not decrease by more than 25 percent of the values before aging nor shall the rubber latex become tacky or brittle when tested as described in ASTM 573.

Marking. The drain shall be permanently and legibly marked with name or trademark of manufacturer, date of manufacture, angle by size and French size.

Workmanship. The surgical drain shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One surgical drain of the French size specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract of purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one surgical drain as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one surgical drain. Sampling shall be inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
-Check the source to verify that this is the current version before use.-

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers and their respective Item Identifications are covered by this document:

NATIONAL STOCK NUMBERS	ITEM IDENTIFICATIONS
6515-00-131-6985	DRAIN, SURGICAL, Rubber, Whistle Tip, Right Angle, 40 Fr.
6515-00-131-6991	DRAIN, SURGICAL, Rubber, Whistle Tip, Right Angle, 45 Fr.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5415
Location: c:\word\nish\drain3cd

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

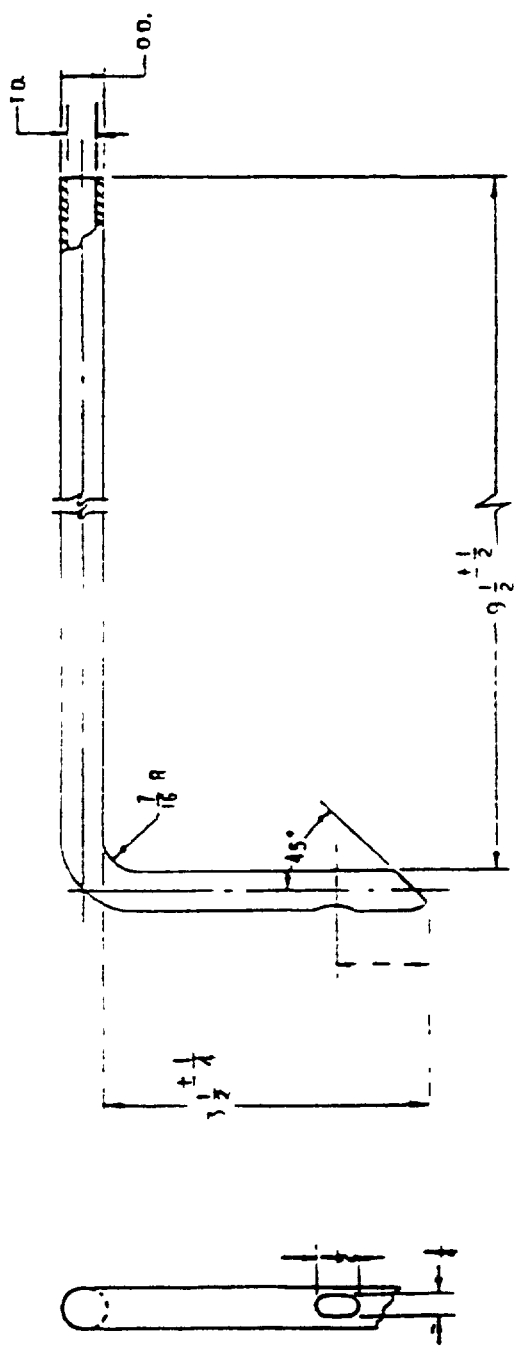

NSN	FR SIZE	I.D.	O.D.
6515-00-131-6385	40	.310	.525
6515-00-131-6391	45	.344	.591

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES
TOLERANCES ON
FRACTIONS ± 1/16 DECIMALS .xxx ± .015 ANGLES ± 5°

FIGURE 1 DRAIN, SURGICAL, ANGULATED WHISTLE TIP

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
	A-A-54673	15 June 1992

3 DOCUMENT TITLE
DRAIN, SURGICAL, Rubber, Whistle Tip, Right Angle, 13 Inches Long, 3-1/2 Inch Leg

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)
	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	215-737-2870 444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 Previous editions are obsolete

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.