INCH-POUND

A-A-54683
19 June 1992

COMMERCIAL ITEM DESCRIPTION

HOLDER, SUTURE NEEDLE, DEBAKEY

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-H-37011A which is cancelled.

This commercial item description covers one type of suture needle holder that is suitable for use in surgical operating procedures of the heart.

Salient characteristics:

General. The suture needle holder shall be straight and have serrated inserts that are brazed to the jaw with a uniform flow of silver-solder that is free of crevices at all interfaces. As an alternate, the serrated inside surfaces of the jaws shall be flame plated with a deposit of tungsten carbide material. Thickness of the plating shall be 0.004 ± 0.001 inch. The suture needle holder shall be of the DeBakey design and be of the following sizes:

SIZE	LENGTH (In Inches)
1	7
2	9
3	10
4	12

Material. The suture needle holder shall be fabricated from class 4, Type 420 martenestic corrosion-resistant steel in accordance with ASTM F899. Jaw insert shall be fabricated of tungsten carbide material that is suitable for the purpose intended.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Hardness. The suture needle holder shall have a Rockwell Hardness C Scale (HRC) of 48 to 55 when tested for hardness in accordance with ASTM E18 or E92 whichever is applicable. The tungsten carbide jaw inserts of the suture needle holder shall have a Rockwell Hardness A Scale (HRA) of 80 to 100 when removed from the jaw of the completed instrument and tested for hardness in accordance with ASTM E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM E140.

Style, design and dimensions. The suture needle holder shall be in accordance with Figure 1 for style, design and dimensions.

Performance. The suture needle holder shall meet applicable requirements as per ASTM F1026 and F1325.

Finish. The suture needle holder shall have a mirror, satin or matte finish.

Passivation The suture needle holder shall be properly passivated.

Corrosion resistance. The suture needle holder shall show no evidence of corrosion when tested in accordance with ASTM F1089.

Identification markings. The suture needle holder shall be legibly marked with the contractor's name or registered trademark and the word "stainless". Foreign manufactured suture needle holder shall bear the name of the country of origin.

Workmanship. The suture needle holder shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One suture needle holder of the size specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:37Z
Check the source to verify that this is the current version before use.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. unit of product for examination purposes shall be one suture needle holder. Sampling shall be Inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one suture needle holder. Sampling shall be Inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Contractor Certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered material. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:37Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

NOTE: The following National Stock Numbers are covered by this document:

NSN	Item Identification	Size
6515-00-690-3198	HOLDER, SUTURE NEEDLE, DeBakey, 7 Inch.	1
6515-00-690-3200	HOLDER, SUTURE NEEDLE, DeBakey, 9 Inch.	2
6515-00-690-3201	HOLDER, SUTURE NEEDLE, DeBakey, 10 Inch.	3
6515-00-690-3202	HOLDER, SUTURE NEEDLE, DeBakey 12 Inch.	4

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS


Project No. 6515-5255

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

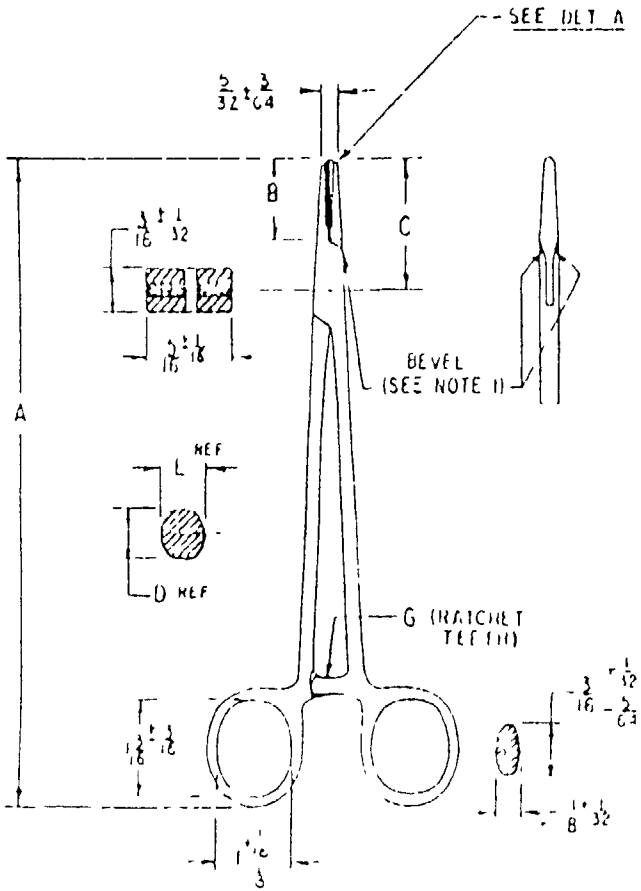

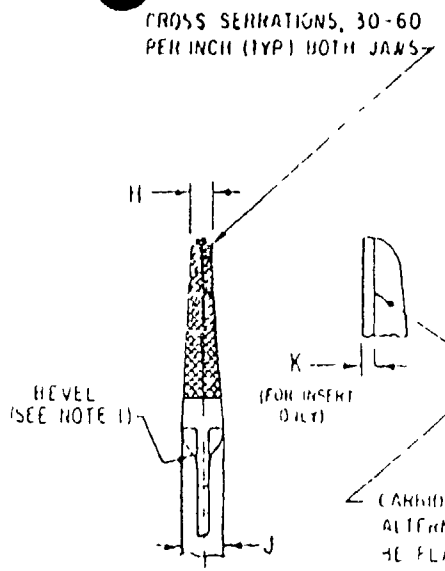

DET A
CARBIDE INSERT
(MALE JAW)

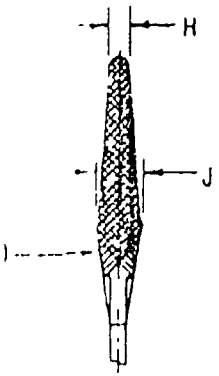

VIEW OF JAW
FLAME PLATED
(MALE JAW)

SIZE	NSN	A ±1/32	B ±1/16	C ±1/32	D REF	E REF	G SEE BELOW	H ±.012 BOTH JAWS	J SEE BELOW BOTH JAWS	K ±.005
1	6515 00 690-3198	7 1/8	7/8	1 1/4	7/64	1/8	3/32 x 3/32 or 4 x 4	069	.156 +.041	015
2	6515 00 690 3200	9	1	1 5/16	7/64	1/8	4 x 4	069	.166 +.032	015
3	6515 00 690 3201	10	1	1 7/16	1/8	5/32	4 x 4	069	.176 +.022	031
4	6515 00 690 3202	12	1	1 7/16	11/64	5/32	4 x 4	069	.186 +.012	.031

NOTES

1. BEVEL SHALL BE PROVIDED ON BOTH SIDES OF THE DISTAL EDGE OF THE RACE MEMBER OF THE JAW, ADJACENT TO THE LOCK.
2. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY, AND FIRST QUALITY WORKMANSHIP.

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES

FIGURE 1 HOLDER, SUTURE NEEDLE, DeBAKEY

Source: https://assist.dla.mil -- Downloaded: 2026/0-26T09:37Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54683	2 DOCUMENT DATE (YYMMDD) 19 June 1992

3 DOCUMENT TITLE HOLDER, SUTURE NEEDLE, DeBAKEY

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME Defense Personnel Support Center	b TELEPHONE (Include Area Code) (1) Commercial (215) 737-2870 (2) AUTOVON 444-2870
c ADDRESS (Include Zip Code) ATTN: MSE 2800 S. 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403, Falls Church, VA 22041 3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 Previous editions are obsolete

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T09:37Z
Check the source to verify that this is the current version before use.