INCH-POUND

A-A-54684
19 June 1992

# COMMERCIAL ITEM DESCRIPTION

## CONTRACTOR, RIB, BAILEY

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-C-36767 which is cancelled.

This Commercial Item Description covers one type of rib contractor suitable for use in thoracic surgery.

Salient characteristics:

General. The rib contractor shall be of the double rake type, having thumbscrew control that is capable of regulating the inter-rake distance and ratchet locking device, be of the Bailey design and be suitable for use during surgical procedures in thoracic surgery to approximate ribs prior to closure of the operative incision.

Material. The rib contractor components comprising of the pawl, slide, jaws, handle and screws shall be fabricated from class 3, austenitic corrosion-resistant steel in accordance with ASTM F899. The rib contractor rack and pinion shall be fabricated from class 4, type 420 martensitic corrosion-resistant steel in accordance with ASTM F899. As an alternate, the rib contractor pinion shall be fabricated from class 4, type 440A martensitic corrosion-resistant steel in accordance with ASTM F899.

Hardness. The rib contractor components fabricated of class 3 material shall have a Rockwell Hardness (HRB) scale of 75 to 90. Components fabricated of class 4, type 420 material shall have a Rockwell Hardness (HRC) scale of 48 to 55, and components fabricated of class 4, type 440A material shall have a Rockwell Hardness (HRC) scale of 50 to 56 when tested for hardness in accordance with ASTM E18 or E92 whichever is applicable. Conversion of hardness values shall be done in accordance with ASTM E140.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Style, design and dimensions. The rib contractor shall be in accordance with figure 1 for style, design and dimensions.

Performance. The rack and pinion teeth shall mesh completely when the rib contractor is assembled and ready for use. Under no circumstances shall looseness or free play permit misalignment of the rack and pinion teeth.

Finish. The rib contractor shall have a mirror or satin finish.

Passivation. The rib contractor shall be properly passivated.

Corrosion resistance. The rib contractor shall show no evidence of corrosion or plating of copper when tested in accordance with ASTM F1089.

Identification marking and labeling. The rib contractor shall be legibly marked with the contractor's name or registered trademark and the word "stainless". Foreign manufactured rib contractors shall bear the name of the country of origin.

Workmanship. The rib contractor shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One rib contractor, of the size specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as specified herein. Unit of product for examination purposes shall be one rib contractor. Sampling shall be Inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one rib contractor. Sampling shall be Inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more text characteristics.

Contractor Certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

| NSN | Item Identification |
|---|---|
| 6515-00-320-8500 | CONTRACTOR, RIB, Bailey |

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5246



Source: https://assist.dla.mil -- Downloaded: 202640-26T09:37Z
Check the source to verify that this is the current version before use.

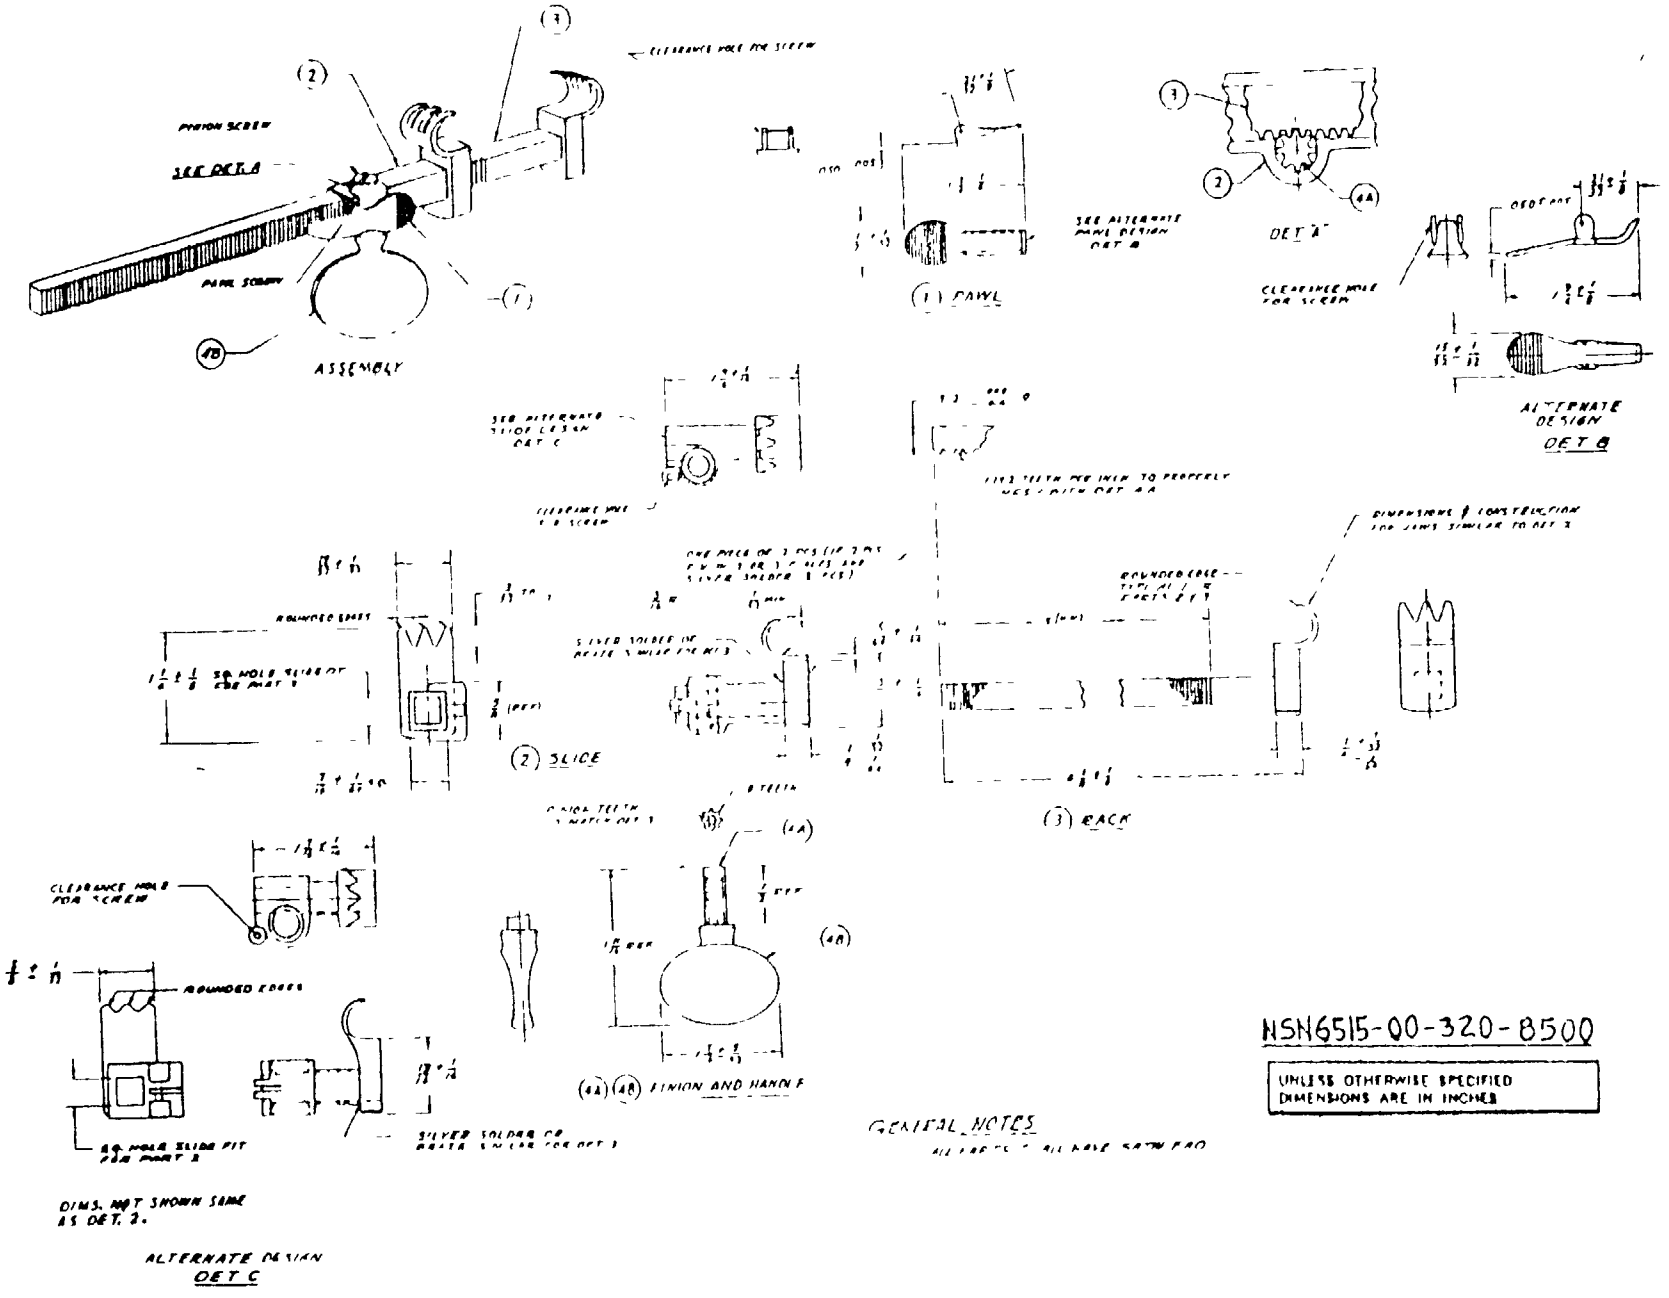



FIGURE 1 CONTRACTOR, RIB, BAILY

Source: https://assist.dla.mil -- Downloaded: 2026-02-26T09:37Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

## INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3 and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

| I RECOMMEND A CHANGE. | 1. DOCUMENT NUMBER<br>A-A-54664 | 2. DOCUMENT DATE (YYMMDD)<br>19 June 1992 |
|---|---|---|

3. DOCUMENT TITLE
CONTRACTOR, RIB, BAILEY

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

| a. NAME (Last, First, Middle Initial) | b. ORGANIZATION | |
|---|---|---|
| c. ADDRESS (Include Zip Code) | d. TELEPHONE (Include Area Code)<br>(1) Commercial<br>(2) AUTOVON<br>(If applicable) | 7. DATE SUBMITTED (YYMMDD) |

8. PREPARING ACTIVITY

| a. NAME<br>Defense Personnel Support Center<br>ATTN: MSE | b. TELEPHONE (Include Area Code)<br>(1) Commercial: (215)737-2870<br>(2) AUTOVON: 444-2870 |
|---|---|
| c. ADDRESS (Include Zip Code)<br>2800 S. 20th Street<br>Philadelphia, PA 19145 | IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT:<br>Defense Quality and Standardization Office<br>5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466<br>Telephone (703) 756-2340 AUTOVON 289-2340 |

DD Form 1426, OCT 89 — Previous editions are obsolete. — 98/2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.