INCH-POUND

A-A-54694
22 June 1992

COMMERCIAL ITEM DESCRIPTION

CALIPER, DENTAL, METAL THICKNESS

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a metal thickness measuring caliper suitable for use in measuring the wall thickness of metal crowns, porcelain and other rigid dental materials.

Salient characteristics:

Material. The long and short legs of the caliper shall be fabricated of properly hardened and passivated, class 4, martensitic stainless steel. The scale shall be fabricated of class 3, austenitic stainless steel. Stainless steel shall be in accordance with ASTM Designation F 899 for composition.

Design and dimensions. The calipers shall be held in a closed position by a straight spring. The pivot point shall consist of two metal disks over the caliper legs securing the caliper but allowing the movement of a long and short leg (one piece), causing the caliper to open when the handle closes. A circular strip of metal for the scale shall be securely welded or soldered (a lap-joint) to the proximal end of the stationary handle. The proximal end of the movable handle shall serve as a pointer (indicator) along the scale. The scale markings shall be permanent and clearly visibly to the eye. A stop on the free end of the scale shall keep the pointer at "0" when in the closed position. A guide on the proximal end of the pointer-handle shall keep the handle on scale. The outside edge of each handle shall be suitably notched to prevent finger slippage. The measuring beaks shall be sharp so as to be suitable for use in measuring the thickness of rigid dental materials and shall be configured so as to be able to make such measurements at any point on a

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

dental crown made of such materials. Design and dimensions shall be as shown in Figure 1. Dimensions shall be measured using an optical comparator, shadowgraph, or other suitable device capable of measuring the caliper dimensions with accuracy specified in the figure.

Autoclavability. The caliper shall show no signs of corrosion after being subjected to 1 steam autoclave cycle using distilled water at $270^0 \pm 5^0$F and 27 ± 1 psi for a minimum of 20 minutes.

Finish. The caliper shall have a smooth satin or matte finish.

Identification marking. In addition to contractor markings, each caliper shall be marked with the name or trademark of the manufacturer if different from that of the contractor. The word "stainless" or "ss" shall also be marked on all instruments to identify the steel as stainless. As an alternate to the word "stainless" or "ss", the use of a registered trademark identifying the steel as stainless shall be acceptable, provided prior approval is received from the cognizant contracting officer. Calipers of foreign manufacture shall be marked with the country of origin.

Workmanship. The caliper shall be free of nicks, burrs and other defects which detract from it's appearance or impair it's serviceability.

Unit. Each (EA). One Caliper, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an inspection level of II and an acceptable quality level (AQL) of 2.5. The unit of product for examination purposes shall be one caliper, as specified in this description.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified below. The unit of product for test purposes shall be zero for all sample sizes.

Test Criteria

Characteristic	Inspection level
Dimensions	S-2
Autoclavability	S-2

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and pack ng shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document.

National Stock Number	Item Identification
6520-01-112-6385	CALIPER, DENTAL, Metal Thickness, 0-10mm capacity, 1/10mm Graduation

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6520-2117
Location: PB #2/CALIPER

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

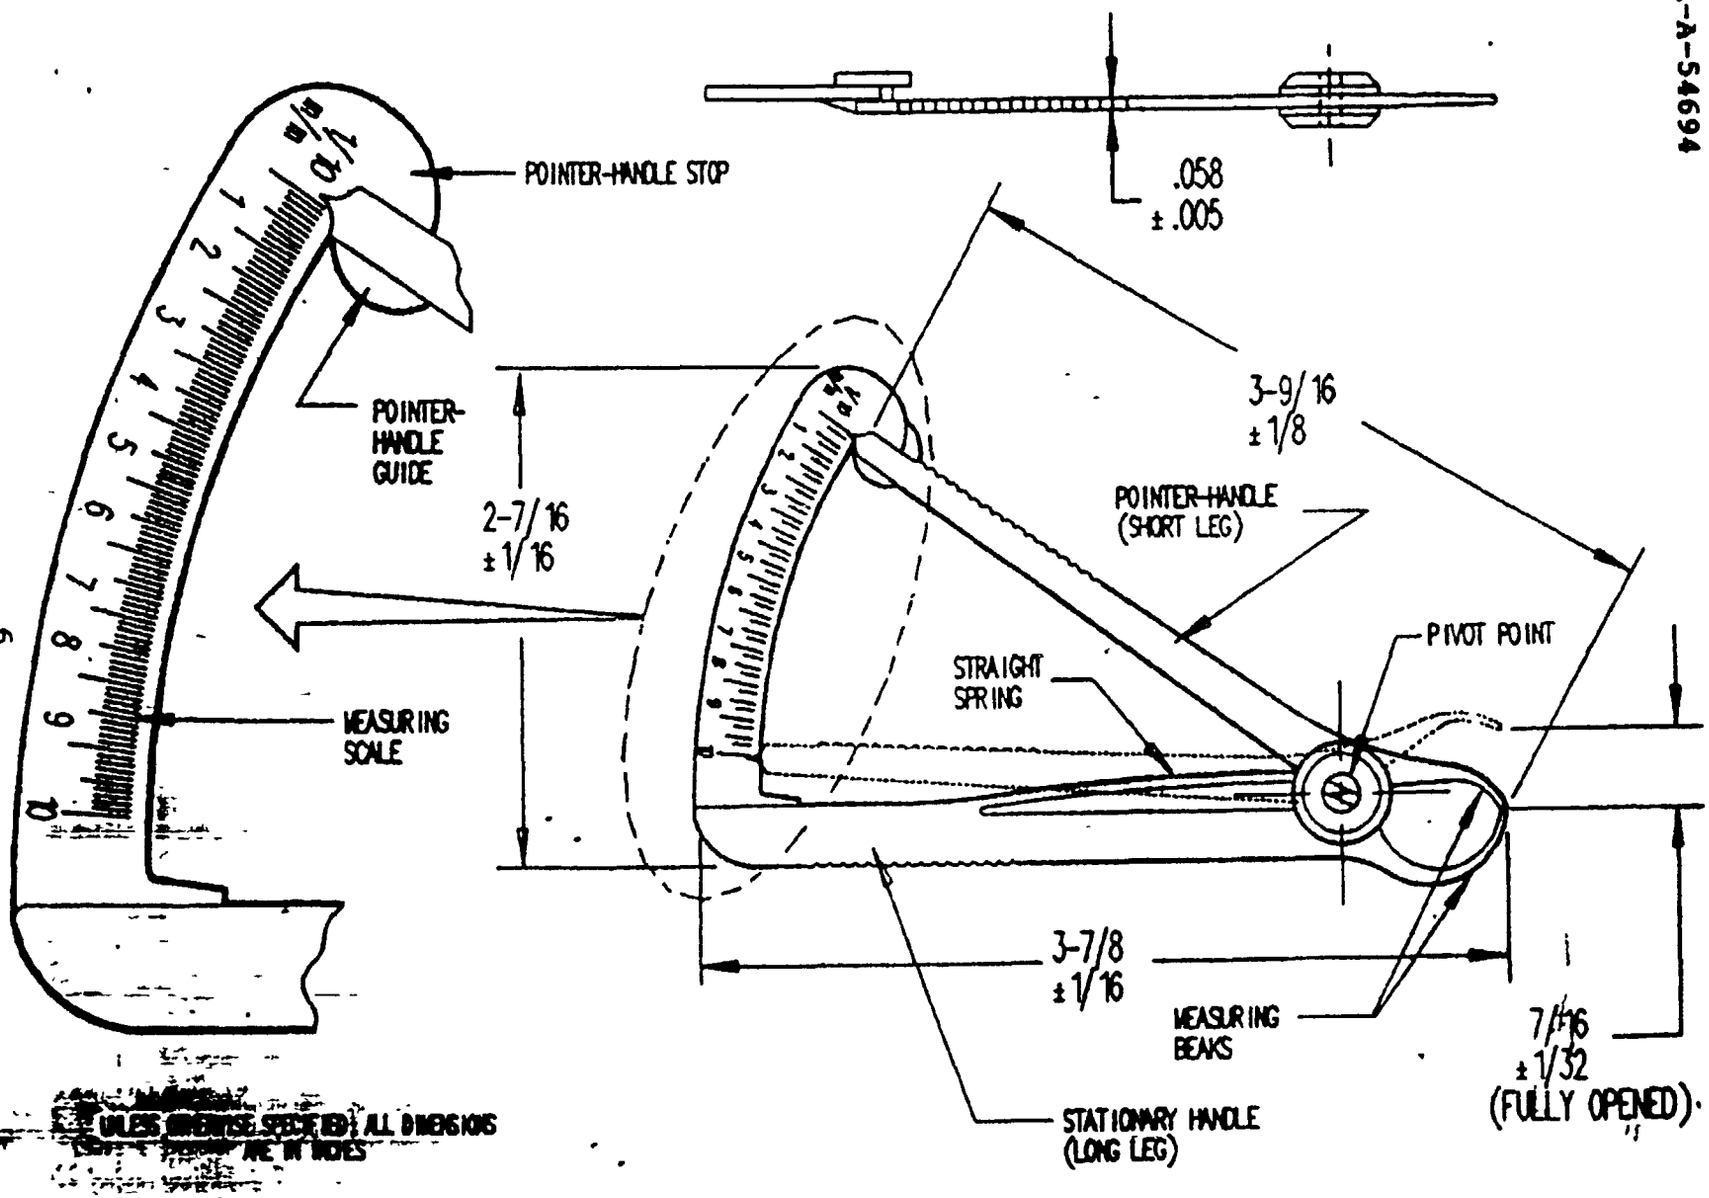


FIGURE 1 Caliper, Dental, Mi(Thickness NSN 6520-01-119-6385

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I. RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54694	22 June 1992

3. DOCUMENT TITLE

CALIPER, DENTAL, METAL THICKNESS

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)

7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center	(215)737-2870	444-2870
c. ADDRESS (Include Zip Code) ATTN: DPSC-MSE 2800 S. 20th Street Philadelphia, PA 19101	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 — Previous editions are obsolete

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33
Check the source to verify that this is the current version before use.