MILITARY SPECIFICATION

FILES, PULP CANAL, DENTAL, RHOMBOIDAL

This specification is approved for use within DLA, Defense Personnel Support Center (DM), and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers standardized pulp canal files of the rhomboidal design for use in endodontic procedures.

1.2 Classification. Rhomboidal files shall be of the following classes and sizes as indicated, (see 6.1).

Class I - 21 millimeter, operative end.

Sizes	
08	35
10	40
15	45
20	50
25	55
30	60

AMSC N/A FSC 6520

Benefical comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

Class II - 25 millimeter, operative end.

Sizes

08	55
10	60
15	70
20	80
25	90
30	100
35	110
40	120
45	130
50	140

Class III - 30 millimeter, operative end.

Sizes

08	55
10	60
15	70
20	80
25	90
30	100
35	110
40	120
45	130
50	140

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications and standards. The following specifications and standards form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of these documents shall be those listed in the issue of the Department of Defense Index of Specifications and Standards (DODISS) and supplement thereto, cited in the solicitation.

SPECIFICATIONS

Federal

PPP-B-566-Boxes, Folding, Paperboard.
PPP-B-636-Boxes, Shipping, Fiberboard.
PPP-B-676-Boxes, Setup.

Military

MIL-P-116-Methods of Preservation.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal
FED-STD-66-Steel, Chemical Composition and Hardenability.
FED-STD-151-Metal: Test Methods.

Military
MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.
MIL-STD-147 - Palletized Unit Loads.
MIL-STD-794 - Parts and Equipment, Procedures for Packaging of.

(Copies of specifications and standards required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting activity.

2.2 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification shall take precedence. Nothing in this specification, however, shall supersede applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 Materials.

3.1.1 Operative end. The operative end of the rhomboidal files shall be fabricated of AISI 302 or 304 vacuum melted stainless steel in accordance with Federal Standard Number 66, with a minimum tensile strength of 310,000 pounds per square inch (psi) for sizes 08 through 20 files and a minimum tensile strength of 270,00 psi for sizes 25 through 140 files, when tested as specified in 4.4.1.

3.1.2 Handle. Handle of the files shall be fabricated of plastic material which is rigid and of a quality suitable to withstand normal operative procedures. Handles shall be capable of being autoclaved or dry heat sterilized without losing the shape of the handle or leaching out of the color, when tested as specified in 4.4.6.


3.2 Design and dimensions. The design and dimensions of the rhomboidal files shall be of the standardized system conforming to the requirements of figure 1 and table I (dimensions), when tested as specified in 4.4.2. The files shall be suitable for use as cutting instruments for gaining access to, clearing, enlarging, and smoothing the walls of a root canal during endodontic procedures. Rhomboidal files shall be of two-piece construction, comprised of an operative end and a handle. Files shall be furnished in class I, sizes 08 through 60, and classes II and III, sizes 08 through 140, as specified, (see 6.1).

Source: https://assist.dla.mil -- Downloaded: 20260-21T20:08Z
Check the source to verify that this is the current version before use.

Table I. Dimensions


Size	Diameter (Tolerance ± 0.02mm) D1mm	D2mm	D3mm	Number of Spirals ± 1	Angle of Cutting Edge ± 1 Degree
08	0.08	0.14	0.40	20	87.5
10	0.10	0.16	0.42	20	87.5
15	0.15	0.21	0.47	19	85
20	0.20	0.26	0.52	18	82.5
25	0.25	0.31	0.57	18	75
30	0.30	0.36	0.62	16	75
35	0.35	0.41	0.67	15	75
40	0.40	0.46	0.72	14	75
45	0.45	0.51	0.77	13	75
50	0.50	0.56	0.82	13	75
55	0.55	0.61	0.87	12	70
60	0.60	0.66	0.92	11	65
70	0.70	0.76	1.02	11	60
80	0.80	0.86	1.12	10	60
90	0.90	0.96	1.22	9	60
100	1.00	1.06	1.32	8	60
110	1.10	1.16	1.42	8	60
120	1.20	1.26	1.52	7	60
130	1.30	1.36	1.62	7	60
140	1.40	1.46	1.72	6	60

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

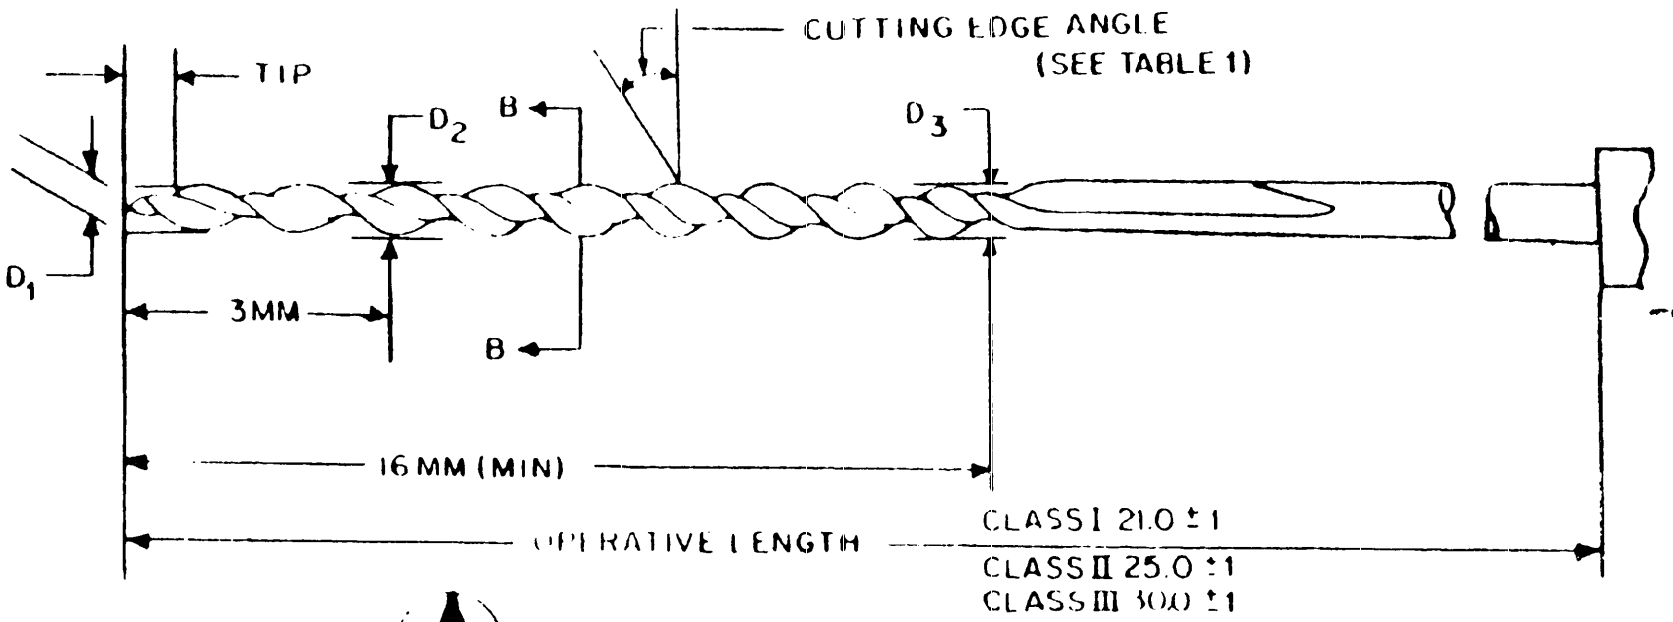





SECTION B B
RHOMBOIDAL CROSS-SECTION

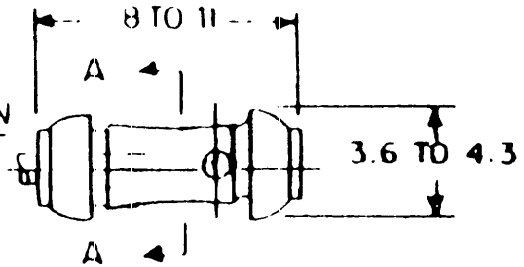


HANDLE



SECTION A-A

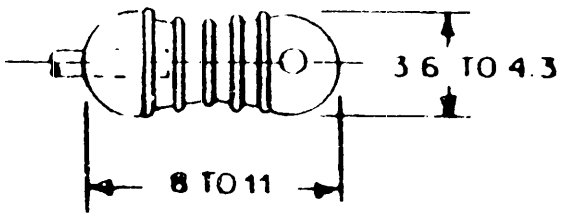

ALTERNATE HANDLE

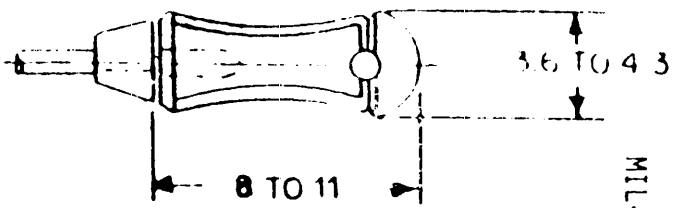

ALTERNATE HANDLE

NOTES:

1. HANDLES SHALL BE IN ACCORDANCE WITH THIS FIGURE FOR DIMENSIONAL REQUIREMENTS; SHAPE OF HANDLES SHOWN ARE TYPICAL AND ARE NOT INTENDED TO RESTRICT OR PRECLUDE THE PURCHASE OF FILES WHICH ARE OTHERWISE IN ACCORDANCE WITH THIS SPECIFICATION
2. HOLE IN HANDLE SHALL BE OPTIONAL
3. ALL DIMENSIONS ARE IN MILLIMETERS

FIGURE 1 — FILE PULP CANAL, RHOMBOIDAL

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

3.2.1.1 Taper. The taper, as measured over the larger diameter cutting edges of the rhomboidal file shall be 0.02mm per millimeter of cutting length when tested as specified in 4.4.2.2.

3.2.1.2 Tip. The tip length of the instrument shall be no greater than twice the diameter of D1 of the respective size number, when tested as specified in 4.4.2.3. The tip of the instrument shall be sharply pointed.

3.2.2 Handles. Operative ends of files shall be securely and permanently affixed in the handle with no movement of operative end within the handles permitted. Color shall be incorporated in the plastic composition. Handles shall be in accordance with figure 1 for dimensions.

3.2.3 Figures. The figures forming a part of the specification are specification control figures. The supplier shall be responsible for preparing his own shop drawings. Where tolerances prescribed could cumulatively result in improper design, the supplier shall provide tolerances within those prescribed on the figure to insure correct function, fit, assembly and operation of the item. No deviation from the prescribed dimensions or tolerances is permissible without prior approval of the contracting officer.

3.3 Resistance to fracture by twisting. The torsional load or torque at various angular deflections for each instrument shall not be less than that given in Table II for each size when tested as specified in 4.4.3.

3.4 Stiffness. The stiffness of all instruments shall not be greater than that given in Table III for each size when tested as specified in 4.4.4.

3.5 Corrosion resistance. The operative ends of the files shall not show evidence of corrosion on their surface when subjected to the corrosion tests as specified in 4.4.5.

3.6 Finish. Spiralled section of operative ends of the files shall have a bright and smooth finish. Handles shall be longitudinally serrated or shall have cross cut serrations. The entire handle may be serrated or only the finger-gripping portion need be serrated. Handles shall be suitable for proper finger-gripping.

3.7 Identification marking. Handles shall be color coded and numbered with the respective size for identification of instrument as specified in Table IV.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

TABLE II.

Torque and Angular Deflection (Minimum Values) Twisted in Clockwise Direction

Size	Torque (gm. cm)	Angular Deflection (Degrees)
08	5.0	360
10	6.0	360
15	8.0	360
20	18.0	360
25	30.0	360
30	45.0	360
35	65.0	360
40	100.0	360
45	120.0	360
50	170.0	360

Table III. Stiffness (Bending Moment) Maximum Values at 45° Bend.

Size	Bending Torque (gm. cm.)
08	16
10	20
15	35
20	65
25	80
30	100
35	170
40	200
45	350
50	400

Table IV. Color Coding

Size	Color	Abbreviation
08	Gray	Gry
10	Purple	Pr
15,45,90	White	Wh
20,50,100	Yellow	Yel
25,55,110	Red	Red
30,60,120	Blue	Blu
35,70,130	Green	Grn
40,80,140	Black	Blk

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

3.2.1 Operative end. The operative end shall consist of a conical distal tip; a uniformly tapered spiral cutting section of rhomboidal cross-section in which the short diagonal imparts flexibility while the long diagonal imparts strength; and a non-tapered round shank. The operative end shall be uniformly twisted to the number of spirals specified in table I to form a sharp cutting instrument. Spirals forming the cutting edges shall be right hand and shall extend to the tip. The cutting edge angle (figure 1) shall be as specified in table I. The flute shall have a positive rake. The file shall have a cutting section featuring high flutes to provide sharper cutting edges and low flutes for greater debris removal.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contactor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, NSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in tables V, VI, and VII, (see 4.2.1, 4.2.2 and 4.3) and 4.3.1.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQLs) shall be as indicated in table V. Unit of product for examination purposes shall be the unit of issue.

TABLE V. Sampling for examination.

Type Defect	Inspection level	AQL (percent defective)
Major A	II	1.0
Major B	S-2	1.5
Minor A	II	2.5
Minor B	S-2	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table VI. Unit of product for test purposes shall be as indicated in table VI.

TABLE VI. Sampling for test.

Component	Characteristic	Requirement	Test procedure	Unit of product	Inspection level	AQL (percent defective)
Operative ends	Tensile strength	3.1.1	4.4.1	Lot of steel stock	*	---
	Dimensions	3.2	4.4.2	One file	S-2	**
	Resist. to frac. by twisting	3.3	4.4.3	One file	S-2	**
	Stiffness test	3.4	4.4.4	One file	S-2	**
Entire instrument	Corrosion resistance	3.5	4.4.5	One file	S-2	**
Handles	Sterilization	3.1.2	4.4.6	One file	***	**

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

*Average of a minimum of three specimens from each lot of steel stock.
**Acceptance number shall be zero for all sample sizes.
***Separate S-2 level quantities for both autoclave and dry heat tests.

4.2.3 Raw materials Sufficient material from each lot of metal used in the construction of the files shall be selected for chemical analysis.

4.2.4 Sample unit usage. Where feasible, the same sample unit shall be tested for the determination of two or more test characteristics.

4.3 Examination. The files shall be examined for defects including, but not limited to, those listed in table VII.

TABLE VII. Classification of Defects.

Categories	Defects
Major A:	
101	Class and size not as specified.
102	Design not as specified.
103	Handles not properly color coded.
104	Operative ends do not have a bright smoothly-honed finish.
105	Cutting edges not sharp.
106	Operative ends not firmly affixed in the handles.
107	Laminations or cracks present.
108	Operative end bent, deformed, or otherwise damaged.
Major B:	
151	Number of spirals not as indicated for size number.
152	Length of operative end not as specified.
153	Cutting edge angle not as indicated for size number.
Minor A:	
201	Finish of handles not as specified.
202	Label or instruction sheet giving color code system not included in unit package.
203	Packaging and packing not as specified.
Minor B:	
251	Dimensions of handles not as specified.

4.3.1 Inspection of packaging. The sampling and inspection of the preservation and interior package marking shall be in accordance with groups A and B quality conformance inspection requirements of MIL-P-116. The sampling and inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

4.4 Tests.

4.4.1 Chemical analysis and tensile strength of the metals. In the absence of certificates of quality for the raw material, the samples selected in accordance with 4.2.3 shall be analyzed in conformance with methods 111 or 112 of Fed. Test Method Std. No. 151. In case of dispute, method 111 shall be used for referee analysis. Tensile strength shall be performed in a tension tester on an 8-inch sample of steel stock used to produce the files.

4.4.2 Equipment. The diameter and tip length of an instrument shall be measured using an optical comparator, shadowgraph, or other suitable device capable of measuring the diameter and length with the accuracy specified in 3.2.1.2 and Table I.

4.4.2.1 Diameters. The rhomboidal file to be measured shall be inserted into an optical comparator, shadowgraph, or other suitable device and the diameters D1, D2, and D3 shall be measured.

4.4.2.2 Taper. The rhomboidal file to be measured shall have its diameter determined at 1 mm increments along the cutting section beginning 1 mm from the tip point up to 6 mm from the tip point.

4.4.2.3 Tip. The tip length of the instrument shall be determined by a suitable measuring device.

4.4.3 Resistance to fracture by twisting. Samples of a given size shall be tested for resistance to fracture by twisting as follows:

4.4.3.1 Equipment. The testing equipment shall be capable of measuring torque with an accuracy of $\pm$ 1 gm. cm. and angular deflection with an accuracy of $\pm$ 2°. The equipment described below shall be used for compliance testing and is presented as the preferred type of equipment for all purposes. The equipment as shown in Figure 2 shall consist of: a reversible geared motor revolving at a speed of 2 RPM which drives a test instrument by means of a separate hardened steel chuck; a torque measuring device fixed on two linear ball bearings, mounted to the shaft of the device is the chuck with jaws made of brass (70% copper-35% zinc) used to clamp the test instrument at the tip along a length of 3 mm. See Figure 3. A separate amplifier and digital display controls the operation of the motor and records the torque and angular deflection. The circuitry of the amplifier should include the feature of retaining for display the maximum torque 1 mm from the tip point up to 6 mm from the tip point.

4.4.3.2 Procedure for twist test. Calibrate the device for the torque range of the test instrument size to be tested. The rhomboidal file to be tested shall have its handle removed with a suitable wire cutter at the point at which the handle is attached to the instrument shaft. Set the test instrument shank into the driving chuck leaving a maximum of 1 mm of the unground portion of the shank out of the

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

chuck. Tighten the chuck. Slowly slide the torque device along the linear ball bearing until the tip of the test instrument enters 3 mm into the brass jaws. Check to assure that the test instrument is straight and centered into the jaws. Tighten the chuck. Since clamping will probably induce a pre-stress of the test instrument, the gear motor must be activiated in steps until the torque digital display or the strip chart recorder shows a zero reading. After insuring that the geared motor is set for clockwise rotation as viewed from the test instrument shank end, activiate the device. The test device will cease operation when the test instrument fails. The maximum torque and angular deflection shall be recorded for each rhomboidal file tested.

4.4.4 Stiffness. Sample of a given size shall be tested for stiffness as follows:

4.4.4.1 Equipment. The equipment as described in 4.3.3.1 shall be used with the modification of the clamping jaws and the bending device or catch pin as shown in Figure 4. The amplifier of the device must be capable of obtaining a pre-selected angular deflection (45°) at which point the test stops. The testing equipment shall be capable of measuring torque with an accuracy of ± 1 gm. cm.

4.4.4.2 Procedure for stiffness test. Calibrate the device for the torque range of the test instrument size to be tested. The rhomboidal file to be tested shall have its handle removed with a suitable wire cutter at the point where the handle is attached to the instrument shaft. Set the device to stop the angular deflection at 45°. Place the chuck onto the shaft of the torque meter device. Set the tip of the test instrument into the jaws of the chuck perpendicular to the axis of the motor. When the tip enters 3 mm into the brass jaws, tighten the chuck. Mount the catch pin into the gear motor shaft. Slide the torque device along the linear ball bearing until the test instrument is located above the rotating pin. By rotating the gear motor in the proper direction in steps, adjust the catch pin until it is lightly touching the test instrument. The torque reading must show zero. Activiate the test device. The test will automatically cease when the angular deflection has reached 45°. The torque at 45° shall be recorded for each rhomboidal file tested.

4.4.5 Corrosion tests. Files shall be tested for corrosion resistance by one of the following procedures:

4.4.5.1 Sample and preparation. Files of each size shall be scrubbed with soap and water, rinsed in hot water, followed by a dip in ethyl alcohol (95%), or isopropyl alcohol (isopropyl; 2-propanol) NF, and dried.

Source: https://assist.dla.mil -- Downloaded: 202610-21T20:08Z
Check the source to verify that this is the current version before use.

4.4.5.2 Copper sulfate test. A copper sulfate solution is made up as follows: Copper sulfate ($CuSO_4$, 5 H_2O) 4.0 g, Sulfuric acid (H_2SO_4, sp gr 1.84) 10.0 g, and Water (H_2O) 90.0 milliliters (ml). The instruments selected and prepared shall be immersed in the copper sulfate solution at a temperature of 65° Fahrenheit (F) for 6 minutes and then wiped off with a cloth saturated with fresh water. The instrument shall then be examined under a magnification of a least 5X for the presence of brown stains indicating corrosion.

4.4.5.3 Agar ion test. An agar ion gel is made up as follows: Potassium ferricyanide ($K_3Fe(CN_6)$ 0.2 g, Sodium chloride (NaCl) 1.0 g, Water (H_2O) 100 ml, Agar-agar 1.5. g. The agar sol shall be poured into a transparent container. The instruments selected and prepared are inserted into the gel (37° ± 2°Celsius (C)) at intervals of not less than 10 mm and at a distance of 10 mm from the periphery of the container. The instruments are inserted to a depth of approximately 20 mm. Visual examination of the instruments while in the gel shall be made for the presence of blue precipitates on the instrument, indicating corrosion.

4.4.6 Sterilization tests. The finished rhomboidal files shall be autoclaved under 27 ± 3 pounds of pressure at 132 ± 5°C(270 ± 9°F) for twenty (20) minutes and dry heat sterilized at 160 ± 5°C(320 ± 9°F) for one hundred and twenty (120) minutes. The handles of the files shall then be examined for compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

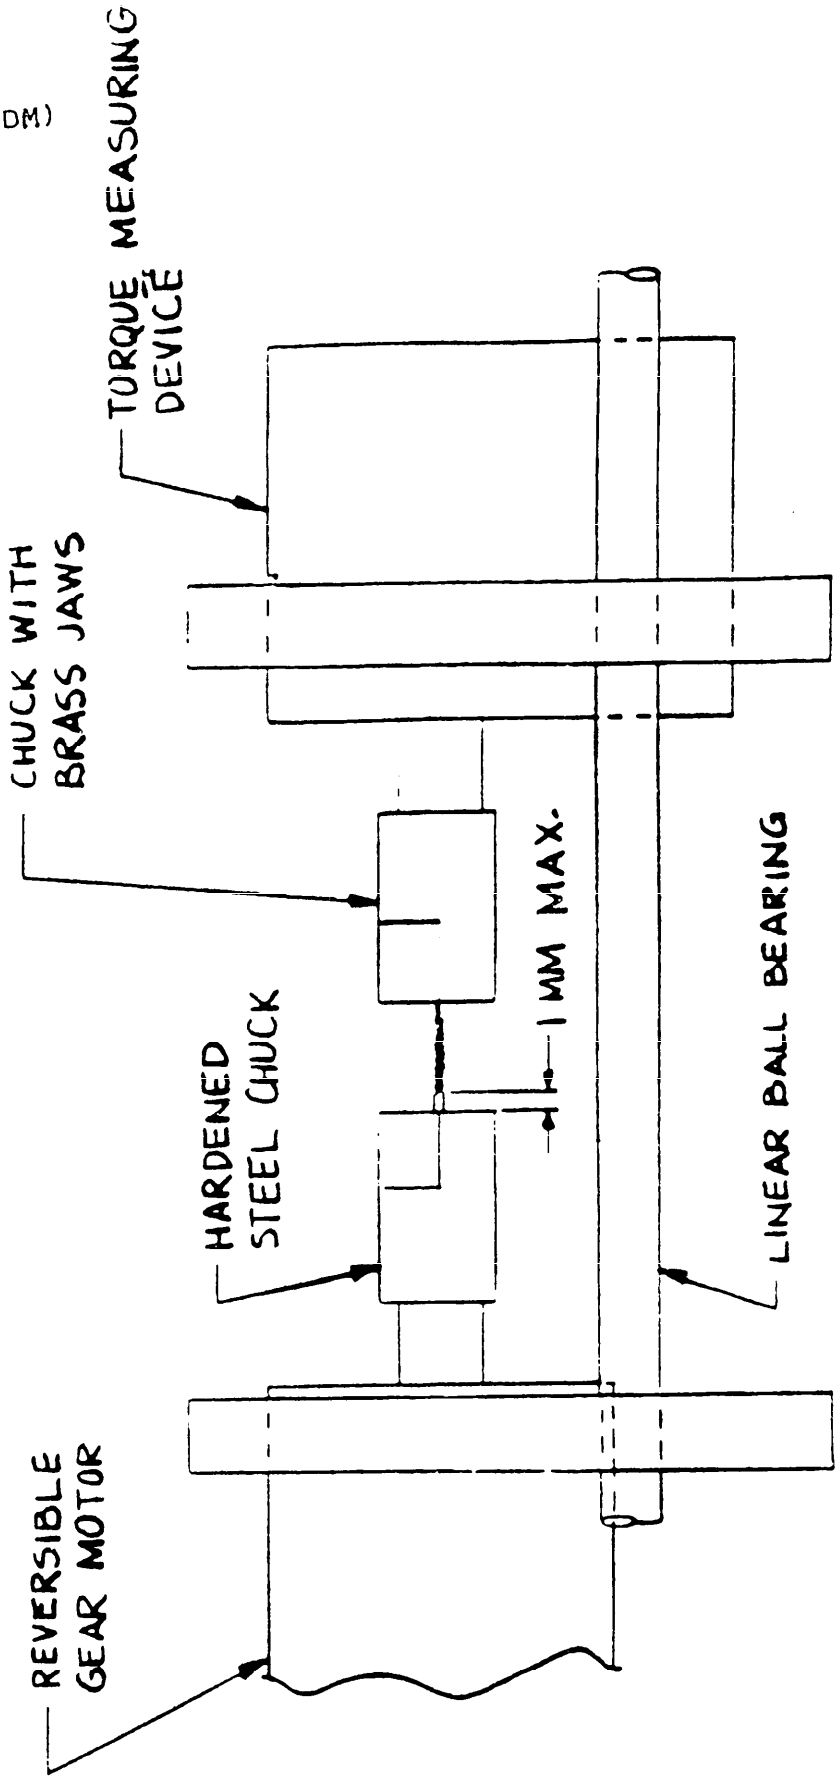


FIG. 2 - TEST EQUIPMENT FOR TORQUE TESTING

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

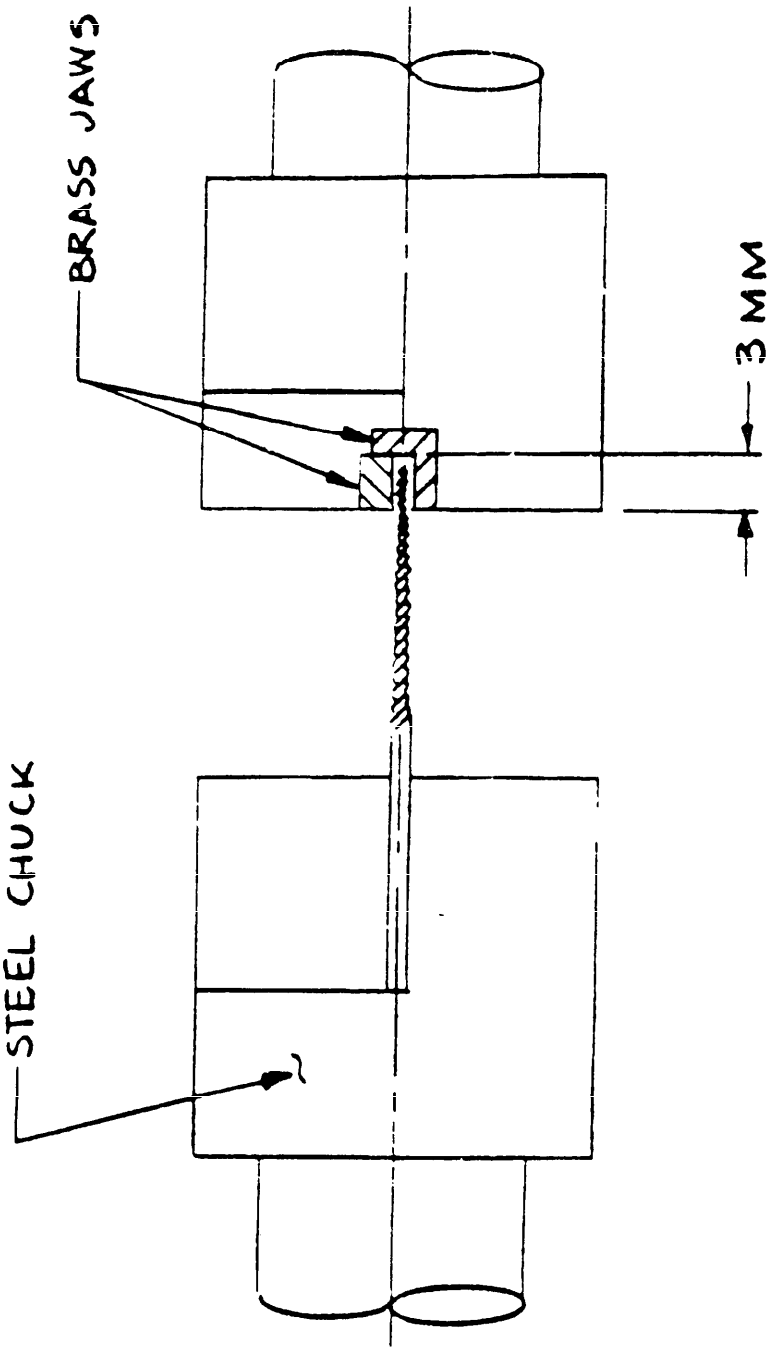


FIG. 3 - TWIST TEST CHUCK DETAIL

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

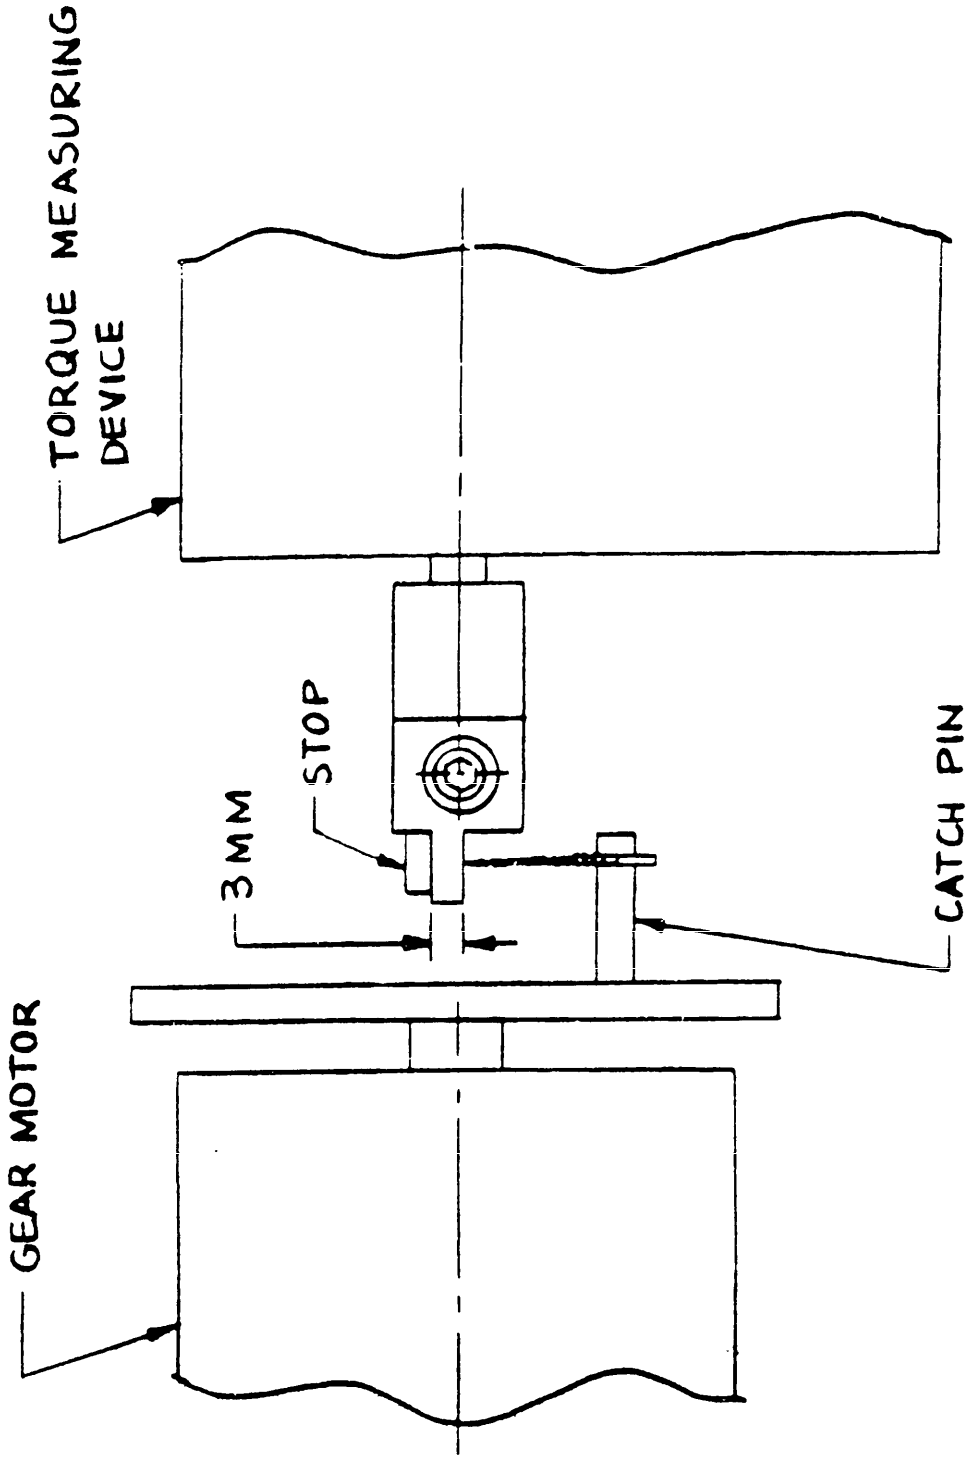


FIG. 4 - STIFFNESS TEST

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

5. PACKAGING

5.1 Preservation. Preservation shall be level A or C, as specified (see 6.1).

5.1.1 Level A.

5.1.1.1 Cleaning. Files shall be cleaned in accordance with MIL-P-116.

5.1.1.2 Drying. Files shall be dried in accordance with MIL-P-116.

5.1.1.3 Preservative applications. Preservatives shall not be used.

5.1.1.4 Unit packaging. Six files of one class and size shall be packaged in a plastic tray having a clear, slip-over cover or a hinged cover. The tray shall be designed with six cavities or inserts to hold each file in a manner to prevent movement and damage to the operative end. The cover shall be secured with a strip of pressure-sensitive tape. Each plastic container shall be further packaged in a bag as specified in MIL-P-116, method IC-1.

5.1.1.5 Intermediate package. Twenty-four unit packages containing files of one class and size only shall be packaged in a box constructed in accordance with PPP-B-566 or PPP-B-676. Closure shall be in accordance with the appendix of the applicable box specification.

5.1.2 Level C. The level C preservation for files shall conform to the MIL-STD-794 requirements for this level.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.1).

5.2.1 Level A. Twenty-four intermediate packages (576 units) containing files of one class and size only shall be packed in a shipping container designed for a type 2 load and constructed in accordance with PPP-B-636, class weather-resistant. Closure, strapping, and waterproofing shall be as specified in the appendix of the box specification.

5.2.2 Level B. Twenty-four intermediate packages (576 units) containing files of one class and size only shall be packed in a shipping container designed for a type 2 load and constructed in accordance with PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

5.2.3 Level C. The level C packing for files shall conform to the MIL-STD-794 requirements for this level.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

5.2.4 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.2.5 Unitized loads. Unitized loads, commensurate with the level of packing specified in the contact or order, shall be used whenever total quantities for shipment to one destination equal 40 cubic feet or more. Loads shall be unitized on pallets. Quantities less than 40 cubic feet need not be unitized. Unitized loads shall be uniform in size and quantities to the greatest extent practicable.

5.2.5.1 Levels A and B. Files packed as specified in 5.2.1 and 5.2.2 shall be unitized on pallets conforming to MIL-STD-147.

5.2.5.2 Level C. Files packed as specified in 5.2.3 shall be unitized as specified in MIL-STD-794.

5.3 Marking.

5.3.1 Levels A, B and C. Each unit pack, intermediate package, exterior container and unitized load shall be marked as specified in MIL-STD-129.

5.4 General.

5.4.1 Exterior container. Exterior container (see 5.2.1, 5.2.2 and 5.2.3) shall be of minimum tare and cube consistent with the protection required and shall contain equal quantities of identical stock numbered items to the greatest extent practicable.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.3.1.

6. NOTES.

6.1 Ordering data.

6.1.1 Acquisition requirements. Acquisition documents should specify the following:

a. Title, number, and date of this specification.
b. Class and size required (see 1.2).
c. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 National Stock Number (NSN) coverage. This specification covers the following items listed in the Federal Supply Catalog:

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

NSN	ITEM IDENTIFICATION
	FILE, PULP CANAL, DENTAL, 21mm End Length
6520-01-180-3567	Rhomboidal, Standardized, Size 8,6s
6520-01-180-3568	Size 10,6s
6520-01-180-3569	Size 15,6s
6520-01-180-3570	Size 20,6s
6520-01-180-3571	Size 25,6s
6520-01-179-5804	Size 30,6s
6520-01-180-3573	Size 35,6s
6520-01-179-5805	Size 40,6s
6520-01-180-3572	Size 45,6s
6520-01-179-5806	Size 50,65s
6520-01-179-5807	Size 55,65s
6520-01-179-5808	Size 60,65s
	FILE, PULP CANAL, DENTAL, 25mm End Length
6520-01-179-5809	Rhomboidal, Standardized, Size 8,6s
6520-01-179-5810	Size 10,6s
6520-01-179-5811	Size 15,6s
6520-01-179-5812	Size 20,6s
6520-01-180-3574	Size 25,6s
6520-01-180-3575	Size 30,6s
6520-01-180-6949	Size 35,6s
6520-01-180-3243	Size 40,6s
6520-01-180-3244	Size 45,6s
6520-01-180-3245	Size 50,6s
6520-01-180-3246	Size 55,6s
6520-01-180-3247	Size 60,6s
6520-01-180-3248	Size 70,6s
6520-01-181-3187	Size 80,6s
6520-01-180-3249	Size 90,6s
6520-01-180-3250	Size 100,6s
6520-01-180-3251	Size 110,6s
6520-01-180-3252	Size 120,6s
6520-01-180-3253	Size 130,6s
6520-01-180-3254	Size 140,6s
	FILE, PULP CANAL, DENTAL, 30mm End Length
6520-01-176-6189	Rhomboidal, Standardized, Size 8,6s
6520-01-176-6190	Size 10,6s
6520-01-176-6191	Size 15,6s
6520-01-176-6192	Size 20,6s
6520-01-176-6193	Size 25,6s
6520-01-176-6194	Size 30,6s
6520-01-176-7531	Size 35,6s
6520-01-176-7530	Size 40,6s
6520-01-176-7532	Size 45,6s
6520-01-176-7533	Size 50,6s

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

6520-01-176-7534	Rhomboidal, Standardized,	Size 55,6s
6520-01-176-4633		Size 60,6s
6520-01-176-4632		Size 70,6s
6520-01-176-4634		Size 80,6s
6520-01-176-4635		Size 90,6s
6520-01-176-4636		Size 100,6s
6520-01-182-3923		Size 110,6s
6520-01-177-0131		Size 120,6s
6520-01-177-0132		Size 130,6s
6520-01-176-7611		Size 140,6s

MILITARY INTERESTS:
Custodians:
Army-MD
Navy-MS
Air Force-03

Review activities:
Army-MD
Navy-MS
Air Force-03

06781

PREPARING ACTIVITY:
DOD-MB

AGENT:
DLA-DM

Project No. 6520-1907

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

4.4.4 The lid of the instrument shall be tested as specified in 4.4.4

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON D. C.
POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Staff Director
Defense Medical Materiel Board
Fort Detrick
Frederick, MD 21701

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:08Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil -- Downloaded: 202610-21T20:08Z
Check the source to verify that this is the current version before use.

DD FORM 1426