INCH-POUND

A-A-52048
March 12, 1992

COMMERCIAL ITEM DESCRIPTION

THERMOMETER, SELF-INDICATING, LIQUID-IN-GLASS, POCKET TYPE

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-T-12625.

This description covers a liquid-in-glass, self-indicating thermometer graduated in Fahrenheit (°F) degrees. The thermometers are intended for use in determining atmospheric temperature during surveying operation.

Salient characteristics:

Design: The thermometer shall be as specified herein and as in figure 1. A protective case shall be provided.

Material: The bulb shall be normalized thermometer glass, cylindrical in shape, or blown from the stem.

Stem: The stem shall be a magnifying type glass with a broad strip of white glass at the back to increase reflected light. The annealed stem shall be designed to increase the angle of vision and effective width of the fluid column. A button top shall be provided for holding the thermometer securely in the case cap.

Bulb: The bulb and tube shall contain a colored fluid, the height of which shall indicate the temperature of the surrounding medium.

Immersion: Total.

Temperature range: -66 °F to +160 °F.

Beneficial comments, recommendations, additions, deletions, clarifications, etc., and other data which may improve this document should be sent by letter to: Commander, U.S. Army Belvoir Research, Development, and Engineering Center, ATTN: STRBE-TSE, Fort Belvoir, VA 22060-5606.

AMSC N/A FSC 6685

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:05Z
Check the source to verify that this is the current version before use.

Graduations: Graduation marks and numbers shall be etched on the stem and spaced at 2 °F intervals. Longer graduation lines shall be at each 10 °F. The marks and numbers shall be filled with an indelible pigment, black for temperatures of zero degrees and above and red for below zero.

Special inscription: The letter "F" shall be etched above the upper limit of the scale.

Case: A 6-inch protective case shall be provided for the thermometer. The case shall be aluminum or brass with a screw cap to engage the bottom or top of the thermometer stem. The case shall have a ball-point pen type pocket clip near the upper end.

Workmanship: The thermometer and thermosensitive fluid shall be free from gas bubbles and foreign material. The thermometer shall be clear and free from pits, chips, sharp edges, or other defects which would prove detrimental to accuracy and appearance.

Certification of commercial item: The contractor shall certify that the product offered to the Government meets the salient characteristics of this description, and that the product conforms to the producer's own drawings, specifications, standards, and quality assurance practices and is the same product as the manufacturer's current product offered by the contractor in the commercial marketplace for at least one year preceding the solicitation. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products: Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, provided they fall within specified tolerances using conversion tables contained in the latest revision of FED-STD-376, and all other requirements of this commercial item description are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements: In accordance with Federal Acquisition Regulation, section 23.403, the Government's policy is to acquire items composed of the highest percentage of recovered materials practicable, consistent with maintaining a satisfactory level of competition without adversely affecting performance requirements or exposing the supplier's employees to undue hazards from the recovered materials.

Preservation, packing, and marking: Preservation, packing, and marking shall be as specified in contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:05Z
Check the source to verify that this is the current version before use.

Quality assurance: The pocket type liquid-in-glass self-indicating thermometer shall be examined for the following defects. Presence of one or more defects shall be cause for rejection.

1. Design not as specified.
2. Material not as specified.
3. Stem not as specified.
4. Bulb not as specified.
5. Immersion not as specified.
6. Temperature range not as specified.
7. Graduation not as specified.
8. Special inscription not as specified.
9. Case not as specified.
10. Workmanship not as specified.

Notes: The procuring agency should specify the preferred options permitted herein and include the following information in procurement documents:

1. Title, number and date of this commercial item description.
2. Preservation, packing and marking required.
3. When this commercial item description is used for procurement, the commercial item certification clause must appear in the solicitation.

The following are suggested sources of supply for this item description (competition is not limited to these sources):

a. Brooklyn Thermometer Co. Inc., 90-T Verdi Street, Farmingdale, NY 11735.
b. Palmer Instruments, Inc., 3131 Wasson Rd., Cincinnati, OH 45209.
c. PSG Industries Inc., 1225 Tunnel Rd, Perkasie, PA 18944.

FED-STD-376 is available from the Standardization Documents Order Desk, Building 4D, 700 Robbins Avenue, Philadelphia, PA 19111-5094.

The preparing activity for this item description is the U.S. Army Belvoir Research, Development, and Engineering Center, Fort Belvoir, VA 22060-5606.

MILITARY INTERESTS:

Custodian
Army - ME

Review Activity
DLA - GS


CIVIL AGENCY COORDINATING ACTIVITY:

GSA-FSS

PREPARING ACTIVITY:
Army - ME

Project 6685-0848

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:05Z
Check the source to verify that this is the current version before use.

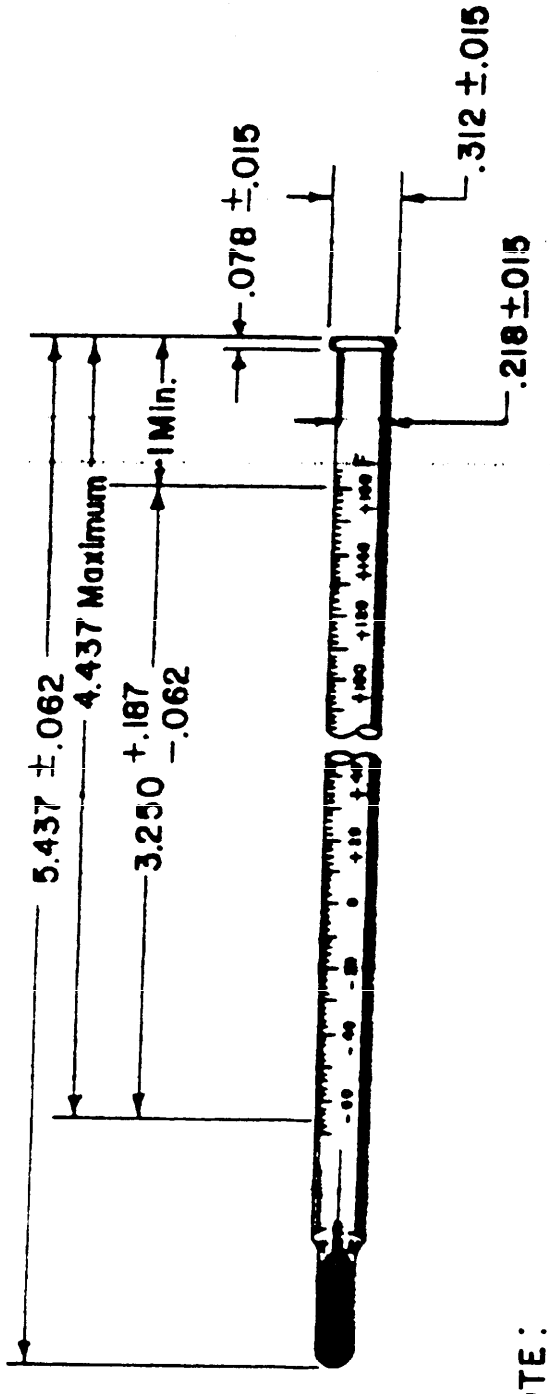

NOTE:
DIMENSIONS ARE IN INCHES.

FIGURE 1. Thermometer tube.

X-3130A

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:05Z
Check the source to verify that this is the current version before use.