INTERIM COMMERCIAL ITEM DESCRIPTION

ADHESIVE TIES, SURGICAL

The General Services Administration has authorized the use of this Interim Commercial Item Description which was developed by the Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA, 19101, based upon currently available technical information.

This interim commercial item description covers adhesive, hypo-reactive, surgical ties.

Salient characteristics.

Shall be a hypo-reactive surgical adhesive tie suitable for use in circumstances where dressings are changed frequently. The adhesive ties shall be constructed as shown in figures 1 and 2 and shall be comprised of a backing, a facing, an overlap strip, a reinforcing strip and adhesive.

The backing and reinforcing strip shall be woven rayon, plain, white taffeta fabric having a thread count of 180 by 54 threads per inch when tested as specified in method 5050 of Federal Test Method Standard 191. The fabric shall be porous and the porosity shall result from the properties of the fabric and weave and not from perforations and the fabric shall have physical properties suitable for the intended purpose.

The overlap strip shall be clear polyethylene terephthalate polyester film (mylar) 0.0009 +/- 0.00012 inches thick.

The facing shall be paper which is coated with polyethylene on one side.

The adhesive shall be pressure sensitive, hypo-reactive acrylic elastomer and shall resist creeping and flowing after it is applied to the backing. The adhesive shall be so applied to the backing that the finished adhesive tie shall be porous.

AMSC/NA FSC 6510

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:22Z
Check the source to verify that this is the current version before use.

The adhesive shall be uniformly applied to one side of the backing and to one side of the reinforcing strip. The adhesive ties shall be 7½ +/- 1/8 by 11 1/8 +/- 1/8 inches. The reinforcing strip shall be 1 +/- 1/16 inches wide. The overlap strip shall be 2 7/8 +/- 1/16 inches wide. The reinforcing strip shall be cemented to the adhesive coated side of the backing and shall run the full length fo the backing parallel to a longitudinal edge of the backing. The overlap strip shall be cemented to the adhesive side of the backing and to the reinforcing strip and shall run the full length of the backing. The facing shall cover the entire exposed adhesive area of the backing. The polyethylene coated side of the facing shall be in contact with the adhesive coated side of the backing. The facing shall be easily removable. The completely assembled adhesive ties shall not show any exposed adhesive. The adhesive ties shall comply with the requirements of Adhesive Tape, USP, except that the tensile strength shall be a minimum of 28 pounds per inch of width and the adhesive strength shall be a minimum of 20 pounds. The adhesive ties shall have a row of eight reinforced tie holes punched through the reforcing strip, the overlap strip and the backing. The edges of the adhesive ties and the holes shall be clean cut.

Workmanship. The adhesive ties shall be free from defects which detract from their appearance or impair their serviceability.

Unit. Package (PG). One package containing 24 adhesive ties, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item. Testing and examination shall be conducted to determine compliance with all specification requirements. Test methods shall be suitable, accurate and reproducible.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for examination shall be one adhesive tie. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5 maximum percent defective.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6510-00-003-3058	ADHESIVE TIES, SURGICAL, 7¼ by 11 1/8 inches, 24s

Ordering data. Inspection/test dating period intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:

VA-OSS
PHS
FDA-MPQAS

PGC 44398

Project No. 6510-0762

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.


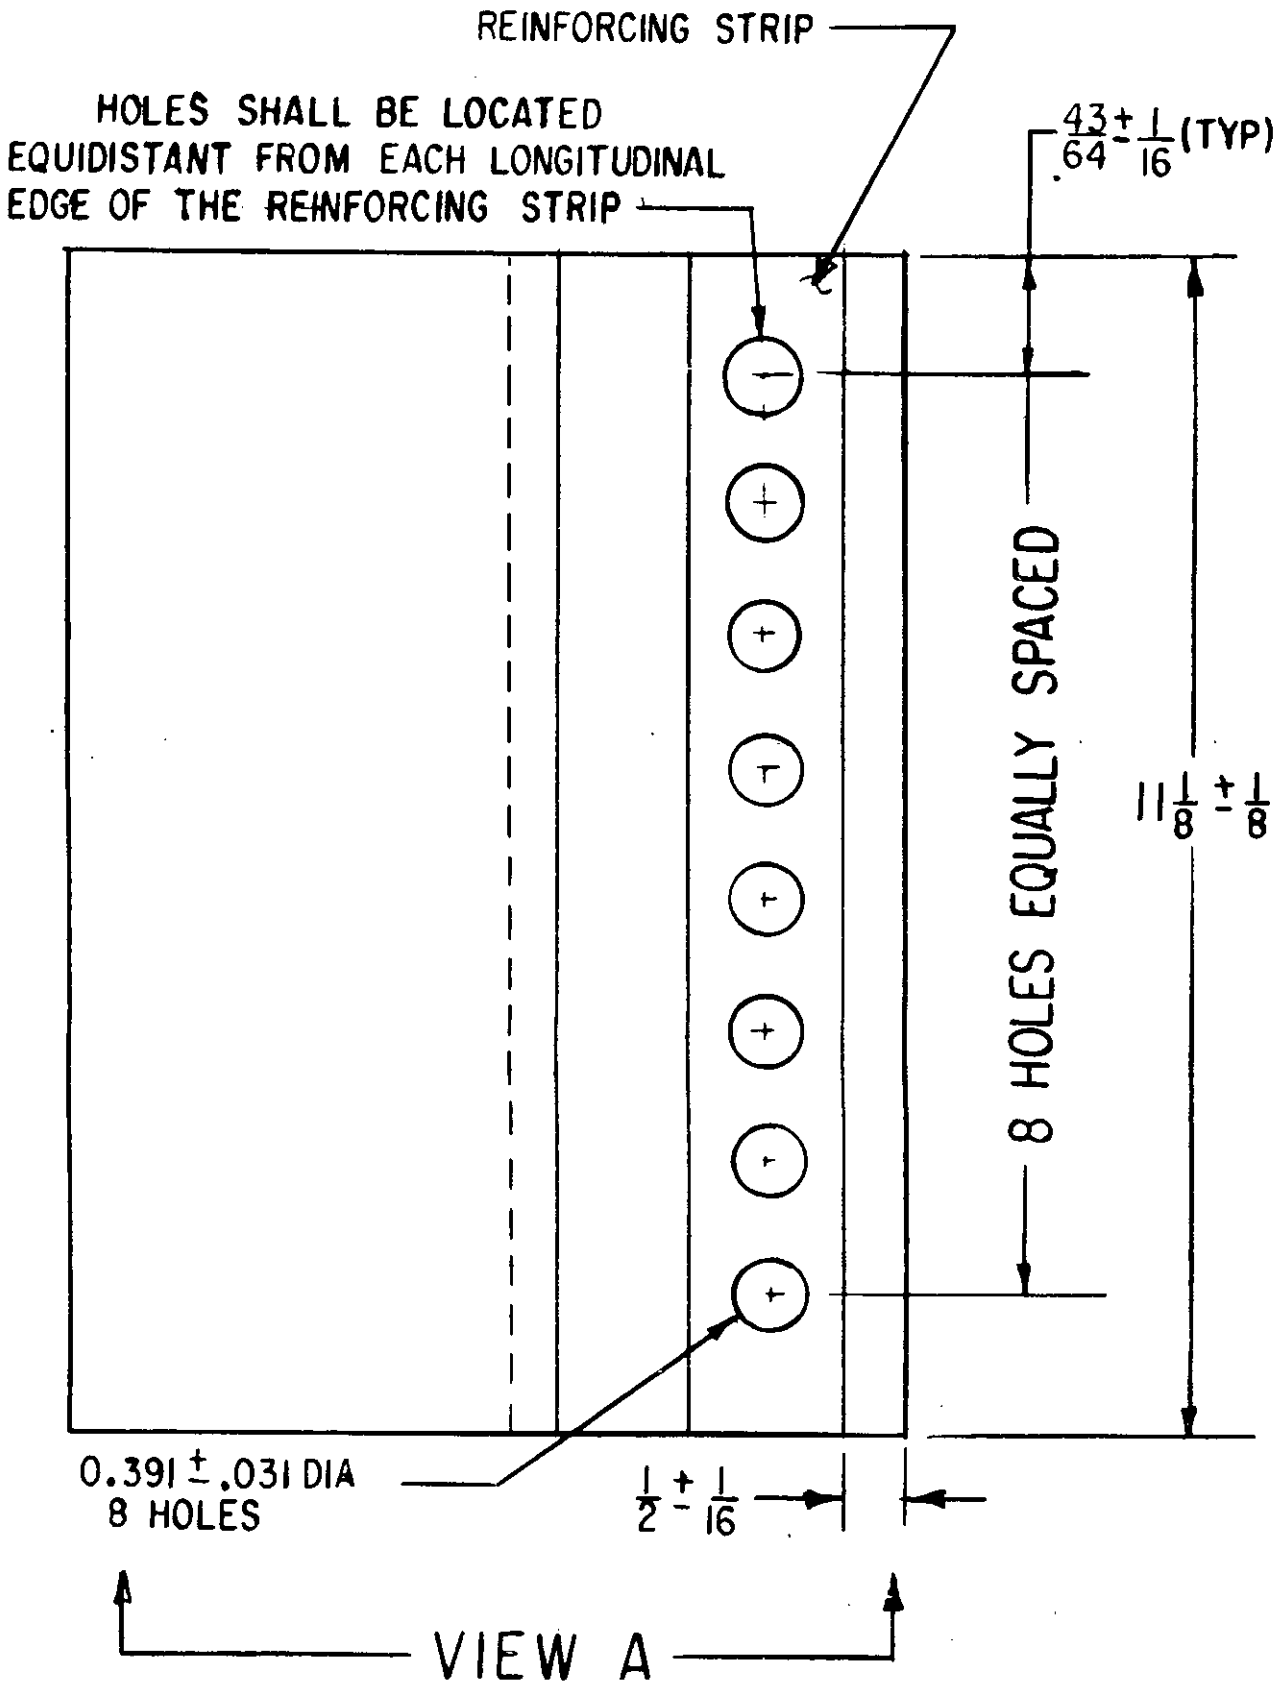


FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:22Z
Check the source to verify that this is the current version before use.

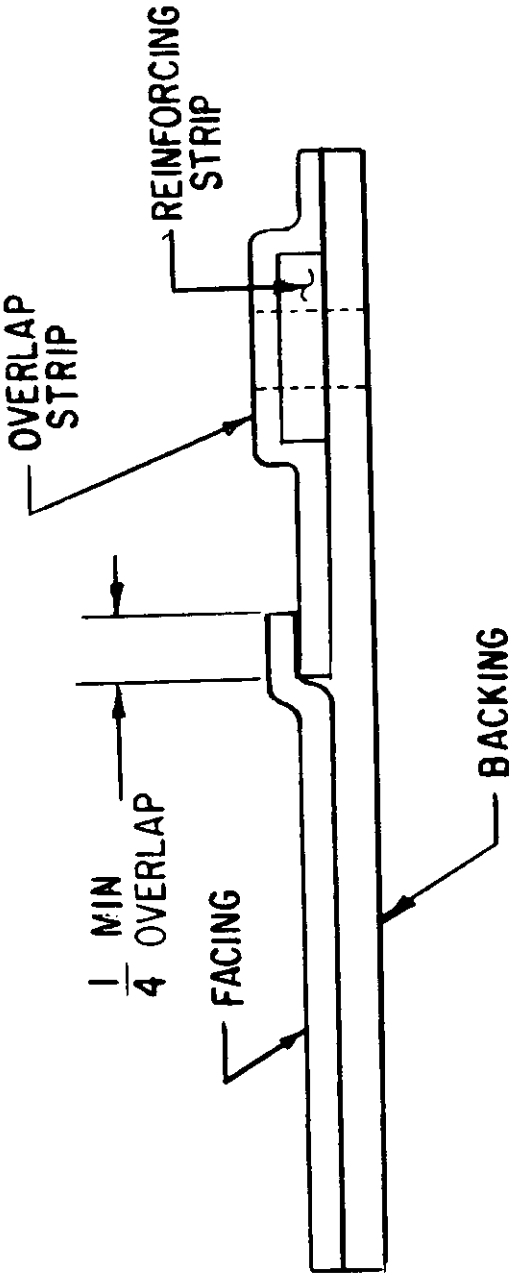

VIEW A

FIGURE 2

☆U.S. GOVERNMENT PRINTING OFFICE: 1989 - 604-033/10861

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:22Z
Check the source to verify that this is the current version before use.