MIL-C-36542C
4 February 1976
SUPERSEDING
MIL-C-36542B
19 May 1970

MILITARY SPECIFICATION

CUP, SPECIMEN

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers two types of disposable plastic specimen cups with lids, suitable for use in military medical treatment facilities.

1.2 Classification.

1.2.1 Types. Specimen cups covered by this specification shall be of the following types:

TYPE I - Individually packaged sterile cup and lid - 4-1/2 ounces capacity.
TYPE II - Packages of non-sterile, nested cups and lids - 6 ounces capacity.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein.

SPECIFICATIONS

Federal

PPP-B-566	- Boxes, Folding, Paperboard.
PPP-B-585	- Boxes, Wood, Wirebound.
PPP-B-601	- Boxes, Wood, Cleated-Plywood.
PPP-B-621	- Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	- Boxes, Shipping, Fiberboard.
PPP-B-676	- Boxes, Setup.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:46Z
Check the source to verify that this is the current version before use.

Military

MIL-L-10547	- Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.
MIL-S-36586	- Sterilization Test Strip Set, Bacterial Spore.

STANDARDS

Military

MIL-STD-105	- Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	- Marking for Shipment and Storage.

(Copies of specifications, standards, and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection and approval (see 4.1.2.1 and 6.2).

3.2 Material. Materials used in the fabrication of the cups and lids shall be of the highest quality and suitable in all respects for the intended purpose.

3.2.1 Polypropylene. Polypropylene shall be rigid, translucent, inert, chemically resistant, virgin resin.

3.2.2 Polystyrene. Polystyrene shall be rigid, transparent, inert, chemically resistant, virgin resin.

3.2.3 Polyethylene. Polyethylene shall be inert, chemically resistant, virgin resin. Density of the polyethylene shall be suitable for the intended use of the part. Color of the polyethylene may be either natural or pigmented.

3.3 Design and construction. The cups shall be one-piece molded units. The lid shall form a leak-proof closure with the cup when tested as specified in 4.4.2. Graduations and numerals shall be molded into the side of the cup and shall be clear and legible. The cups shall be sufficiently transparent to permit viewing of the contents. The bottom of the cups shall be formed so that it sits stable on a flat surface.

3.3.1 Cup.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:46Z
Check the source to verify that this is the current version before use.

* 3.3.1.1 Type I cup. The type I cup shall be constructed in accordance with figure 1. The cup shall be circular in section. The top of the cup shall be threaded to accomodate a screw-type lid (see 3.3.2). The cup shall be fabricated of either polypropylene or polystyrene. The cup shall have a minimum brimful capacity of 4-1/2 ounces. The cup shall be graduated on at least one side. Minimum graduations shall be from at least 3/4 to 4 ounces in 1/4 ounce increments and 20 to 110 milliliters (ml.) or cubic centimeters (cc.) in 10 ml. or cc. increments. Graduations shall be numbered at each ounce and at least four ml or cc levels. The cup shall be provided in a sterile condition. The cup and lid shall be sterile when tested as specified in 4.4.1.

* 3.3.1.2 Type II cup. The type II cup shall be fabricated of either polystyrene or polypropylene. The top of the cup shall be either threaded to accept a screw-type lid or beaded to accomodate a snug fitting snap-on lid (see 3.3.2). The cup shall have a minimum brimful capacity of 4-1/2 ounces. The cup shall be a graduated in 1/4 ounce and 10 ml. increments over a minimum range of 3/4 to 4 ounces and 20 ml. to 110 ml. A frosted panel on the exterior of the cup shall be acceptable if provided. The cups and lids shall be provided in a sanitary condition.

3.3.2 Lid. The lid for the type I cup shall be threaded to mate with the threads on the cup. The lid for the type II cup shall be either threaded to mate with the threads on the cup or shall have an inside groove to engage the bead on the top edge of the cup. The lid shall be capable of being easily installed and removed from the cup. The lid shall be fabricated of polyethylene.

3.4 Sterility. The type I cups shall be sterile when tested with a biological indicator as specified in 4.4.1.

3.4.1 Certificate of sterility. A certificate of sterility, stating that samples from each sterilizer lot have been tested and found to be sterile, shall be submitted to the procuring activity. The certificate of sterility, shall include:

a. Item identification.
b. National stock number.
c. Contract or purchase order number.
d. Sterility lot or control number.
e. Date of sterilization.
f. Quantity of product in sterilizer lot.
g. Type of sterilization (gas, radiation, heat, steam, etc.)
h. Form of biological indicator (i.e., inoculated paper spore strip or carrier, inoculated product, or inoculated simulated product).

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:46Z
Check the source to verify that this is the current version before use.

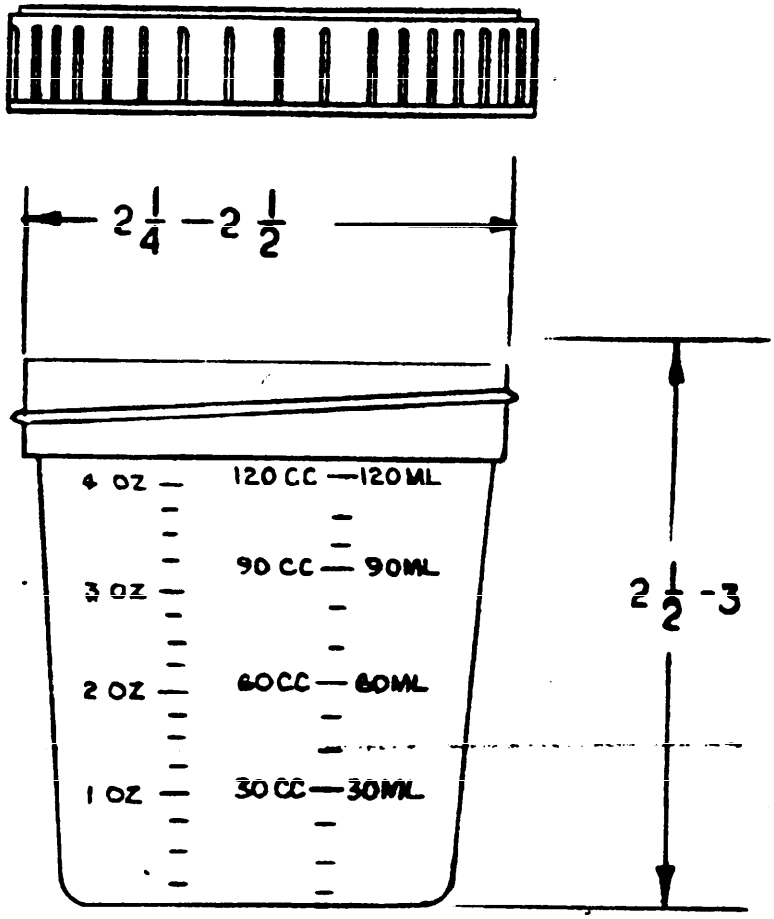


Figure 1. Cup, specimen.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:46Z
Check the source to verify that this is the current version before use.

i. Test organism(s) and population density used.
j. Test medium, incubation temperature, incubation time, and dates of tests.
k. Number of test units.
l. Statement that samples comply with sterility tests.
m. Signature of head of laboratory or a designated qualified alternate.

When inspection is made at destination, the certificate of sterility shall be submitted by the contractor to the Directorate of Medical Materiel, ATTN: DPSC-ATQ, Defense Personnel Support Center, 2800 South 20th Street, Philadelphia PA, 19101, and a copy forwarded with each shipment to the consignee. When inspection is made at source, certificate of sterility shall be furnished to the cognizant Government Quality Assurance Representative for submission to the procuring activity.

3.4.2 Sterility lot. A sterility lot is that single quantity of product subjected to the same manufacturing operation and simultaneously sterilized in the same sterilizer chamber. Each unit package shall be clearly marked with a sterility lot (control) number and date of sterilization as specified in 5.3.2. Each sterility lot shall be traceable to the pertinent manufacturing lot(s).

3.5 Workmanship. Workmanship shall be first class throughout. The cups and lids shall be free from burrs, sharp edges, cracks, holes, or other defects which affect the appearance or may impair their serviceability. The cups and lids shall be free from contamination such as hair, grease, oil, dirt or other foreign matter visible to the naked eye.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:46Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

4.1.2.1.1 First article inspection. First article inspection shall be performed on cups when a first article sample is required (see 3.1). This inspection shall include examination of 4.3, and tests of 4.4.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.3 and tests of 4.4.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the cup or lid, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and table I. The unit of product for inspection purposes shall be individual cup and lid. Sample units shall be selected at random in such a manner that not more than five individual covers and lids shall be selected from any one package.

TABLE I. Sampling for examination (individual cup & lid)

For visual examination	Inspection level	AQL (Defects per hundred units)
Major defects	S-2	2.5
Minor defects	S-2	4.0
For dimensional examination	S-2	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:46Z
Check the source to verify that this is the current version before use.

Additional sampling for examination shall be conducted in accordance with MIL-STD-105 and table II. The unit of product for inspection purposes shall be the unit package. Sample packages shall be selected at random in such a manner that not more than five packages shall be selected from any one exterior container (see 5.1.2).

TABLE II. Sampling for examination (unit package)

For visual examination	Inspection level	AQL (Defect per hundred units)
Major defects 1/	S-2	2.5
For count	S-2	2.5

1/ See paragraph 4.3.1 for Major 107 and 108 defects.

* 4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table III. The unit of product for purposes of testing for water-tightness shall be the individual cup and lid. Sample units shall be selected at random in such a manner that not more than five cups and lids shall be selected from any one package. Samples for sterility testing shall be selected from each sterilizer load (see 4.4.1).

TABLE III. Sampling for tests

Characteristic	Requirement	Test procedure	Inspection level	AQL
Water-tightness between cup and lid	3.3	4.4.2	S-2	2.5
Sterility	3.4	4.4.1	1/	0

1/ Not applicable.

4.3 Examination. The cups and lids shall be examined to determine compliance with all requirements contained in this specification.

* 4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table IV. Examination shall not be restricted to the classified possible defects listed below.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:46Z
Check the source to verify that this is the current version before use.

TABLE IV. Classification of defects

Categories and Defects	
Major	
101	Cup or lid not free from any deformation.
102	Scale numerals or lines not clearly defined and easily read.
103	Cup or lid not free from oil or grease smears on either inside or outside.
104	Cup or lid not free from water drops or dried stains.
105	Cup or lid not free from pits, scratches, burrs, and abrasions.
106	Cup not stable when placed on a flat surface.
107	Type I individual package not properly sealed to maintain sterility of contents.
108	Individual package not free of cuts or openings which permit entry of dust or foreign matter.
109	Cup or lid not free from dirt or loose particles on either inside or outside.
110	Cups not free of holes, especially at the gate on the bottom of the clip.
Minor	
201	Cup or lid not free from horizontal flash greater than 1/64 inch.
202	Cup not free from vertical flash greater than 1/16 inch high and greater than 1/2 inch wide.
203	Cup not free from waviness that obliterates the lines or numerals, or otherwise detracts from their serviceability.

4.3.2 Dimensional examination. The cups and lids shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.3.3 Count examination. The number of cups and lids in the unit package shall be counted. Any unit package with a short count of either cups or lids shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:46Z
Check the source to verify that this is the current version before use.

4.4.1 Sterility test. The cups shall be tested for sterility in accordance with the method specified in the U.S.P. for non-parenteral devices using inoculated product, inoculated simulated product, or paper spore strip (carrier). Product containing a biological indicator shall be marked or labeled so that it clearly differentiates from product intended for distribution. The incubation medium and minimum time in each case shall be soybean casein digest for 7 days for inoculated product, inoculated simulated product, or paper spore strip (carrier). The incubation temperature shall be as indicated in paragraph 4.4.1.1. The minimum number of test units, regardless of lot size, shall be 10, except for inoculated carrier which shall be 20 for type I sterilization and 30 for type II sterilization including inoculated carrier and product test units. Type I sterilization shall be by steam under pressure. Type II sterilization shall be all other means.

4.4.1.1 Inoculated product or simulated product. For each type of sterilization the organism used shall be as listed below:

Type of Sterilization	Organism	Incubation Temperature
Steam	B. Stearothermophilus	55°- 65°C
Dry Heat	B. Stearothermophilus	55°- 65°C
	B. subtilis var. niger (or globigii)	30°- 35°C
Gas	B. Subtilis var. niger (or globigii)	30°- 35°C
Radiation	B. pumilus	30°- 35°C

The number of viable cells shall be sufficient to provide assurance that the product has been sterilized.

4.4.1.2 Inoculated carrier. Inoculated carriers (paper spore strips) if used shall be in accordance with MIL-S-36586. Other paper carriers shall be inoculated to be of equivalent resistance. The method of incubation and number of test units shall be as indicated in 4.4.1 Sterility test and 4.4.1.1 Inoculated product or simulated product. The method sterilization will control the organism in the spore strip to be tested for as shown in 4.4.1.1.
NOTE: When an inoculated carrier is chosen, product samples must also be tested as required by the U.S.P.

4.4.1.3 Alternate method. Suppliers conducting sterility tests or designating lots in a manner other than that indicated herein shall submit proof that the alternate method provides equal assurance concerning the sterility of the product. However, all sterility tests shall be conducted using biological indicators. Requests for approval of any alternate method of testing for sterility shall be made to the Contracting Officer, and approval obtained before employment of the alternate method on a government contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:46Z
Check the source to verify that this is the current version before use.

4.4.1.4 Product testing. Testing for sterility of the product after receipt by the government shall be without a biological indicator and in accordance with the U.S.P.

4.4.2 Water-tightness. The cup shall be filled with tap water at room temperature to top of graduations that are specified in paragraph 3.3. A lid shall be firmly secured on cup; and then the cup shall be inverted. The inverted cup shall then rest on a sheet of paper which is placed on a flat surface. After fifteen minutes the sealed lid and paper shall be inspected for evidence of leakage.

4.5 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of section 5. Defects shall be scored as specified in table V. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

TABLE V. Examination for preparation for delivery

Examination	Defect
Containers	Not as specified.
Quantity	Quantity in interior packages and shipping containers not as specified.
Packaging & Packing Materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size location, sequence, or method of application.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One package containing one hundred (100) cups with lids of Type I or one package containing twenty-five (25) cups with lids of Type II as specified, constitutes one unit of issue.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:46Z
Check the source to verify that this is the currentversion before use.

5.1.1.1 Level A.

5.1.1.1.1 Immediate container.

5.1.1.1.1.1 Type I. One cup and one lid shall be sealed in a plastic or plastic paper combination (cellophane not permitted) bag of appropriate size and design capable of maintaining sterility of the cup and lid unless damaged or opened. The lid shall be attached to the cup.

5.1.1.1.1.2 Type II. Twenty-five (25) nested cups and twenty-five (25) lids shall be packaged in separate plastic or plastic paper combination (cellophane not permitted) bags of appropriate size and design. Bags shall be sealed in such a manner as to prevent entry of dust or other foreign matter.

5.1.1.1.2 Unit package.

5.1.1.1.2.1 Type I. Each unit of issue shall be packaged in a box designed for a type 2 load and constructed in accordance with PPP-B-636, type CF, class domestic. Box shall be provided with suitable interior fittings such as partitions and/or pads so designed so as to maintain the cups in a neat and orderly fashion. Closure of box shall be as specified in the appendix of PPP-B-636.

5.1.1.1.2.2 Type II. Each unit of issue shall be packaged in a box of appropriate size constructed in accordance with PPP-B-566, PPP-B-676, or PPP-B-636, class domestic. Closure shall be adequate to prevent accidental opening.

5.1.1.2 Level C. Units of issue shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Two (2) units of issue of type I cups or twenty (20) units of issue of type II cups shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather resistant, grade V3c. Closure and strapping shall be in accordance with the appendix of the applicable box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof in accordance with the appendix of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:46Z
Check the source to verify that this is the current version before use.

5.2.2 Level B.

5.2.2.1 Type I. No further packing is required. Unit package as specified in 5.1.1.1.2.1 shall be shipped as the exterior container.

5.2.2.2 Type II. Twenty (20) units of issue shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type1 PPP-B-621, class 1; or PPP-B-636, type CF, class domestic. Closure of box shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. Units of issue shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Immediate containers.

5.3.1.1 Type I. Each immediate container shall be commercially marked. In addition, marking shall include the sterility lot (control) number, the word "STERILE" and the legend "STERILITY GUARANTEED UNLESS PACKAGE IS DAMAGED OR OPENED."

5.3.1.2 Type II. Marking of immediate containers is not required.

5.3.2 Unit package.

5.3.2.1 Type I. Each unit package shall be marked in accordance with MIL-STD-129. Marking shall include the name of contractor, sterility lot (control) number and the legend: "STERILE-CONTENTS OF INNER WRAP ARE STERILE UNLESS IT HAS BEEN OPENED OR DAMAGED" or similar statement. In addition, the method of sterilization (G-Gas, R-Radiation, C-Cold, S-Steam, D-Dry Heat Sterilization). Marking shall follow the level of packaging and date of packaging. Example: "(A-1/76-G)." Final sterilization shall be on or after indicated packaging date.

NOTE: When level B packaging is specified, the unit package shall be marked as specified in 5.3.3.1. Level of preservation shall be shown as "B" in lieu of "A/B."

5.3.2.2 Type II. Each unit package shall be marked in accordance with MIL-STD-129. Marking shall include the legend: "NOT STERILE."

5.3.3 Exterior container.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:46Z
Check the source to verify that this is the current version before use.

5.3.3.1 Type I. Each exterior container shall be marked in accordance with MIL-STD-129. Marking shall include method of sterilization as specified in 5.3.2.1.

5.3.3.2 Type II. Each exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. Specimen cups are intended for use in collecting, transporting and storing specimens in military medical facilities.

6.2 Ordering data. Procurement documents should specify the following:

a. Title, number and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
c. Type required (see 1.2).
d. When a first article is required (see 3.1, 4.1.2.1 and 6.3).

6.3 First article. When a first article is required, it shall be tested and approved under the appropriate provisions of 7-104.55 of the Armed Services Procurement Regulation. The contract or purchase order specifies the quantity, procedure for delivery and other specific instructions for inspection and approval of the first article.

6.4 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock No.	Item Identification	Specification Designation Type
6530-00-837-7472	CUP, SPECIMEN, Plastic, Disposable 4-1/2 oz., 100s (Sterile)	I
6530-00-855-7706	CUP, SPECIMEN, Plastic, Disposable 6 oz., 25s (Not Sterile)	II

6.5 Cross reference of classification. Table VI provides a cross reference of 1.2.1 in MIL-C-36542B and MIL-C-36542C.

TABLE VI. Cross reference of classification

MIL-C-36542B	MIL-C-36542C
Size I, Style A	Type I
Size II, Style B	Type II

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:46Z
Check the source to verify that this is the current version before use.

6.6 Changes from previous issue. The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DSA-DM

Project No. 6530-1365

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:46Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-C-36542C CUP, SPECIMEN

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:46Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:46Z
Check the source to verify that this is the current version before use.