MILITARY SPECIFICATION

JAR, PIPET, PLASTIC

1. SCOPE

1.1 This specification covers a polyethylene jar suitable for use in soaking and washing pipets and other laboratory glassware.

1.2 Classification.

1.2.1 Styles. Jars shall be of the following styles:

Style A - Integral Base

Style B - Removable Base

2. APPLICABLE DOCUMENTS

2.1 The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

L-P-390	Plastic, Molding Material, Polyethylene, Low and Medium Density.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:43Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

3. REQUIREMENTS


3.1 Material.

3.1.1 Jar. Polyethylene for the jar shall be a low density, general purpose polyethylene, in accordance with type I, class L, grade 2 of Federal Specification L-P-390.

3.1.2 Removable Base. Polyethylene for the removable base (Style B) shall be high density linear polyethylene.

3.2 Construction. Pipet jar shall consist of a polyethylene cylindrical container with a flanged base, in accordance with style A or B of figures 1 and 2 respectively. The rim at the open end shall have a smooth, even finish, and shall be in a plane at right angles to the sides. Pipet jar shall not rock when placed on a smooth, plane surface.


Source: https://assist.dla.mil -- Downloaded: 202610-21T08:43Z
Check the source to verify that this is the current version before use.

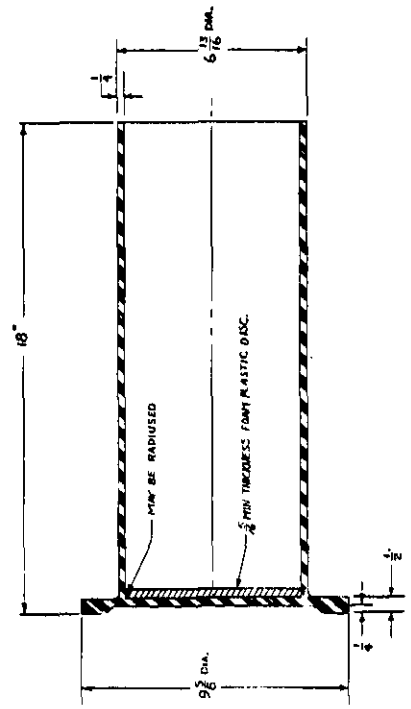

STYLE A

Jar, Pipet, Style A
Figure 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

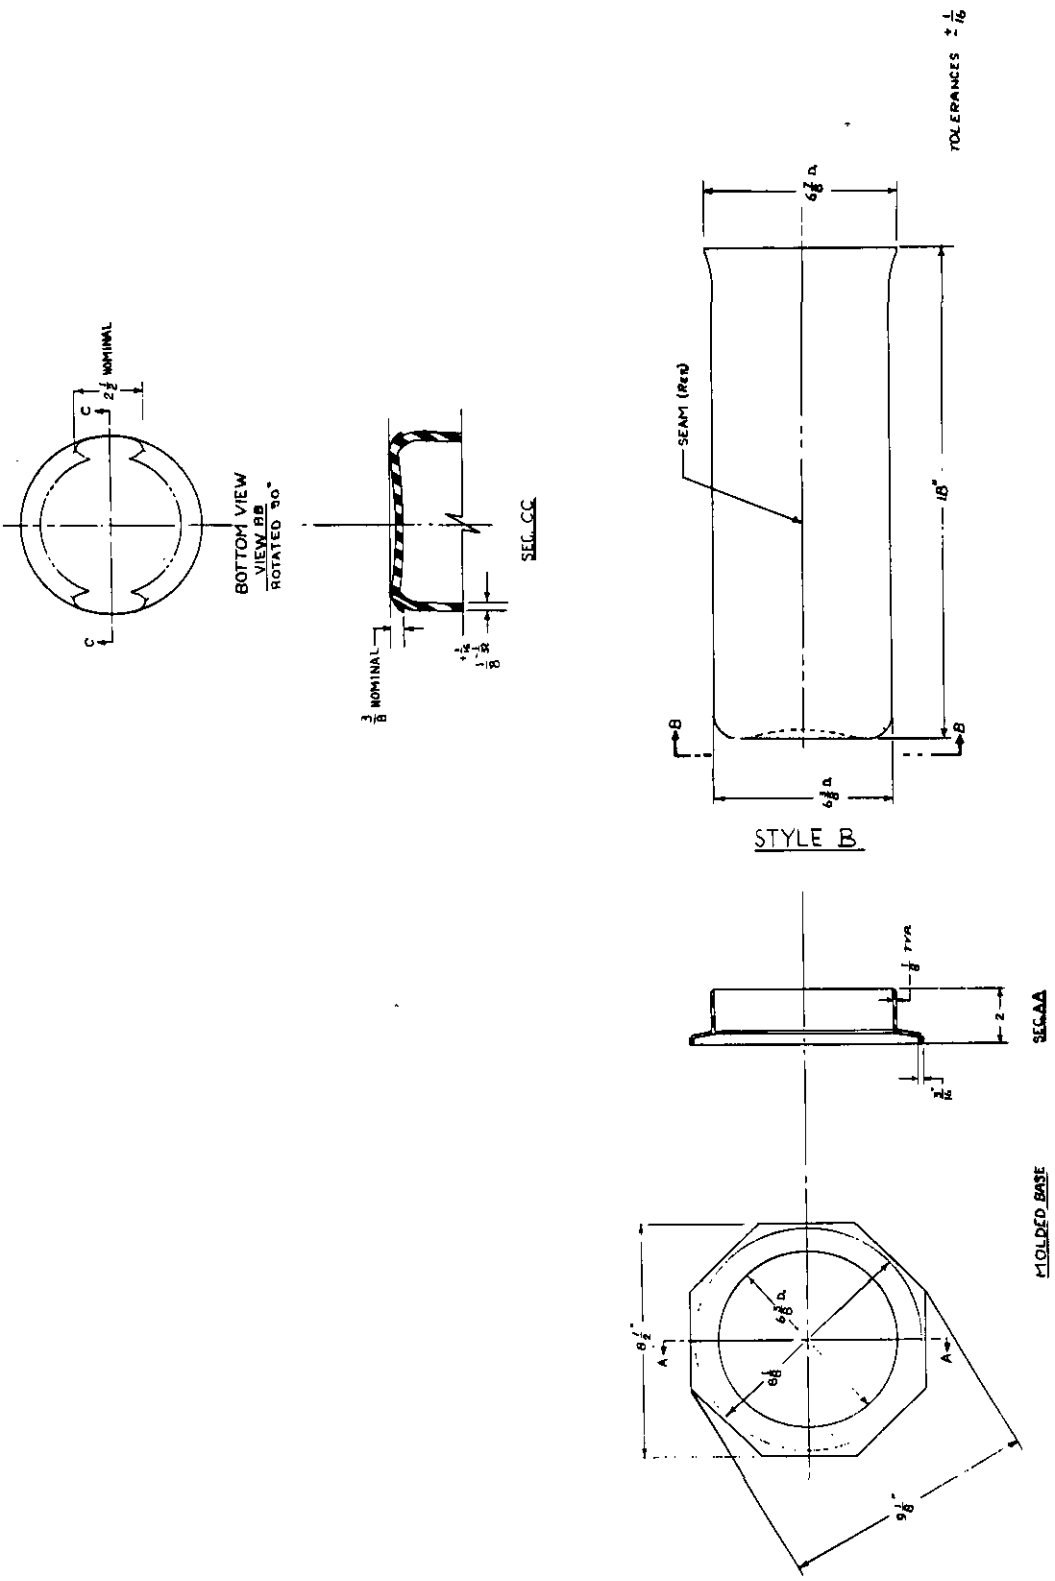

Jar, Pipet, Style B
Figure 2

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:43Z
Check the source to verify that this is the current version before use.

3.2.1 Style A. Style A jar shall be molded polyethylene (see 3.1.1) cylinder with bottom having a sturdy, integrally flanged base, in accordance with figure 1. A foamed plastic disc shall be furnished on the inside bottom of the jar.

3.2.1.1 Foam disc. A removable, soft pliable polyethylene foam disc shall be provided to serve as cushioning for the pipets. The disc shall fit snugly on the inside bottom of the jar.

3.2.2 Style B. Pipet jar shall be a cylindrical polyethylene container with a removable flanged base, and shall be in accordance with figure 2.

3.2.2.1 Jar. Jar shall be a molded polyethylene (3.1.1) cylinder, closed at one end, and having a flared rim at the open end, as shown in figure 2. The bottom of the jar shall be capable of being press-fitted into the base.
The jar shall set upright within the base and shall be perpendicular to the bottom of the base.

3.2.2.2 Base. Base shall be molded of polyethylene (3.1.2) and shall be in accordance with figure 2. Base shall be sturdy and shall be constructed so as to provide stability to the jar. Base shall hold the bottom end of the jar snug and firm.

3.3 Identification marking. Jar shall be permanently and legibly marked with the name or registered trademark of the manufacturer.

3.4 Workmanship. Workmanship shall be first class throughout. Pipet jars shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105.

	Inspection level	AQL (percent defective)
For visual examination		
Major defects	II	2.5
Minor defects	II	4.0
For dimensional examination	S-1	2.5

4.3 Examination. The pipet jar shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Categories and defects*

Major

101	Component missing.
102	Jars not free of cracks, chips or breaks.
103	Jars not free of tears.
104	Jars not stable on a flat smooth surface.
105	Jars not free of deformation.
106	Rim at open end not at right angles to the sides.
107	Jars rock when placed on a smooth, plane surface.
108	Jars not free of sharp edges.
109	Foam disc not free of holes, cracks or tears.

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:43Z
Check the source to verify that this is the currenversion before use.

Minor

201	Identification marking missing, illegible, or incomplete.
202	Rim at open end of jars not straight and even.
203	Rim at open end of jars not smoothly finished.
204	Foam disc not with snug fit in bottom of jar.
205	Foam disc not free of deformation.
206	Removable base (style B) not free of warping.
207	Jars not free of rough mold marks.
208	Jars not free of protrusions.

* Examination shall not be restricted to the defects listed above.

4.3.2 Dimensional examination. The pipet jar shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. Each jar, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table I shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table I. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not Reqd	6 units

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

Source: https://assist.dla.mil -- Downloaded: 20261O-21T08:43Z
Check the source to verify that this is the current version before use.

5.1.3 Level A.

5.1.3.1 Unit package. Unit package shall be a carton of appropriate size constructed in accordance with PPP-B-636. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4, of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:43Z
Check the source to verify that this is the current version before use.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic and method I closure shall be utilized.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. Pipet jar is intended to be used with FSN 6640-782-6015 Basket, Pipet, Plastic.

6.2 Ordering date. Procurement documents should specify the following:

(a) Number and date of this specification.

(b) Selection of applicable levels of packaging and packing. (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:43Z
Check the source to verify that this is the current version before use.

6.3 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet military requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this dodument. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION
MIL-J-36511 (DSA-DM)

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO (If "yes", in what way?)

4. REMARKS (Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)

SUBMITTED BY (Printed or typed name and activity - Optional)

DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.