MIL-P-36506B
16 September 1976
SUPERSEDING
MIL-P-36506A
22 February 1974

MILITARY SPECIFICATION

PATIENT UTILITY KIT

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a lightweight, opaque, plastic, washable and durable patient utility kit suitable for use in military hospitals and other medical treatment facilities.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

PPP-B-585	-	Boxes, Wood, Wirebound.
PPP-B-601	-	Boxes, Wood, Cleated-Plywood.
PPP-B-621	-	Boxes, Wood, Nailed and Lock Corner.
PPP-B-636	-	Boxes, Shipping, Fiberboard.

MILITARY

MIL-P-116	-	Preservation-Packaging, Methods of.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, Code ATT, 2800 South 20th Street, Philadelphia, Pa. 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

STANDARDS

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications, standards, drawings, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

D1248 Polyethylene Plastics Molding and Extrusion Materials.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, Pa. 19103.

3. REQUIREMENTS

3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection and approval (see 4.1.2.1 and 6.2).

3.2 Materials. The wash basin, emesis basin, soap holder and tumbler shall be fabricated of medium impact, high density polyethylene, flexible polypropylene, or flexible polystyrene. Polyethylene, when used, shall conform to ASTM D1248, type III, Class B, Category 2, grade E3.

3.3 Design and construction. Each kit shall consist of an emesis basin, a tumbler, and a soap holder placed in a wash basin and packaged ready for use in a closed, transparent polyethylene bag approximately 0.003 inch (0.076 millimeter-mm) thick. The edges of all items shall be broken to preclude injury to patients. All items shall be sturdy enough to permit repeated use and shall be capable of being washed in hot water. Each item shall be free from objectionable odor, sharp edges, cracks, holes or thin areas. All items shall rest evenly on a flat surface and shall be of the same solid color.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

3.3.1 Wash basin. The wash basin (figure 1) shall have a capacity of 5-quarts, (4732 millilitres-ml) minimum.

3.3.2 Emesis basin. The emesis basin (figure 2) shall have a capacity of 1/2 quart, (473 ml) minimum.

3.3.3 Soap holder. The soap holder (figure 3) shall be capable of accepting a bar of soap 4 inches (101 mm) long and 2 1/2 inches (63 mm) wide. Along the inside bottom of the holder, perpendicular to the long axis of the holder there shall be four evenly spaced, raised ridges to allow for drainage.

3.3.4 Tumbler. The tumbler (figure 4) shall have a capacity of 8 ounces, (286 ml) minimum.

3.4 Drop test. The wash basin, emesis basin, soap holder and tumbler shall not show evidence of cracks, chips, or other defects when tested as specified in 4.4.1.

3.5 Temperature test. The wash basin, emesis basin, soap holder and tumbler shall not show evidence of leakage, cracks, warping, or other deformation when tested as specified in 4.4.2.

3.6 Identification marking. Each wash basin, emesis basin, soap holder and tumbler shall be marked permanently and legibly with the manufacturer's name or registered trademark.


3.7 Workmanship. Workmanship shall be first class throughout. Wash basins, emesis basins, soap holders and tumblers shall be free from defects which detract from their appearance or may impair their serviceability. All burrs and sharp edges shall be removed.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

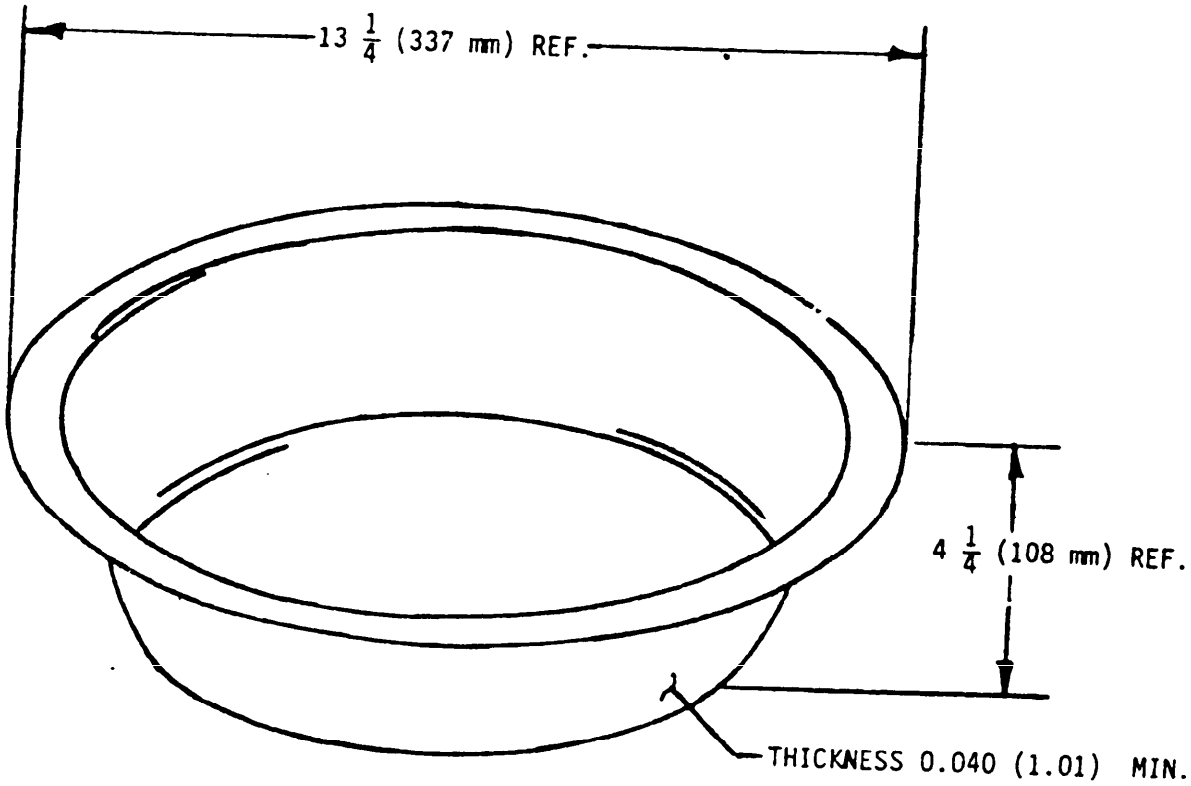


NOTES

1. PRIMARY DIMENSIONS ARE IN INCHES AND SECONDARY DIMENSIONS ARE IN MILLIMETRES.
2. MANUFACTURING TOLERANCES SHALL BE ± 1/32 INCH (0.79 MILLIMETRES).
3. VARIATIONS TO SHAPE AND STYLE WHICH DO NOT CONFLICT WITH INTENDED USE OF ITEM OR SPECIFICATION REQUIREMENTS SHALL BE ACCEPTABLE.

FIGURE 1. Wash Basin

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

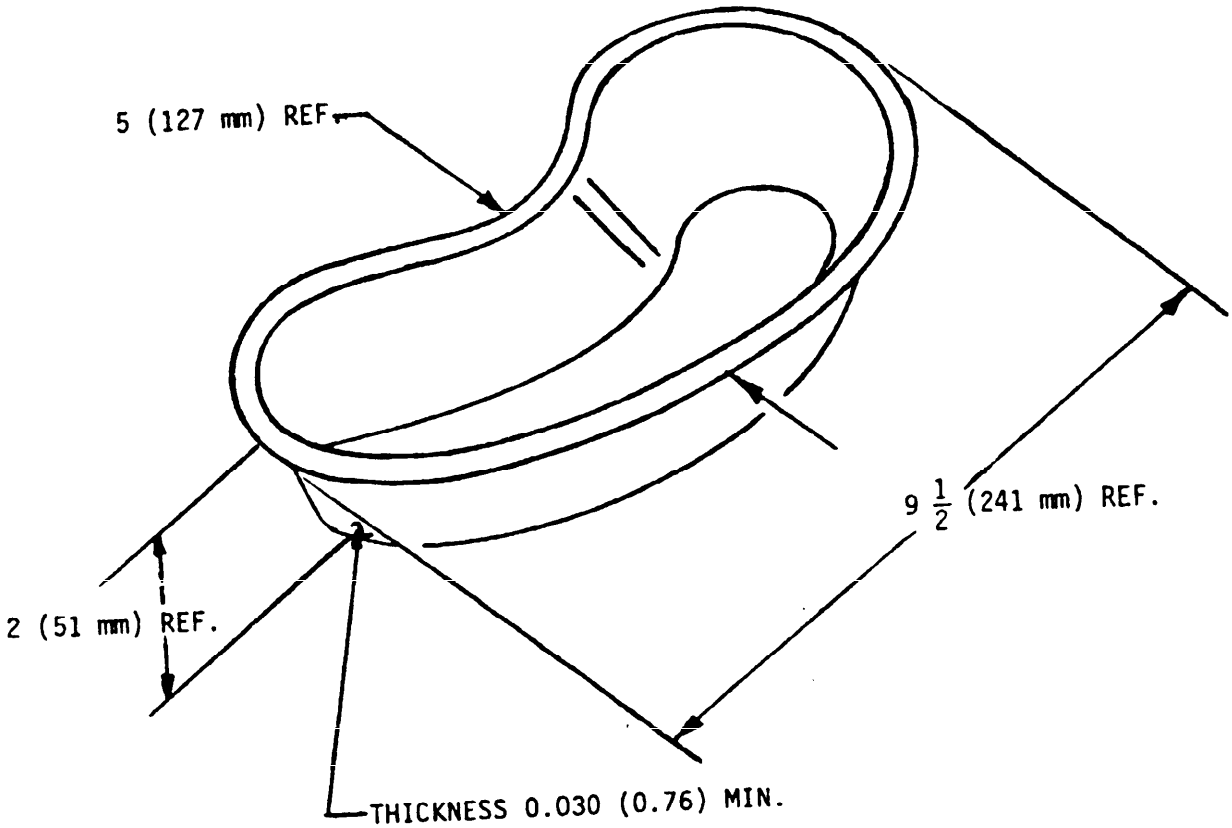


NOTES

1. PRIMARY DIMENSIONS ARE IN INCHES AND SECONDARY DIMENSIONS ARE IN MILLIMETRES.
2. MANUFACTURING TOLERANCES SHALL BE ± 1/32 INCH (0.79 MILLIMETRES).
3. VARIATIONS TO SHAPE AND STYLE WHICH DO NOT CONFLICT WITH INTENDED USE OF ITEM OR SPECIFICATION REQUIREMENTS SHALL BE ACCEPTABLE.

FIGURE 2. Emesis Basin

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

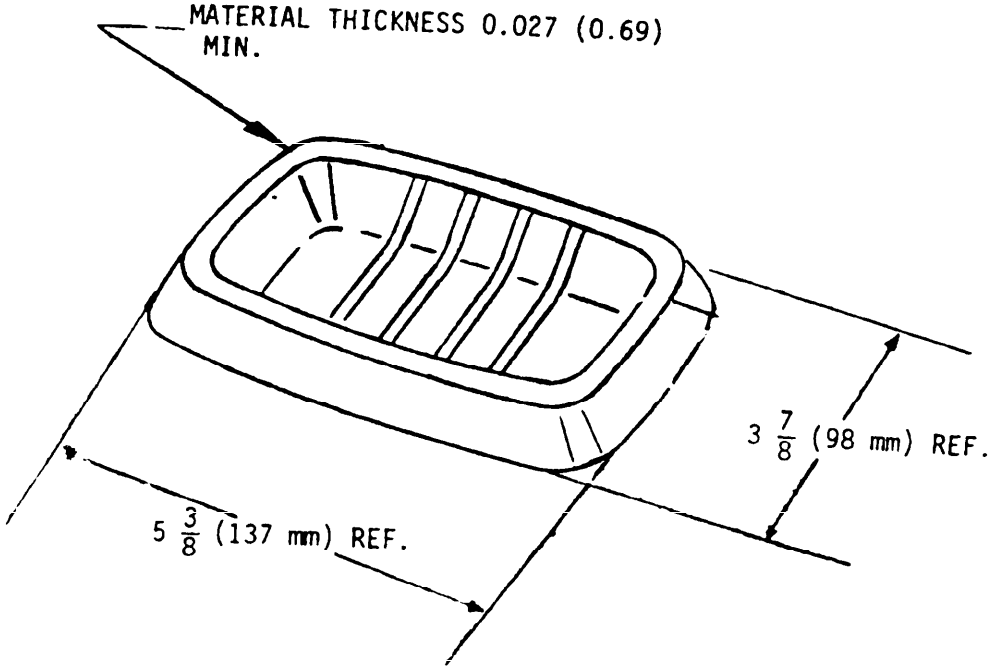


NOTES

1. MANUFACTURING TOLERANCES SHALL BE ± 1/32 INCH (0.79 MILLIMETRES).
2. VARIATIONS TO SHAPE AND STYLE WHICH DO NOT CONFLICT WITH INTENDED USE OF ITEM OR SPECIFICATION REQUIREMENTS SHALL BE ACCEPTABLE.

FIGURE 3. Soap Holder

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

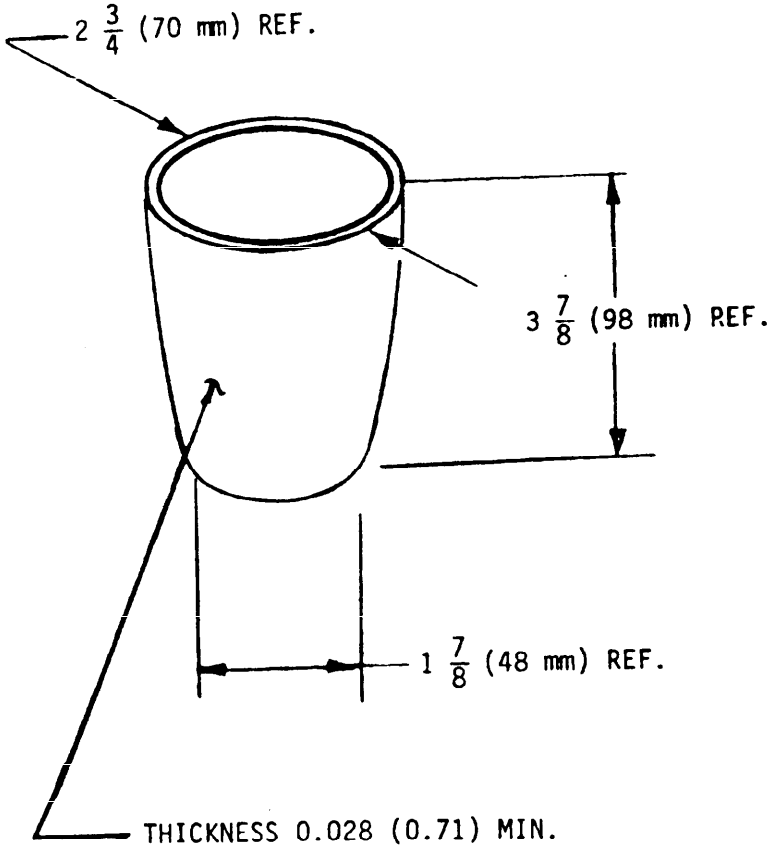

NOTES

1. PRIMARY DIMENSIONS ARE IN INCHES AND SECONDARY DIMENSIONS ARE IN MILLIMETRES.
2. MANUFACTURING TOLERANCES SHALL BE ± 1/32 INCH (0.79 MILLIMETRES).
3. VARIATIONS TO SHAPE AND STYLE WHICH DO NOT CONFLICT WITH INTENDED USE OF ITEM OR SPECIFICATION REQUIREMENTS SHALL BE ACCEPTABLE.

FIGURE 4. Tumbler

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

4.1.2.1.1 First article inspection. First article inspection shall be performed on utility kits when a first article sample is required (see 3.1). This inspection shall include examination of 4.3. and tests of 4.4.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.3 and tests of 4.4.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and table I. The unit of product for sampling purposes shall be one each of; wash basin, emesis basin, soap holder and tumbler.

TABLE I. Sampling for examination.

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Total defects (Major and Minor combined)	II	4.0
For dimensional examination	S-1	4.0

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:43Z
Check the source to verify that this is the currentversion before use.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II, for an inspection level of S-2. Acceptance number shall be zero for all sample sizes. The unit of product for sampling purposes shall be one each of: wash basin, emesis basin, soap holder and tumbler.

TABLE II. Sampling for tests.

Characteristic	Requirement	Test Procedure
Drop test	3.4	4.4.1
Temperature test	3.5	4.4.2

4.3 Examination. The utility kit shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table III. Examination shall not be restricted to the classified possible defects listed below.

TABLE III. Classification of defects.

Category	Defect
Major:	
101	Not free of cracks, holes, tears or thin areas.
102	Not free of burrs, sharp edges.
103	Any component missing.
104	Color not solid or not uniform.
105	Not clean, not free of grease, oil, dirt, other foreign matter.
Minor:	
201	Identification marking not present, complete, legible, correct.
202	Finish not free of scratches, mars, chips, etc.
203	Bags not closed.
204	Any item does not rest evenly on flat surface.
205	Any item not free of objectionable odor.

4.3.2 Dimensional examination. The utility kit shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

4.3.3 Packaging inspection. The inspection of the packaging and interior package marking shall be in accordance with the group A quality conformance inspection requirements of MIL-P-116. The inspections of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Drop test. The wash basin, emesis basin, soap holder, and tumbler shall be dropped from a height of 36 inches onto a concrete floor. The attitude of the items during the drop shall not be controlled. Each item shall pass this test regardless of it's attitude when its contacts the concrete floor.

4.4.2 Temperature test. The wash basin, emesis basin, soap holder and tumbler shall be placed on a flat surface at room temperature. They shall be filled with water at 140^{0} + 10^{0}, - 0^{0} F (60^{0} + 6^{0}, - 0^{0} C) and left filled for one hour.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Unit packaging. Each kit shall be packaged in accordance with MIL-P-116, method III. Each kit shall be packaged clean and ready for use in a transparent polyethylene bag, wall thickness approximately 3 mils. Closure shall be adequate to maintain cleanliness, and to prevent accidental opening.

5.1.2 Level C. Kits shall be packaged in standard commercial containers the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Twelve (12) kits shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather resistant, grade V3C. Closure and strapping shall be as specified in the appendix of the applicable box specification.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:43Z
Check the source to verify that this is the current version before use.

5.2.2 Level B. Twelve (12) kits shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, type CF, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. Kits shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking. Each unit package and exterior container shall be marked as specified in MIL-STD-129.

6. NOTES

6.1 Intended use. This patient utility kit is intended for use by patients in government hospitals.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

a. Title, number and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
c. When a first article is required (see 3.1, 4.1.2.1 and 6.3).

6.3 First article. When a first article is required, it shall be tested under the appropriate provisions of 7-104.55 of Armed Services Procurement Regulation. The contract or purchase order specifies the quantity, procedure for delivery and other specific instructions for inspection and approval of the first article.

6.4 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6530-00-890-1786	PATIENT UTILITY KIT, Plastic

6.5 Changes from previous issue. Asterisks are not used in this revision to identify changes with respect to the previous issue, due to the extensiveness of the changes.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
DSA - DM

Project No. 6530-1407

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-P-36506B PATIENT UTILITY KIT

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:43Z
Check the source to verify that this is the current version before use.