MILITARY SPECIFICATION

SCISSORS, IRIS, CURVED, 4-7/8 INCH

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of curved iris scissors for use in the practice of eye surgery.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Set-up.

Military

MIL-P-116	Preservation, Methods of
MIL-L-10547	Liners, Case and Sheet, Overwrap; Watervaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

Federal Test Method Standard 151

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The scissors shall be fabricated of class 4, type 420 corrosion-resistant steel in accordance with the requirements of GG-I-526, except that the minimum carbon content of the blade material shall be .30 percent.

3.2 Hardness. After proper stress relieving, the Rockwell hardness of the material specified in 3.1 shall be Rc 50-55, when tested as specified in 4.4.1.

3.3 Style, design and dimensions. Shall be a curved iris scissors, double sharp points and spring handle. Scissors shall be in accordance with Figure 1.

3.4 Construction.

3.4.1 Serrations. Serrations in handles shall be in accordance with the requirements of GG-I-526.

3.4.2 Locks. Shall be screw-type lock, in accordance with the requirements of GG-I-526.

3.4.3 Cutting edges. Cutting edges of blades shall be in accordance with the requirements of GG-I-526.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

3.4.3.1 Scissors performance. The scissors when tested as specified in GG-I-526 shall cut a continuous length of 3/32 inch of the test material. This cutting requirement shall apply for the entire length of the cut, specified herein, including the tips of the scissors. All three cuts made with each scissors tested shall meet the requirement of GG-I-526. The test material shall be rubber dam meeting the requirements of the Defense Medical Purchase Description for Stock No. 6520-00-754-2795, Rubber Dam, Medium, 6 inches square, 36s.

3.4.4 Finish. Finish shall be mirror, except that the inside of the blades may be crocus finish, in accordance with the requirements of GG-I-526.

3.5 Corrosion-resistance. Scissors shall meet the requirements for the boil test and the copper sulfate test of GG-I-526.

3.6 Identification marking. Scissors made in U.S.A. shall be marked with the name or registered trademark of the contractor and the word "stainless." Scissors of foreign (other than U.S.) manufacture, shall be marked with the name of the country of origin, the name or registered trademark of the contractor, and the word "stainless."

3.7 Workmanship. Workmanship shall be first class throughout. Scissors shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in Table I. The unit of product for examination purposes shall be one iris scissors.

Table I. Sampling Criteria for Examination

Type of defect	Inspection level	AQL (Percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. Unit of product for test purposes shall be one iris scissors.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

Table II. Sampling Criteria for Tests.

Component	Characteristic	Req.	Test Procedure	Unit of Product	Insp. level	AQL
Scissors	Hardness	3.2	4.4.1	1-Scissors	S-2	*
	Scissors performance test	3.4.2.1	GG-I-526	1-Scissors	II	1.0
	Copper Sulfate	GG-I-526	GG-I-526	1-Scissors	S-2	*
	Boil test	GG-I-526	GG-I-526	1-Scissors	S-2	*

*Acceptance number shall be zero for all sample sizes.

4.2.3 Raw materials. Four ounces of each lot of each metal used in construction of the scissors shall be selected for chemical analysis.

4.2.4 Test sample. Where possible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination. The iris scissors shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in Table I and III. Examination, however, shall not be restricted to defects listed in Table III. Any iris scissors in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.

Table III Classification of Defects

Categories	Defects
Critical	None defined
Major	
101	Style and design not as specified.
102	Scissors not free from cracks, pits, dents, nicks and burrs.
Minor	
201	Finish not as specified.
202	Instrument not permanently and legibly marked with either the name or trademark of the contractor.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Hardness test. Hardness shall be determined in accordance with methods 243 (Rockwell) or 244 Diamond Pyramid) of Federal Test Method Standard No. 151.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One scissors, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	288 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IC-1.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-676, except commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Fiberboard boxes shall conform to special requirements specified in PPP-B-636.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure of wood boxes shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes, shall conform to Method II of PPP-B-636. In addition, fiberboard boxes shall conform to the special requirements specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The iris scissors are intended for use in the practice of eye surgery.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

6.3 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

National Stock No.	Item Identification
6515-00-619-8305	SCISSORS, IRIS, Curved, 4-7/8 inch

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 3, dated 28 May 1964.

Custodians:

Army - MD
Navy - MS
Air Force - 03

Review activities:


Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1767

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

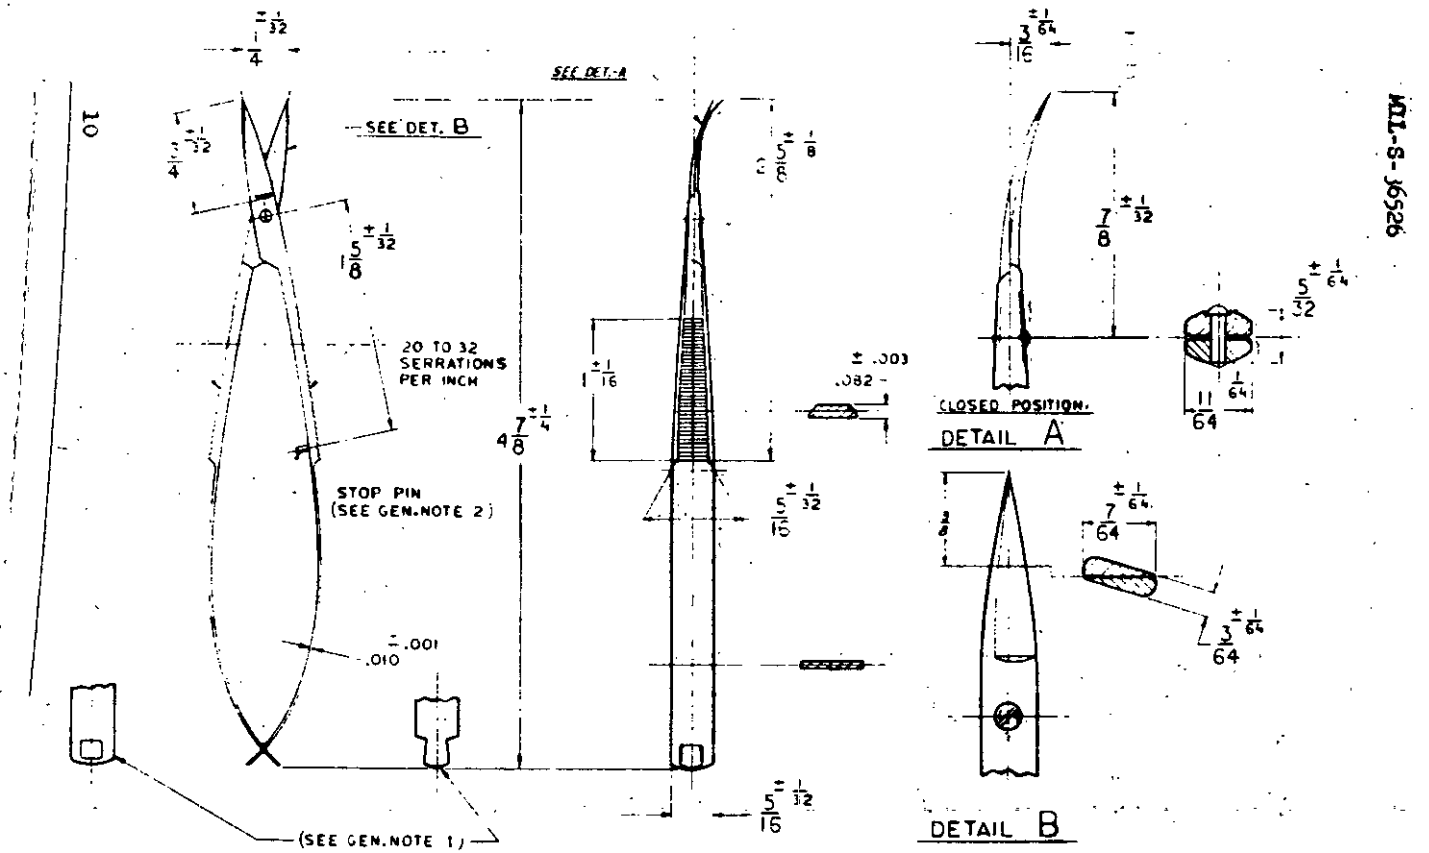

NSN 6515-00-619-8305

GENERAL NOTES:

1. MALE SHANK MEMBER (I.E., AT PROXIMAL END) SHALL FIT THRU RECTANGULAR HOLE IN FEMALE SHANK DIAGONALLY ONLY.
2. STOP PIN SHALL STOP BLADES FROM OVERLAPPING WHEN IN CLOSED POSITION. (SEE DET.-B)
3. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY, AND FIRST QUALITY WORKMANSHIP.
4. UNLESS OTHERWISE SPECIFIED ALL DIMENSIONS ARE IN INCHES.

FIGURE 1

SCISSORS, IRIS, CURVED, $4\frac{7}{8}$ INCH

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

FOLD

POSTAGE AND FEES PAID

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

COMMANDER
DEFENSE PERSONNELL SUPPORT CENTER
ATTN: DPSC-ATTS
2800 SOUTH 20th STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

S/N 0102-014-1802

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:45Z
Check the source to verify that this is the current version before use.