
AMSC N/A
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.


REVIEWER ACTIVITIES: ARMY - ME
NAVY - OS
AIR FORCE - 82

USER ACTIVITIES: ARMY - MD, DM
NAVY - MS


FED. SUP CLASS
6640

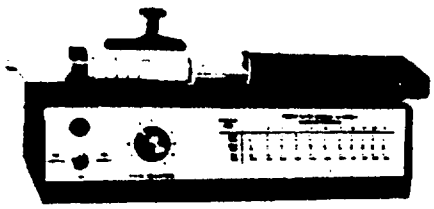

MS36590-1

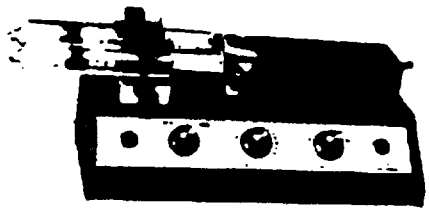

MS36590-2

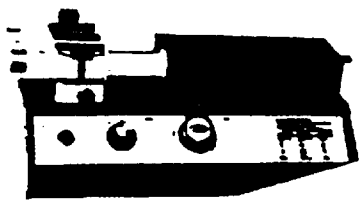

CANCELLED
CANCELLED AFTER 9 OCT 1991
NO SUPERSEDING STANDARD

		NUMBER OF SYRINGES
MS3	0.07 µL/day to 140 mL/min	1 3 up to 30 cc 2 up to 50 cc 1 - 100 cc

MATERIAL: Housing shall be made of vinyl coated aluminum. All other materials shall be as required for satisfactory functioning.

DESIGN: Pumps shall meet the following design requirements:

MS36590-1 shall hold a single pump for continuous infusion and shall hold all types of syringes in any size up to 50 mL. Pumps shall be precalibrated and highly reproducible with eleven rates in each range and a total of 22 for each syringe size. Pulser motor shall provide power through set of gears moving syringe piston smoothly down its barrel. Motor shall stall at end of run to prevent syringe damage.

MS36590-2 pump shall have direct dialing of 19 most frequently used flow rates and is precalibrated to infuse or withdraw fluids, only one syringe can be held in holder for withdrawal mode. Gear drive shall provide a continuous and uniform flow at all except slowest rates with largest syringes. Slip clutch shall protect driver motor and syringe at end of travel.

(A) CANCELLATION

APPROVED 20 JUL 1983 REVISED (A) 9 OCT 1991

P.A.	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
EA		PUMP, SYRINGE	MS36590
Other Coor: MS 99			
Procurement Specifications: NONE	SUPERSEDES:		SHEET 1 OF 2

DD FORM 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

CANCELLATION

Project Number 6640-1735-03

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:44Z
Check the source to verify that this is the current version before use.

FED. SUP CLASS
6640

MS36590-3 pump shall be continuously variable with complete range covered by direct dialing and no gear changes. Syringe holder shall meet all pumping needs, accepting syringes of any type including microliter. Pump drive shall be geared to maintain uniform flow at all speeds, with built-in slip clutch protection. Electronic feedback circuit controls reproducibility regardless of back pressure variations. Stabilized DC motor shall drive syringe piston for uniform fluid flow.

Syringe pumps shall be enclosed to prevent damage from solutions and mechanism shall allow for quick set-up for filling. Units shall operate on 115/120V AC, 50/60Hz.

All electrical components shall conform to the standards of Underwriters Laboratories, Incorporated.

NOTE: Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements specified herein.

FSCM: 13134 and 59728.

CANCELLED
CANCELLED AFTER
NO SUPERSEDING STANDARD

USER ACTIVITIES:

REVIEWER ACTIVITIES:

...ilitary standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

APPROVED 3 OCT 1975 REVISED (A)

P.A. Other Cust	INTERNATIONAL INTEREST	TITLE PUMP, SYRINGE	MILITARY STANDARD MS36590
Procurement Specifications	SUPERSEDES		SHEET 2 OF 2

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE Project Number 6640-1735-03

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:44Z
Check the source to verify that this is the current version before use.