MIL-G-36339C
14 March 1969
SUPERSEDING
MIL-G-36339B
21 June 1968

MILITARY SPECIFICATION

GLOVE, PATIENT EXAMINING AND TREATMENT

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers a prepackaged, sterile, disposable, impermeable, light-weight seamless plastic glove of one utility size for all wearers, which fits either hand. Glove shall be suitable for medical use in examinations, diagnostic and therapeutic procedures by physicians, nurses and paramedical personnel in clinic and nursing-unit care.

2. APPLICABLE DOCUMENTS

* 2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Boxes, Fiberboard
PPP-B-676	Boxes, Set-up

Military

MIL-L-10547	Liners, Case, And Sheet Overwrap; Water-Vaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN SOCIETY FOR TESTING MATERIALS (A.S.T.M.)

D882	Tests for Tensile Properties of Thin Plastic Sheeting.

(Application for copies should be addressed to the American Society for Testing Materials, 116 Race Street, Philadelphia, Pennsylvania 19103.)

U.S. PHARMACOPOEIAL CONVENTION, INC. (U.S.P)
Pharmacopeia of the United States.

(Application for copies should be addressed to the Mack Publishing Company, Easton, Pennsylvania 18042.)

3. REQUIREMENTS

3.1 Material.

* 3.1.1 Glove. The glove shall be fabricated from virgin, translucent polyvinyl chloride.

* 3.1.2 Dusting Powder. Gloves shall be uniformly prepowdered on the interior only with a minimum of absorbable dusting powder meeting the following requirements: Powder shall be a white, odorless powder and shall be in accordance with the tests, standards, and requirements of the latest revision of the Pharmacopeia of the United States (U.S.P.) for Absorbable Dusting Powder.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

* 3.2 Style and design. The patient examining glove shall be constructed in one piece, free of seams and welts, and shall have a smooth finish. Shall be a five-fingered glove suitable for use on either hand. A small continuous bead shall be formed on the glove circumference at the cuff end to prevent tearing. The glove shall be constructed with maximum tactility, and straight or curved, well-fitting fingers that permit maximum freedom of movement. The palm section shall be of sufficient width to permit comfortable flexing of the hands. The glove shall be supplied in a folded inner wrapper which in turn shall be enclosed in an outer wrapper as specified in 3.2.2. The glove shall be placed flat, prior to folding the inner wrapper over glove, with the cuff folded over to retain sterility for 1½ to 3½ inches. The inner wrapper shall be of sufficient size to permit such flat placement of the glove and shall completely cover and separate glove from outer wrapper. The inner wrapper shall be folded in such a manner as to permit easy removal of the glove. Inner wrapper shall have the "CUFF END" and "THUMB" clearly identified with a permanent type marking (e.g., ink stamping). The glove shall not slide in the package or adhere to the inner wrapper while in storage.

* 3.2.1 Dimensions. The glove shall have the dimensions (in inches) as indicated in table I.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

TABLE I. Characteristic	Dimensions
Overall length	10 ± 1, -1/4
Flat width at wrist	4-1/4 ±1/2, -1/4
Flat width at palm at base of thumb	4-1/4 ± 1/4
Length of thumb	2-3/8 ± 1/4
Length of little finger	2-1/4 ± 1/8
Length of middle finger	3 ± 1/4
Length of index and ring fingers	2-7/8 ± 3/8
Flat width of thumb at base	1-1/2, ± 1/8
Flat width of thumb 3/4 inch from tip	1-1/4, ± 1/4, -3/16
Flat width of base of index, middle and ring fingers	1-1/4 ± 1/8
Same as line above, 3/4 inch from tips	1-1/8 ± 1/8
Flat width of base of little finger	1-1/8 ± 1/8
Same as line above, 3/4 inch from tip	1-1/8 ± 1/8
Thickness at finger tips	0.002 to 0.0045
Thickness at remainder of glove (except for area adjacent to cuff head)	0.005 to 0.008

* 3.2.2 Outer wrapper (envelope). The outer wrapper (envelope) shall completely enclose the inner wrapper and glove, and shall be capable of maintaining sterility of the glove. The inner wrapper shall be permanently imprinted to denote "CUFF END" and "THUMB" to assure strict aseptic removal technique.Outer wrapper shall be so designed as to permit ready dispensing of the contents by sterile techniques. Closure of the outer wrapper shall be accomplished by heat or cold sealing. The outer wrapper shall be a sealed, peel-back outer wrapper. The peel-back design shall include two free tabs along the top edge of the wrapper. The tabs shall be capable of being readily peeled back along the sealed edges to expose the inner wrapper as shown in figure 1. Opening (peeling) the outer wrapper shall be accomplished without contaminating or damaging the inner wrapper and the glove. Each unit package (100 gloves) shall be made waterproof by placing unit package in a sealed plastic bag. The sealed plastic bag may be on the interior or exterior of the unit package. There shall be no evidence of moisture within the plastic bag, when plastic bag of unit package is opened after subjection to leakage test specified in 4.4.4.

* 3.3 Physical requirements. The gloves shall comply with the physical requirements contained in table II. Tests for physical requirements shall be conducted as specified in 4.4.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

TABLE II. Physical Requirements

Tensile strength - pounds per square inch (average)	1500 min. *
Tensile strength - pounds per square inch (single glove)	1300 min.
Breaking strength - pounds per inch of width	5 min.
Percentage elongation at break	280 min.

* The tensile strength shall be run on a minimum of 50 gloves and represents an average value.
No single glove shall run below 1300 pounds per square inch.

3.4 Sterility. Gloves shall be sterile when tested as specified in 4.4.2.

3.5 Freedom from pinholes. The glove shall be supplied free of pinholes, and when tested as specified in 4.4.3, the glove shall not leak or show sign of air bubbles.

* 3.6 Finish. The glove shall have a visually dull but smooth-to-the-touch exterior, and visually glossy and smooth-to-the-touch interior surface. The glove shall be free from holes, visible ingrained particles, tackiness, bloom, strings, bleeding, and other imperfections.

* 3.7 Low temperature flexibility. The glove shall not crack at -20°F when tested as specified in 4.4.5.

* 3.8 High temperature exposure. The glove shall withstand exposure at 165°F for 72 hours without evidence of tackiness, plasticizer exudation, or other deterioration when tested as specified in 4.4.6.

3.9 Instructions. Each envelope shall be labeled with instructions for withdrawing and donning the glove without compromising its sterility.

3.10 Certificate of sterility. A certificate of sterility, listing all sterility lot or control numbers, shall state that representative samples from each lot or control have been tested and found to be sterile. The certificate shall include the method used in determing sterility and the test results. For destination inspection only, certificates of sterility shall be submitted by the contractor directly to Defense Personnel Support Center, Directorate of Medical Materiel, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, ATTN: DPSC-ATQ, and one copy shall be forwarded with each shipment to the consignee. For source inspection, certificates shall be furnished to the procuring activity via the Government inspector.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

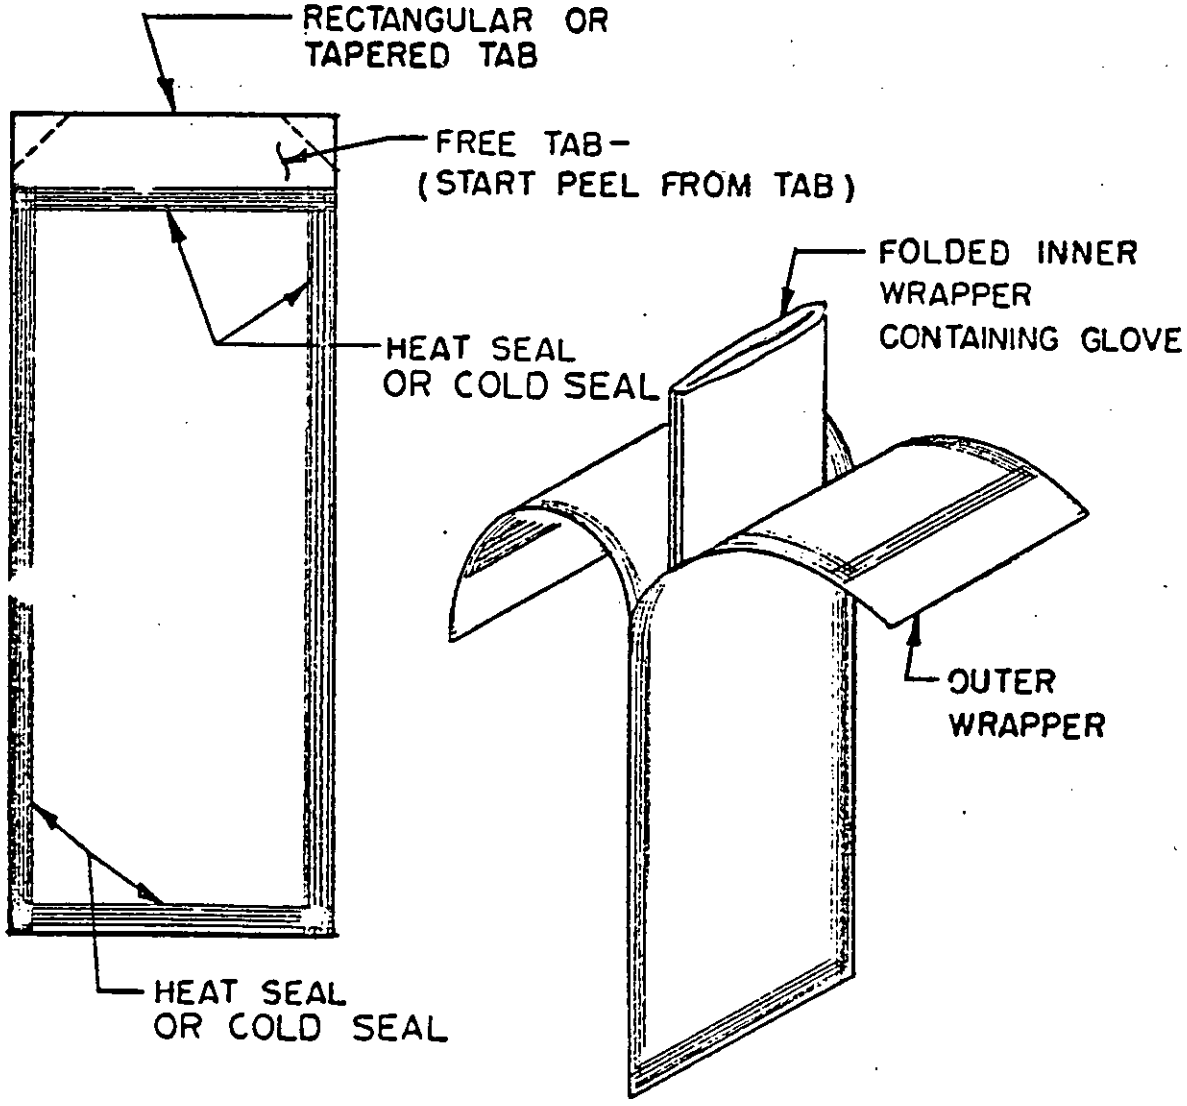


FIGURE 1

PEEL-PACK OUTER WRAPPER
FOR GENERAL STYLE ONLY

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

3.11 Workmanship. Workmanship shall be first class throughout. Gloves shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in table III. The unit of product for examination shall be one glove.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

TABLE III. Sampling for Examination

Type defect	Inspection level	AQL (percent defective)*
Major	S-3	2.5
Minor	S-3	2.5

* If acceptance number is not exceeded, lot shall be accepted.

If rejection number is equaled or exceeded, inspection at level II may be performed to determine final rejection or acceptance.

* 4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and in accordance with the table IV.

TABLE IV. Sampling for Tests

Characteristic	Unit of Product	Requirement	Test Procedure	Inspection level	AQL (percent defective
Dusting powder	Glove	3.1.2	U.S.P.	S-3	2.5
Tensile strength	Glove	3.3	4.4.1	S-3 **	2.5
Percentage elongation	Glove	3.3	4.4.1	S-3	2.5
Sterility	Glove	3.4	4.4.2	S-3	*
Freedom from pinholes	Glove	3.5	4.4.3	S-3	*
Low temperature flexibility	Glove	3.7	4.4.5	S-1	2.5
High temperature exposure	Glove	3.8	4.4.6	S-1	2.5

* Acceptance number shall be zero.

** Tensile strength shall be run on a minimum of 50 gloves.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

4.2.3 Sample unit usage. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination. The gloves shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in tables III and V. Inspection, however, shall not be restricted to defects listed in table V. Any glove in the sample containing one or more defects shall be rejected (defective) and if the number of defective gloves in any sample exceeds the acceptance number for that sample, the lot represented by the sample shall be rejected (see 4.2.1).

TABLE V. Classification of Defects in Accordance with MIL-STD-105

Categories	Defects
Critical:	None defined
Major	
101	Tears, large holes.
102	Large open blisters.
103	Imbedded grit-like particles.
104	Ingrained grit-like particles clearly noticeable without distending the glove.
105	Excessively thin spots (under 0.002 inch).
106	Tackiness.
107	Pinholes.
108	No inner wrapper included.
109	CUFF END and THUMB not identified on inner wrapper.
110	Glove adhering to inner wrapper.
111	Gloves not having a small continuous bead located upon the cuff end.
112	Gloves powdered on exterior.
113	Foreign matter present.
Minor:	
201	Fingertips over 0.0045 inch.
202	Palm thickness over 0.008 inch.
203	Wrist thickness over 0.008 inch.
204	Short, gloves under 9-3/4 inches.
205	Excessive blisters that would interfere with accepted professional use (clusters of small blisters as contrasted with large open blisters).
206	Bloom, bleeding, strings, and other imperfections.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Physical requirements tests shall be conducted in accordance with American Society for Testing Materials D882.

* 4.4.2 Sterility test. Samples of the finished gloves shall be tested for sterility, in accordance with the current edition of the Pharmacopeia of the United States (U.S.P.) for "Purified Cotton, Gauze, Surgical Dressings and Related Materials".

4.4.3 Pinhole test. Gloves shall be filled with 300 milliliters of water and held suspended from the cuff end for 5 minutes. Gloves shall be examined for leaks.

* 4.4.4 Leakage test. (unit package). The finished sealed unit package (comprising 100 gloves) shall be held at ambient conditions for at least 4 hours prior to performing the submersion test described herein. The samples shall be immersed in water at a temperature of 35°F ± 2°F for 1 hour. The sample shall be immersed so that the top surface of the sample is 1 inch below the surface of the water. After removal, the sealed outer wrapper, or the sealed unit package shall be opened and inspected.

* 4.4.5 Low temperature flexibility. The glove shall be placed on a wooden rack and exposed in a low temperature cabinet so that it is at a temperature of -20°F for a minimum of 1/2 hour. It is then manipulated with a stick to determine if it will flex without cracking.

* 4.4.6 High temperature exposure. The glove shall be exposed in a mechanical convection oven for 72 hours at 165°F. Upon removal and cooling of the glove, it shall be examined for exudation, tackiness or other deterioration.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One package (100 gloves), as specified, constitute one unit of issue.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

5.1.2 Packaging quantities. The number of units of issue indicated in table VI shall be packaged in each unit and exterior container, as applicable, for the required level of protection specified in the procurement document.

TABLE VI. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	10 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package.

5.1.3.1.1 Envelope. Each glove shall be packaged in an envelope which shall be capable of maintaining sterility of contents as specified in paragraph 3.2.2.

* 5.1.3.1.2 Carton. Each unit (100 gloves) shall be packaged in a carton of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676 except that commercial colors are acceptable. Closure of carton shall be adequate to prevent spilling of contents under normal handling. Waterproofing shall be as specified in 3.2.2.

5.2 Packing.

5.2.1 Level A.

* 5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table III, using type I, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant. Closure and strapping shall be in accordance with the appendix of the applicable box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

* 5.2.1.2 Case liner. Each level A wood box shall be lined with a water-proof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table II, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic. Closure shall be in accordance with the appendix of the applicable box specification.

5.3 Marking.

5.3.1 Envelope. Each envelope shall be labeled with instructions for withdrawing and donning glove without compromising sterility. Lot (control) number, item identification, name of contractor and the following legends shall be shown: "DISPOSABLE", "FITS EITHER HAND" and "STERILITY GUARANTEED UNLESS PACKAGE IS DAMAGED OR OPENED" or similar statement.

5.3.2 Unit package. Each unit package (carton) shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number, name of contractor, lot (control) number, and the legend "STERILE" shall be shown.

5.3.3 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Lot (control) numbers shall be shown.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.

(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

6.2 This specification does not include all types, classes, grades, and sizes of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, which are normally procured to meet Military requirements.

* 6.3 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE

3. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil – Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.