MIL-L-36353B
11 March 1976
SUPERSEDING
MIL-L-36353A
7 November 1974

MILITARY SPECIFICATION

LIGHT, SURGICAL, STAND

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of explosion-proof, mobile surgical operating room light.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

Federal

PPP-B-601	- Boxes, Wood, Cleated-Plywood.
PPP-B-621	- Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	- Boxes, Shipping, Fiberboard.

Military

MIL-M-7298	- Manual, Technical, Commercial Equipment.
MIL-L-10547	- Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Federal

FED-STD-595	- Colors

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

NATIONAL FIRE PROTECTION ASSOCIATION (NFPA)

NFPA NO. 56A Standard For the Use of Inhalation Anesthetics

(Application for copies should be addressed to the National Fire Protection Association, 60 Batterymarch Street, Boston, MA 62110.)

UNDERWRITERS' LABORATORIES, INC.

UL57	Electric Lighting Fixtures
UL781	Portable Electric Lighting Units, For Use in Hazardous Locations Class I Groups C and D Class II Group G

(Application for copies should be addressed to the Underwriters' Laboratories, Inc., 207 East Ohio Street, Chicago, IL 60611, 333 Pfingsten Rd., Northbrook, IL 60052, 1285 Walt Whitman Rd., Melville, LI, NY 11746 and 1655 Scott Blvd., Santa Clara, CA 95050.)

3. REQUIREMENTS

* 3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection and approval (see 4.1.2.1 and 6.2).

3.2 Fire and casualty hazards.

3.2.1 The contractor shall submit proof, prior to delivery, that the items to be delivered under the contract conform to the applicable requirements of UL57, UL781 and NFPA 56A. Paragraph 31.1 of UL781 shall be modified as follows: First sentence after "center line" delete "or" and substitute "and". Proof shall consist of one of the following:

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

A. UL label affixed to the product. The contractor shall agree to have Underwriters' Laboratories, Inc. forward a copy of the UL report of testing directly to the Contracting Officer, upon the latter's request.

B. Laboratory report from a nationally recognized independent laboratory. The laboratory must be adequately equipped and competent to determine compliance with these standards. The Government reserves the right to require a facilities report and to conduct a facilities survey. The laboratory report shall include actual test methods, data taken, and results of tests. Detailed findings of examinations necessary to determine compliance shall also be included. The test report shall also have a section that describes the test sample in such a way that the report can be used to insure identity of production items with the test sample. This section shall be supplemented with construction information such as materials used, spacings between electrical components, types of bushings, photographs, wiring diagrams, sketches, and parts list, all appropriately identified. Compliance with this paragraph does not excuse compliance with all other requirements of the contract and specifications.

3.3 Material. Material shall be as specified herein, of the best quality used for the purpose in commercial practice, and shall be free of defects and imperfections that may affect the serviceability of the finished light.

3.4 Design. Shall be a mobile, explosion proof, surgical operating room lamp, constructed to comply with Underwriters' Laboratories' requirements and NFPA 56A. The lamp shall consist essentially of a base, a telescopic upright, a pantograph type of extension arm, a lamphead, and electric cord.

3.4.1 Construction. Construction shall be as shown on Figures 1 or 2 as specified herein.

* 3.4.2 Base. The light shall have a circular base 24 inches ± 1 inch diameter, of suitable weight and design to provide a unit capable of passing the stability test specified in 4.4.1.4. The base shall be fabricated from smoothly finished pressed steel. As an alternate, a cast iron base with a spun sheet metal cover, of steel, aluminum, or brass conforming to the shape of the base and held down by the upright, shall be acceptable. The steel cover or pressed steel base shall be finished as specified in 3.10, and the cast-iron shall be finished with a coat of primer to prevent corrosion. The base shall be mounted on eight swivel ball-bearing casters

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

with 2 ± 1/16 inches diameter electrically conductive rubber wheels. As an alternate, the base shall be provided with three ball bearing rubber casters 2 ± 1/16 inches in diameter plus three steel ball casters 1-1/8 ± 1/16 inches in diameter. The casters shall be designed and constructed so that there will be positive metal-to-metal contact with the lamp base. All casters shall rest uniformly on a flat surface without any wobble. No caster shall contact casting such as to bind or impair caster function. The tires shall be of such composition and construction as to pass the electrical conductivity test specified in 4.4.1.5.

* 3.4.3 Vertical standard. The vertical standard shall be rigidly attached to the base in such a manner as to provide a permanent joint which shall not loosen under normal service usage. The standard shall consist of two telescoping tubes and a clamping device. A counterbalance spring shall be provided within the standard so that vertical adjustment of the lamphead may be made with little effort. A stop shall be provided to prevent the inner tube from being ejected when the clamp is released. The clamping device shall be completely concealed within the tubing, and shall be of such design that the tubing shall not be marred or defaced. The outer tube shall be fabricated from 2 inch diameter steel or brass tubing not less than .065 inch thick (No. 16 Birmingham Wire (B.W.) gage). The inner tube shall be fabricated from either steel or brass not less than .095 inch thick (No. 13 B.W. gage). The height of the upper pivot point of the pantograph arm above the floor, with the telescoping rod fully extended, shall be approximately 85 inches. The telescopic section of the upright shall be of such dimension that the lamphead can be adjusted vertically through a distance of 27 ± 1/4 inches.

* 3.4.4 Extension arm. The extension arm shall be the pantograph-type constructed with two, 5/8 inch diameter, steel or brass tubes as shown in figure 1 or the spring balanced type with one such tube as shown in figure 2. The tube ends shall terminate in cast aluminum housings. The inner housing shall contain provisions for mounting the lamphead assembly. The outer housing shall contain provisions for mounting the lamphead and yoke assembly. The extension arm shall provide a minimum of 18 inches vertical travel, measured at the center of the lamphead. The upward and downward vertical movement of the extension arm, from the horizontal position, shall be equal in magnitude. The extension arm, in its horizontal position, shall locate the center of the lamphead a minimum of 30 inches from the center of the vertical standard. The extension arm shall be capable of being rotated about the vertical standard without stop limitations. Lamphead assemblies utilizing spring counterbalancing shall contain a means for adjustment using ordinary hardware tooling; the adjustment means shall be readily accessible for the medical technician.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

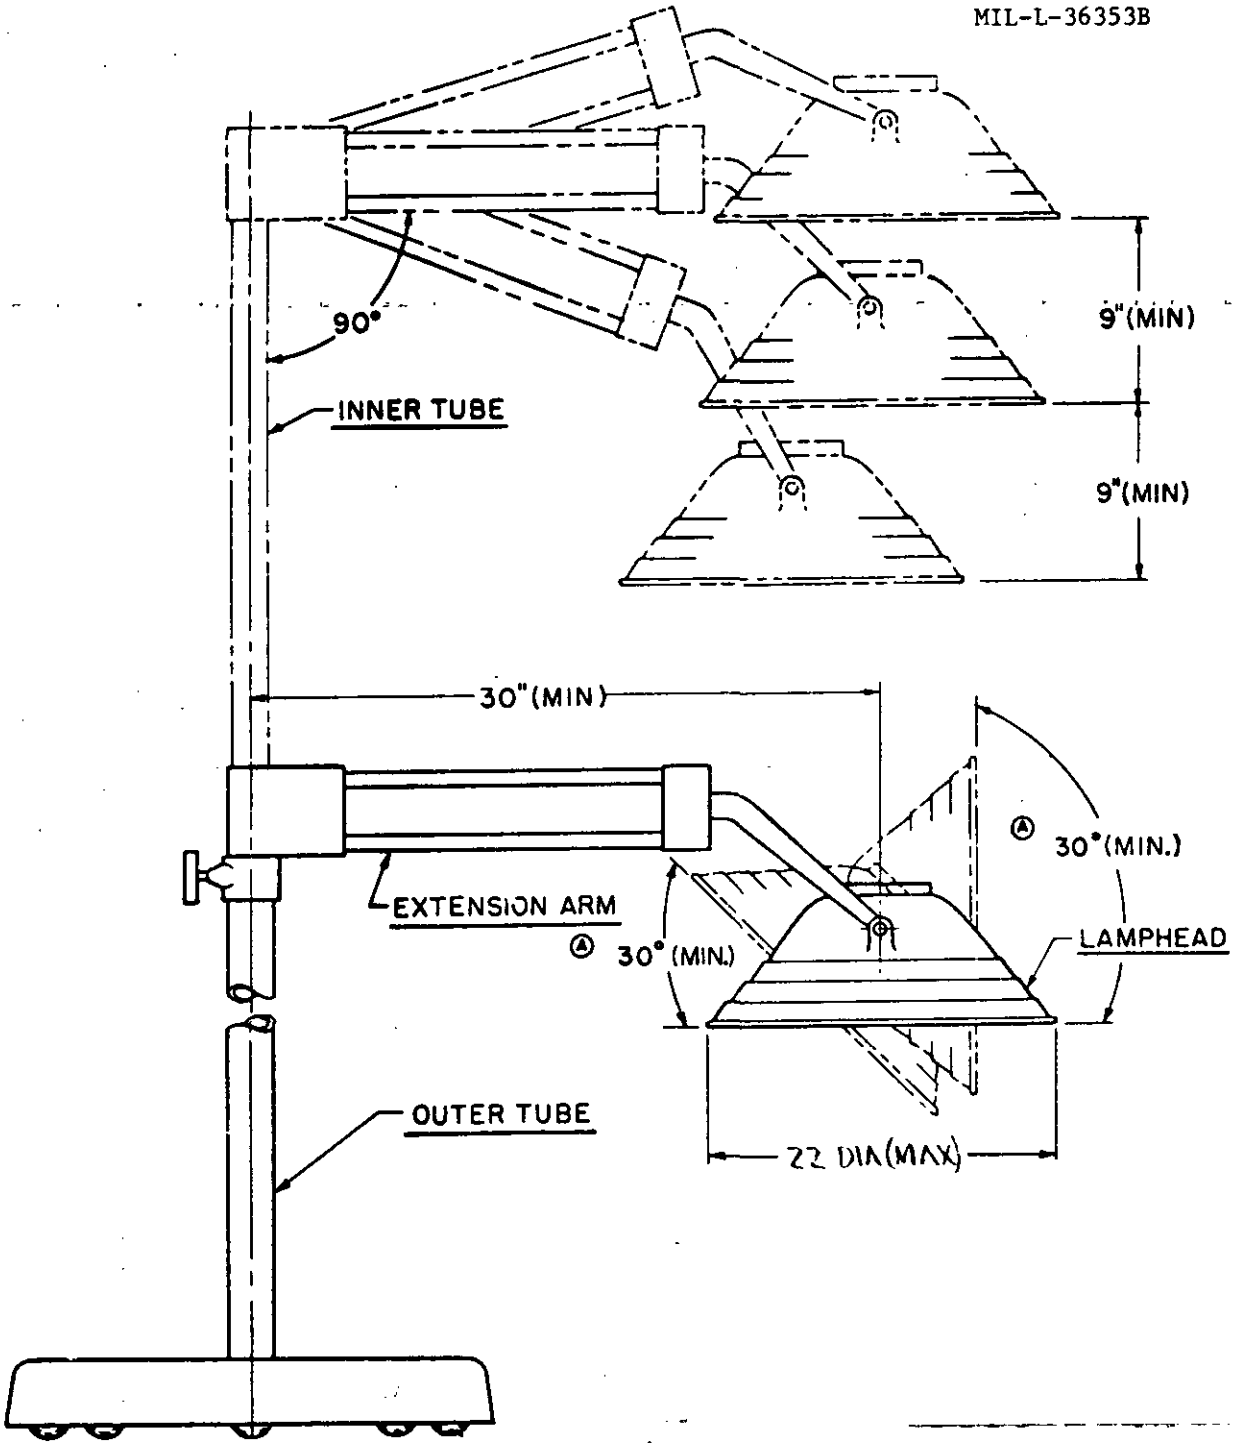


Figure 1. Surgical stand light construction.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

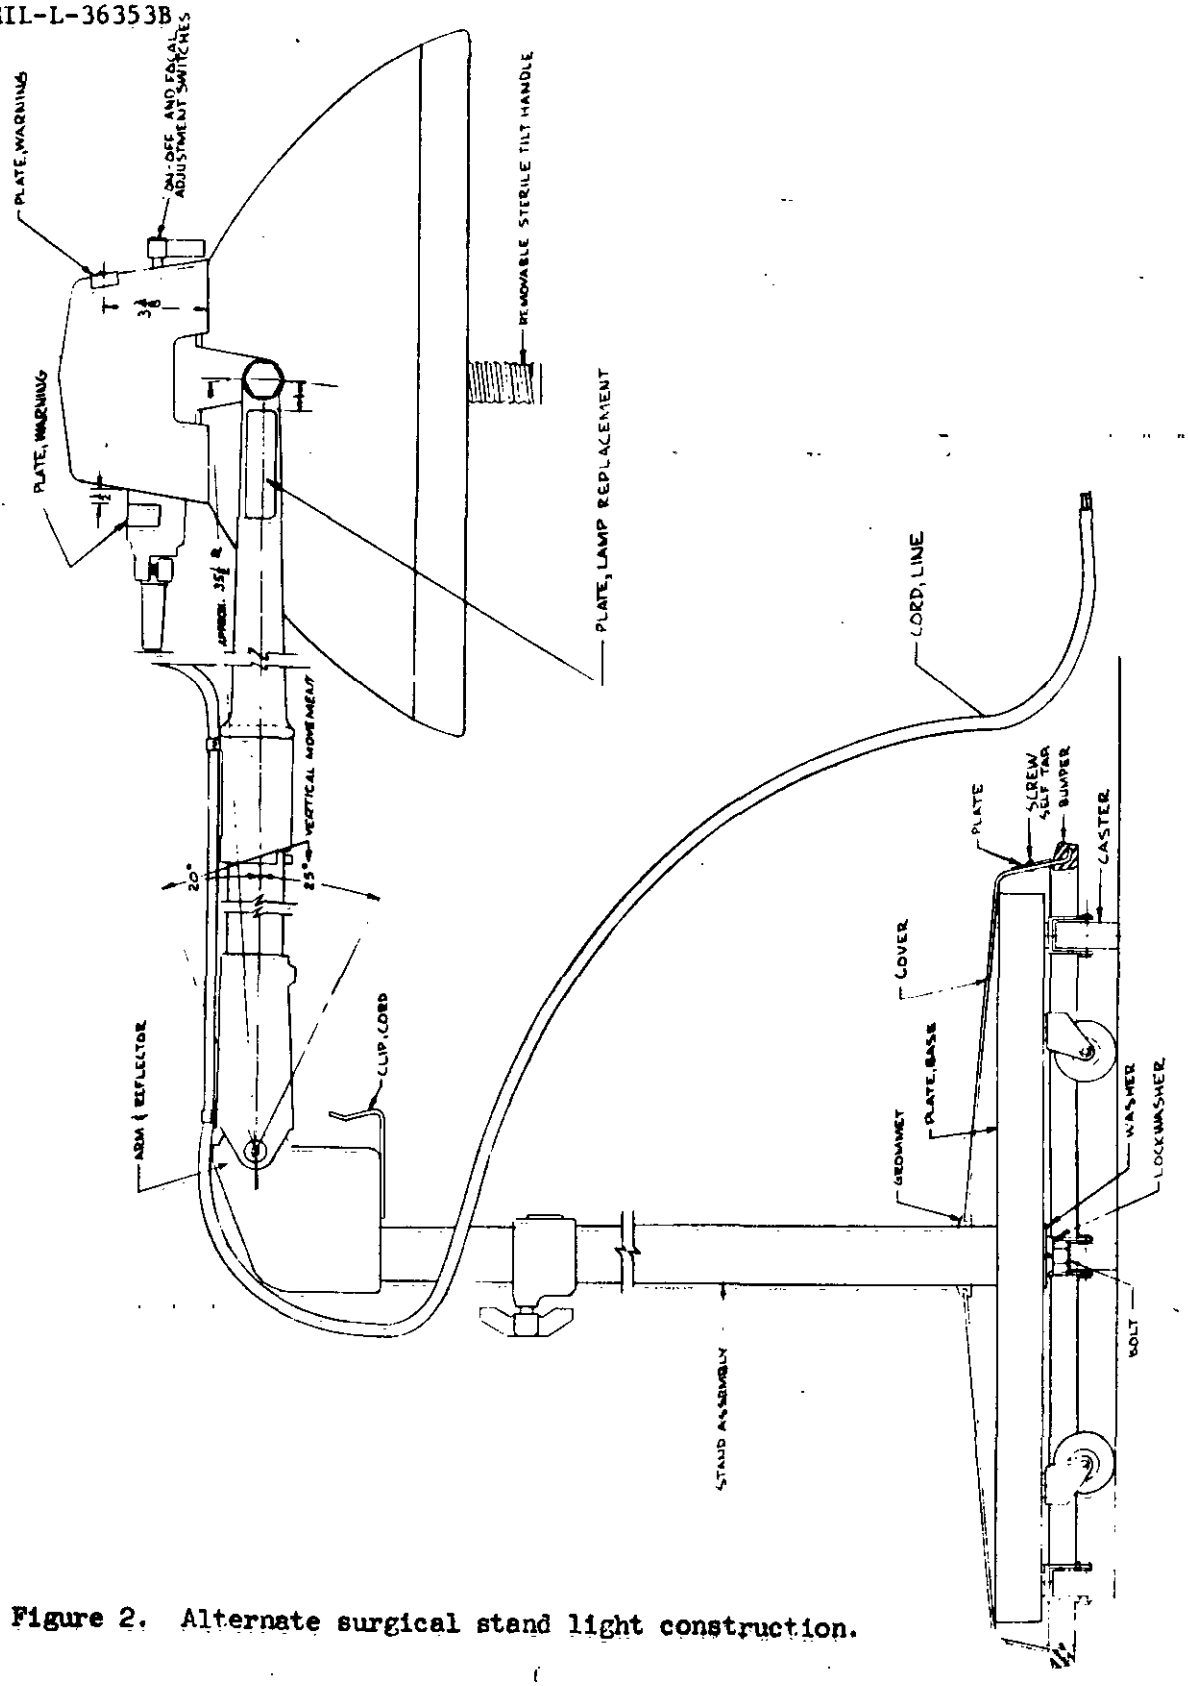


Figure 2. Alternate surgical stand light construction.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

3.4.5 Lamphead. The lamphead shall consist of an open-type focused reflector assembly, suitably secured to an explosion-proof incandescent bulb housing. The lamphead shall be easily and universally adjustable. Provision shall be made to facilitate raising, lowering, tilting, and swiveling the lamphead to angular positions desired, by means of a removable and sterilizable handle which can be quickly secured to the lamphead support. The lamphead shall be easily adjustable and capable of being angulated in its supporting yoke a minimum of 30° toward the vertical support column and 30° away from the vertical support column. The maximum angulation of the lamphead away from and toward the vertical support column shall not exceed that required for U.L. approval. Lamphead assembly shall be free of wobble and other unnecessary motions due to improperly machined parts and poor assembly techniques. Counter balancing assemblies shall provide for immediate 'dampening' (2 seconds or less) for the lamphead assembly to return to the designated position without any indication of 'drifting' (a position above or below the designated position).

* 3.4.5.1 Reflector. The reflector section of the lamphead shall be 17 to 22 inches in diameter. The reflector shall be of aluminum and of the open type. The reflecting surface shall have a reflectivity of 82 percent minimum as specified in 4.4.1.3. The reflective surface shall have a specular finish protected by a film of clear anodize of sufficient thickness to prevent clouding, staining, oxidizing or peeling during the life of the unit, and shall be tested as specified in 4.4.1.7.

* 3.5 Beam characteristics. The light output shall have shadow reducing qualities with a color temperature of 3750° K ± 500° K (Kelvin), when tested as specified in 4.4.1.2. The intensity of the light beam, when measured on a plane surface located 38 inches from and parallel to the plane formed by the rim of the reflector, shall be 2500 minimum footcandles at the center and may reduce uniformly to not less than 600 footcandles at the periphery of a 5-inch diameter field. The eccentricity between the mechanical center of the light and the center of the beam shall not exceed 2-1/2°. Light beam intensity and eccentricity shall be tested as specified in paragraph 4.4.1.8. A graphic representation of the test results shall be submitted to the contracting officer for approval, 60 days prior to shipment. The radiant energy, measured perpendicular to the light beam at a distance of 38 inches from the beaded edge of the reflector, shall not exceed 50,000 micro-watts per square centimeter when measured in accordance with the procedures specified in 4.4.1.6.

3.6 Explosion-proof housing. The explosion-proof housing shall comply with the Underwriters' Laboratories' requirements for class I, group C equipment, as specified in UL-781. The housing shall contain an inside frosted 120-volt, 150-watt, P25/10 or P25/8SB bulb, as recommended by the manufacturer. The housing or the yoke holding the lamphead shall be permanently marked with a legend indicating the proper replacement lamp. The lampholder shall meet the shell, medium base receptacle. The globe or cylinder shall be heat absorbing, color correcting glass, and shall provide beam characteristics as specified in 3.5. As an alternate to a single cylinder, two separate cylinders,

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

one for heat absorption and one for color correction shall be acceptable. Conductor leads passing into the lamphead shall be securely held and fitted with an electrical cord connector conforming to NFPA 56A. The lamp housing shall be designed to properly dissipate heat so that those areas which can be contacted by personnel during normal use shall not have a temperature rise greater than 12° C. (centigrade) above an ambient temperature of 25° C. An explosion proof switch, or a switch in an explosion-proof mounting, conforming to UL 781 shall be provided in the lamphead housing. Design and construction of the housing shall be in accordance with UL 781, with provisions for replacement of the lamp with ease and safety without the use of tools.

3.7 Spare lamp. A spare lamp, as described in paragraph 3.6 shall be furnished with each light.

3.8 Electric cord. Each light shall be furnished with not less than 20 feet of 3-conductor, flexible, type "STO" cord, with grounding conductor. One end of the cord shall terminate in the explosion-proof connector specified in 3.6. The free end shall be provided with a brightly colored warning tag to indicate attachment of an explosive proof plug by the using activity, of a type to match the hospital receptacle. The extension arm shall be provided with a suitable wire cable clip to support the cord.

3.9 Service data. The contractor shall furnish, with each unit, two copies each of a technical manual which contains complete instructions for installation, operation, and maintenance and lists of component parts. The manual shall comply with the requirements of MIL-M-7298. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer, via the cognizant Government inspector, two preliminary copies of his proposed technical manual for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract, or purchase order. In addition, the Contractor shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of the contract and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies may be waived upon request to the Contracting Officer. Waiver of submission of drafts and submission of 15 additional copies shall be at the option of the Government.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

3.10 Finish. The light base, yoke, swivel, and fork parts shall be finished in a baked-on enamel. The color of the enamel shall be either a hammer tone silver or a light green color 14241 of FED-STD-595. The vertical standard, extension arm, and trim shall be polished chromium over nickel plate. The outer surface of the reflector shall be polished aluminum or enameled light green.

3.11 Identification marking. Each light shall be marked with the manufacturer's name or registered trademark, serial number, electrical characteristics, and a statement that the light is suitable for use in class I, group C locations.

* 3.12 Workmanship. Workmanship shall be first class throughout. Lights shall be free from defects which detract from their appearance or may impair their serviceability. Sheet metal screws shall not be used. All surfaces through which electric wires pass shall be smooth and edges broken to prevent abraiding of the wire insulation.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

* 4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

4.1.2.1.1 First article inspection. First article inspection shall be performed on the light when a first article sample is required (see 3.1). This inspection shall include examination of 4.3 and tests of 4.4.1.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.3 and tests of 4.4.2.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the light may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and table I.

TABLE I. Sampling for examination

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Total defects (Major and Minor combined)	II	4.0
For dimensional examination	S-3	2.5

* 4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II.

TABLE II. Sampling for tests

	Inspection level	AQL (defects per hundred units)
Group I tests - First Article testing	One unit	1/
System test		
Color temperature		
Reflectivity measurements		
Stability test		
Electrical conductivity		
Beam radiant energy		
Sealing test		
Beam intensity		
Lamphead vibration test		

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

TABLE II. Sampling for tests (continued)

	Inspection level	AQL (defects per hundred units)
Group II tests - Acceptance testing		
Stability test	S-3	2.5
Electrical conductivity	100%	1/
System test	II	2.5
Sealing test	S-1	1/
Lamphead vibration test	S-3	1/

1/ Acceptance number is zero. Any test failure constitutes a rejection during these tests.

4.3 Examination. The lights shall be examined to determine compliance with all requirements contained in this specification.

* 4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table III. Examination shall not be restricted to the classified possible defects listed below.

TABLE III. Classification of defects

Categories	Defects
Major	
101	Lamphead not easily and smoothly adjustable throughout the entire range of required motion.
102	Vertical upright not easily adjustable throughout entire range.
103	Base does not move freely on casters or any caster binds.
104	Stop does not limit upper travel.
105	Lamp holder assembly cannot be removed easily.
106	Operating handle missing.
107	Any component not free of defects which impair use of product.
108	Casters do not rest firmly on flat surface.
109	Lamphead assembly not free of wobble.
Minor	
201	Warning tag not on cord or not as required.
202	Service data not as specified.
203	Nameplate incorrectly marked, missing, or illegible.
204	Electric cord less than 20 feet in length.
205	Wire clip to support cord not present or will not perform as required.
206	Any component not free of defect which impairs appearance of product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

4.3.2 Dimensional examination. The lights shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.3.3 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of section 5. Defects shall be scored as specified in table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

TABLE IV. Examination for preparation for delivery

Examination	Defect
Containers	Not as specified.
Quantity	Quantity in interior packages and shipping containers not as specified.
Packaging and Packing Materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

4.4 Tests. Tests shall be conducted, to determine compliance with specification requirements.

4.4.1 Group I tests.

4.4.1.1 System test. A system operation simulation test shall be performed to insure proper functioning of all applicable components.

4.4.1.2 Color temperature. Color temperature as specified herein establishes the isothermal relationship between the Planckian locus and a point, which is a plot of the x, y, coordinates of color, on the chromaticity diagram. Measurement shall be performed at room temperature by means of a suitable spectrophotometer of standard make and model (see 6.5).

4.4.1.3 Reflectivity measurements. Measurements shall be performed at room temperature by means of a suitable reflectometer of standard make and model (see 6.4). Certification by the company applying the finish to the reflector, shall be acceptable as evidence that the finished reflector meets the reflectivity requirements specified herein.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

4.4.1.4 Stability test. The inner tube of the vertical standard shall be completely extended and the lamphead adjusted to its greatest elevation by means of the extension arm. The lamphead shall be suspended in the direction of pull. A horizontal pull of 12 pounds shall be exerted 4 feet above the floor on the vertical standard by means of a spring scale, while the light base is blocked so that the light cannot move on the floor. The pull required to start tilting the light shall be the value recorded as a measure of stability.

4.4.1.5 Electrical conductivity. The light, while mounted on the casters, shall be tested for electrical conductivity using the equipment described in NFPA 56A.

4.4.1.6 Beam radiant energy. The beam radiant energy shall be measured by means of a calibrated thermopile. The thermopile shall be calibrated against a standard light source which has been certified by the National Bureau of Standards. The beam radiant energy in the opening field shall be measured at the point of maximum light intensity.

4.4.1.7 Sealing test. Apply one drop of a water solution of anthraquinone violet R (1 gm. per 50 cc) to the specular surface of the reflector, at room temperature. Allow to stand for 5 minutes then wash with running water. Saturate a soft cloth with a solution of mild soap and water and abrade the area treated. There shall be no evidence of stain or discoloration.

* 4.4.1.8 Beam intensity. The average foot-candle distribution curve shall be contained by plotting foot-candle values as the ordinate against inches from nadir zero as the abscissa. The test procedure shall be as follows: Mount the light to be tested in a suitable test fixture capable of 360° rotation about the nadir axis and calibrated in increments of 10°. Mechanically center the illumination meter on nadir zero. Energize the light to be tested with rated voltage and rotate the test fixture through 360° recording foot-candle values for each 10° increment. Reposition the illumination meter in 1/2 inch increments in a straight line (left and right) through nadir zero to the periphery of the light beam. For each position of the meter, 36 measurements at 10° increments shall be recorded. The value in foot-candles to be plotted shall be the difference between the average value (average of 36 readings for each position of the meter) and the ambient intensity level. The resulting curve and eccentricity value shall conform to the requirements of 3.5. The eccentricity of the light beam shall be the distance along the abscissa between nadir zero and the point of maximum illumination and shall not exceed 1-1/2 inches. Intensity measurements shall be performed at room temperature by means of a suitable photometric or reflectometer of standard make and model (see 6.4).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

* 4.4.1.9 Lamphead vibration test. The light shall be set up such that the height of the upper pivot point of the pantograph arm above the floor with the telescoping rod fully extended shall be approximately 85 inches. Extension arm shall be positioned normal to the telescopic section of the upright. Lamphead shall be placed face down and positioned in a plane which is parallel to the room floor. The lamphead handle shall be grasped and the lamphead raised at least 4 inches in vertical height and returned to its original position and released. Using a stopwatch, the time shall be recorded in seconds from the release of the lamphead assembly after its return to the original position to the final oscillation in this position. The same procedure in its entirety shall be followed when the lamphead is lowered at least four inches in vertical height from the original position.

* 4.4.2 Group II tests.

4.4.2.1 Stability test. The inner tube of the vertical standard shall be completely extended and the lamphead adjusted to its greatest elevation by means of the extension arm. The lamphead shall be suspended in the direction of pull. A horizontal pull of 12 pounds shall be exerted 4 feet above the floor on the vertical standard by means of a spring scale, while the light base is blocked so that the light cannot move on the floor. The pull required to start tilting the light shall be the value recorded as a measure of stability.

4.4.2.2 System test. A system operation simulation test shall be performed to insure proper functioning of all applicable components.

4.4.2.3 Electrical conductivity. The light, while mounted on the casters, shall be tested for electrical conductivity using the equipment described in NFPA 56A.

4.4.2.4 Sealing test. Apply one drop of a water solution of anthraquinone violet R (1 gm. per 50 cc) to the specular surface of the reflector, at room temperature. Allow to stand for 5 minutes then wash with running water. Saturate a soft cloth with a solution of mild soap and water and abrade the area treated. There shall be no evidence of stain or discoloration.

4.4.2.5 Lamphead vibration test. Same test as 4.4.1.9.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

* 5.1.1.1 Unit preparation. Each surgical light shall be disassembled as far as is practicable including removing the bulb from the lamphead. The lamphead assembly, bulb and spare bulb shall be individually packaged in a fiberboard box constructed in accordance with PPP-B-636, class domestic. The boxes shall be designated with suitable interior fittings or shall contain sufficient cushioning material to insure against damage to the contents. All other components shall be wrapped in kraft paper and the wrapping secured with tape. The manufacturer shall place a warning tag on the locking mechanism stating the following: "Do not loosen the locking knob until the lamphead assembly is placed on the telescoping member."

5.1.2 Level C. Each surgical light shall be packaged in standard commercial containers of the size and kind commonly used which will afford the degree of protection required for shipment and use of the item for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Each surgical light, prepared as specified in 5.1.1.1, shall be packed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-601, overseas type or PPP-B-621, class 2. The components comprising the surgical light shall be blocked, braced and cushioned within the exterior container in such a manner to prevent shifting, damage or marring of surfaces. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each exterior container shall be lined with a case liner conforming to MIL-L-10547. Closure and sealing shall conform to the applicable paragraphs of the appendix thereto.

5.2.2 Level B. Each surgical light shall be packed as specified in 5.2.1 except the exterior containers shall conform to PPP-B-601, domestic type or PPP-B-621, class 1. Case liner and strapping shall not be required.

5.2.3 Level C. Each light shall be packed in a substantial commercial container of the type, size, and kind commonly used for the purpose and so constructed as to insure acceptance and safe delivery by common or other carriers at the lowest rate to point of delivery called for in the contract or order.

5.3 Marking.

5.3.1 Interior packages. Interior packages shall be marked to identify contents and quantity contained.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

5.3.2 Exterior container. Exterior containers shall be marked in accordance with MIL-STD-129. Fragile markings as specified in MIL-STD-129 shall also be shown.

6. NOTES

6.1 Intended use. Shall be suitable for use in military hospital operating rooms.

6.2 Ordering data. Procurement documents should specify the following:

a. Title, number and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
c. When a first article is required (see 3.1, 4.1.2.1, and 6.3).

6.3 First article. When a first article is required, it shall be tested and approved under the appropriate provisions of 7-104.55 of the Armed Services Procurement Regulation. The contract or purchase order specifies the quantity, procedure for delivery and other specific instructions for inspection and approval of the first article.

6.4 Acceptable instruments for the measurement of intensity reflectivity are the Baumgartner reflectometer, Taylor brightness meter, Macbeth illuminator, Weston Illumination meter, and International Light Co., Color Radiometer IL 600.

6.5 An acceptable instrument for the measurement of color temperature is the Spectra-3 color meter manufactured by Photo Research Corp., Hollywood, California and International Light Co. Color Radiometer IL 155.

6.6 Instruments other than those specified above may be considered acceptable provided they are approved by the contracting officer prior to delivery.

6.7 This specification covers the following item appearing in the Federal Supply Catalog:

NSN	Item Identification
6530-00-299-8298	Light, Surgical, Stand, Mobile, Explosion-Proof, 115 Volt, AC-DC

6.8 The margins of this specification are marked with an sterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6530-1369

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-L-36353B - LIGHT, SURGICAL, STAND

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

☆ U.S. GOVERNMENT PRINTING OFFICE: 1976— 603-766/3433

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:27Z
Check the source to verify that this is the current version before use.