MIL-N-36333A
4 December 1969
SUPERSEDING
MIL-N-36333(DM)
18 November 1964

MILITARY SPECIFICATION

NOZZLE, RECTAL IRRIGATING

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers one type of adult size, rectal irrigating nozzle, suitable for use as a disposable, enema tip.

2 APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

MMM-A-250	Adhesive, Water Resistant (For Sealing Waterproof Paper)
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper, (For Carton Sealing).

STANDARDS

Federal

Fed. Std. 406 Plastic, Methods of Testing

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

* 3.1 Material. The irrigating nozzle shall be made of rigid, polyethylene plastic throughout. The polyethylene plastic shall have the following physical properties and shall be tested as specified in 4.4.1.


Tensile strength, pounds per square inch (min.)	1700
Modulus of elasticity, pounds per square inch (min.)	30000
Elongation, percent (min.)	125
Coefficient of linear thermal expansion, inch per inch per degree Fahrenheit	.00017 ± 10%
Hardness Rockwell M scale	43 ± 5
Specific gravity	.925 ± 5%

3.2 Design and construction. Shall be as shown in Figure I, and as follows: Shall be a rectal type irrigating nozzle. Shall have corrugations on one end so that a tight fit is obtained when the nozzle is inserted into the rubber tubing used with irrigators. The other end shall be bulbous in shape with two holes in the center, 180 degrees apart; or there shall be two pairs of holes, each pair straddling the center of the bulbous area, with 180 degrees between the pairs. Holes shall have clean bores. Measurements shall be as shown on the drawing.


3.3 Identification marking. The nozzles shall be legibly and permanently marked with the manufacturer's name or registered trademark.

3.4 Workmanship. Workmanship shall be first class throughout. The nozzle shall be free from defects which detract from its appearance or may impair its serviceability.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:25Z
Check the source to verify that this is the current version before use.

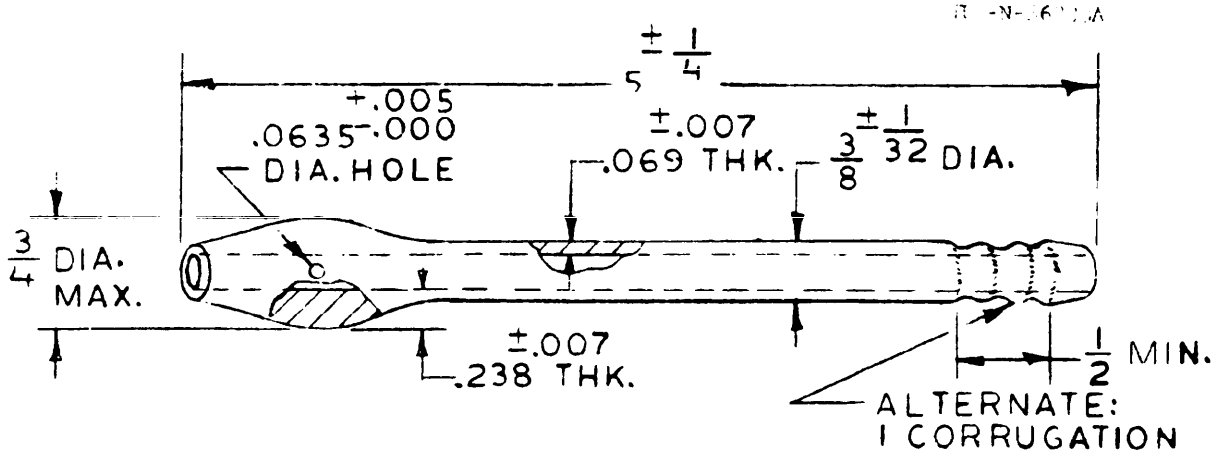

NOZZLE, RECTAL IRRIGATING

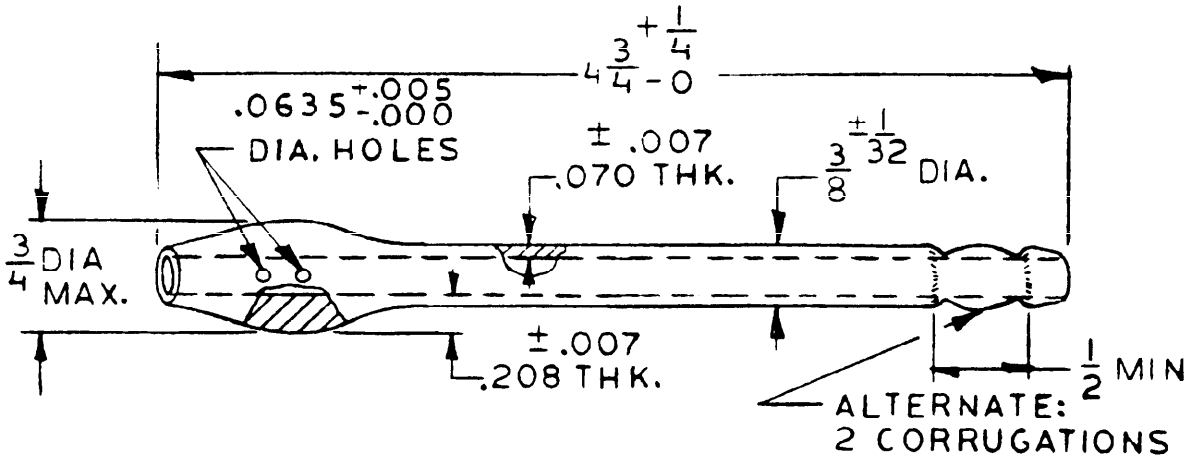

ALTERNATE NOZZLE

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:25Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, or auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105.

	Inspection level	AQL (percent defective)
For visual examination		
Major defects	II	1.0
Minor defects	II	4.0
For dimensional examination	S3	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105.

4.3 Examination. The nozzles shall be examined to determine compliance with all requirements contained in this specification.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:25Z
Check the source to verify that this is the currentversion before use.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects as shown in Table I.

TABLE I

Category	Defects*
Major	
101.	Diameter and length of nozzle not within specified tolerances.
102.	Cross section at diameter of bulbous end not within specified tolerance.
103.	Two holes required in bulbous area missing or not properly located 180 apart.
104.	Nozzle not free of burs and sharp edges.
105.	Openings of nozzle not free of obstructions.
Minor	
201.	Internal portion of nozzle not free of dirt or other foreign particles.
202.	Identification marking not legible.
203.	End of nozzle opposite the bulbous end not corrugated as specified.

*Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The nozzles shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Physical properties. Physical properties shall be determined in accordance with the appropriate test method of Fed. Test Method Std. No. 406, as follows:

TABLE II

Property	Test Method
Tensile strength	1011
Modulus of elasticity	1011
Elongation	1011
Coefficient of linear thermal expansion	2031
Hardness	1081
Specific gravity	5012

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One package (12 nozzles), as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in the following table shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table III. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	60 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each nozzle shall be individually packaged in a bag fabricated of polyethylene. Closure shall be effected by heat sealing. Each unit (12 nozzles) shall be packaged in a carton of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676. Closure shall be adequate to prevent accidental opening.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2 inch wide tape conforming to PPP-T-76. Closing of bottom flap with adhesive conforming to MMM-A-250 or metal stitches is permitted.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:25Z
Check the source to verify that this is the currentversion before use.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type, PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Intended use. Military hospitals and medical facilities.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packing (see 5.1 and 5.2).

6.3 This specification covers the following item appearing in the Federal Supply Catalog.

Item	FSN
Nozzle, Rectal Irrigating	6530-680-0124

6.4 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

6.5 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 20261021T08:25Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel of Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION

MIL-N-36333A FSN

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD, FORM 1 JAN 68 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE [illegible]
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:25Z
Check the source to verify that this is the current version before use.