MILITARY SPECIFICATION

SUCTION APPARATUS, SURGICAL, AUTOMATIC, THERMOTIC, PORTABLE, 110 VOLT, AC-DC.

1. SCOPE

1.1 This specification covers one type of automatic surgical suction apparatus, suitable for gastrointestinal decompression or suprapubic drainage.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposal form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-636	Box, Fiberboard.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Material. All material and parts used in the fabrication of surgical suction apparatus shall be as indicated in table I.

TABLE I. SURGICAL SUCTION APPARATUS

PARTS LIST

PART NO.	NOMENCLATURE
1	Tube and bracket assembly.
2	Rubber tubes, 3/16 inch inside diameter by 3/32 inch wall by 10 inches, 4 and 5 feet long.
3	Angular metal tubes, set of 2.
4	Stopper clamp, 1/8 inch diameter wire, overall dimensions 3 inches long by 3 inches wide.
5	Rubber stopper for gallon bottle, two hole, size 12.
6	Bottle sealing hood, rubber, two hole.
7	Trap bottle, wide mouth, round, 3 ounces, 2-1/4 inches outside diameter.
8	One gallon vacuum bottle, wide mouth, round, 6-1/2 inches outside diameter.
9	Heating element, complete.
10	Heating chamber shell cover.
11	Suction valve pipe.
12	0.25 microfarad capacitor with 0.75 ohm. resistance wire.
13	Suction inlet valve.
14	Pressure outlet valve.
15	Pilot lamp socket.
16	Pilot lamp, 115 volt, 6 watt, bulb S-6, clear, 1-7/8 inches long overall.
17	Pilot lamp red jewel, 3/8 inch long, 11/16 inch - 27 externally threaded.
18	Thermostat switch, single pole, single throw, normally closed contacts.
19	Thermostat heater arm:
20	16 ohm. ± 10%, 20 watt resistor, vitreous enameled.
21	High-low off switch single pole, single throw, 125 volt, 3 amperes, 15/32 in diameter bushing.
22	Heating chamber shell.
23	Brass hexagon nut.
24	Heating unit terminal plate.
25	Wiring plate cover.
26	Heating unit terminal plate basket.
27	Suction valve nut.
28	Suction valve hose connection.
29	Mounting post for wiring plate cover.
30	Thermostat frame.
-	Thermostat; complete.
31	Hook.
-	Rubber cord with plug, 6 feet minimum length.
-	1/4 inch fiber washers.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.

3.2 Design. The suction apparatus shall be designed to provide mild suction for cavity drainage where precision control is essential for the protection of delicate tissues. The apparatus shall operate on a potential of 110 to 120 volts.

3.3 Construction. The automatic surgical suction apparatus shall be as shown in figure 1.

3.4 Performance. When tested as specified in 4.4.1, the apparatus shall produce intermittent suction for indefinite periods of time at either 70 millimeter (mm.) or 100 mm of mercury. Selection of the vacuum shall be made by means of a switch.

3.5 Dielectric strength. There shall be no electrical breakdown when tested as specified in 4.4.2.

3.6 Accessories. Each unit shall be furnished with the following accessories:

One (1) inlet valve
One (1) outlet valve
Two (2) gaskets

3.7 Finish. Finish shall be in accordance with the manufacturer's standard commercial practice.

3.8 Identification marking. Each suction apparatus shall have a metal nameplate permanently attached bearing the following information:

Federal stock number.
Name or registered trademark of the manufacturer.
Contract or purchase order number.
Electrical ratings; i.e., voltage, amperage, wattage, frequency, etc.
Letters U.S.

The markings on the plate shall be clear, legible and permanent, and shall be accomplished by die stamping into the surface of the metal. Nameplates secured by adhesives shall not be used.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.

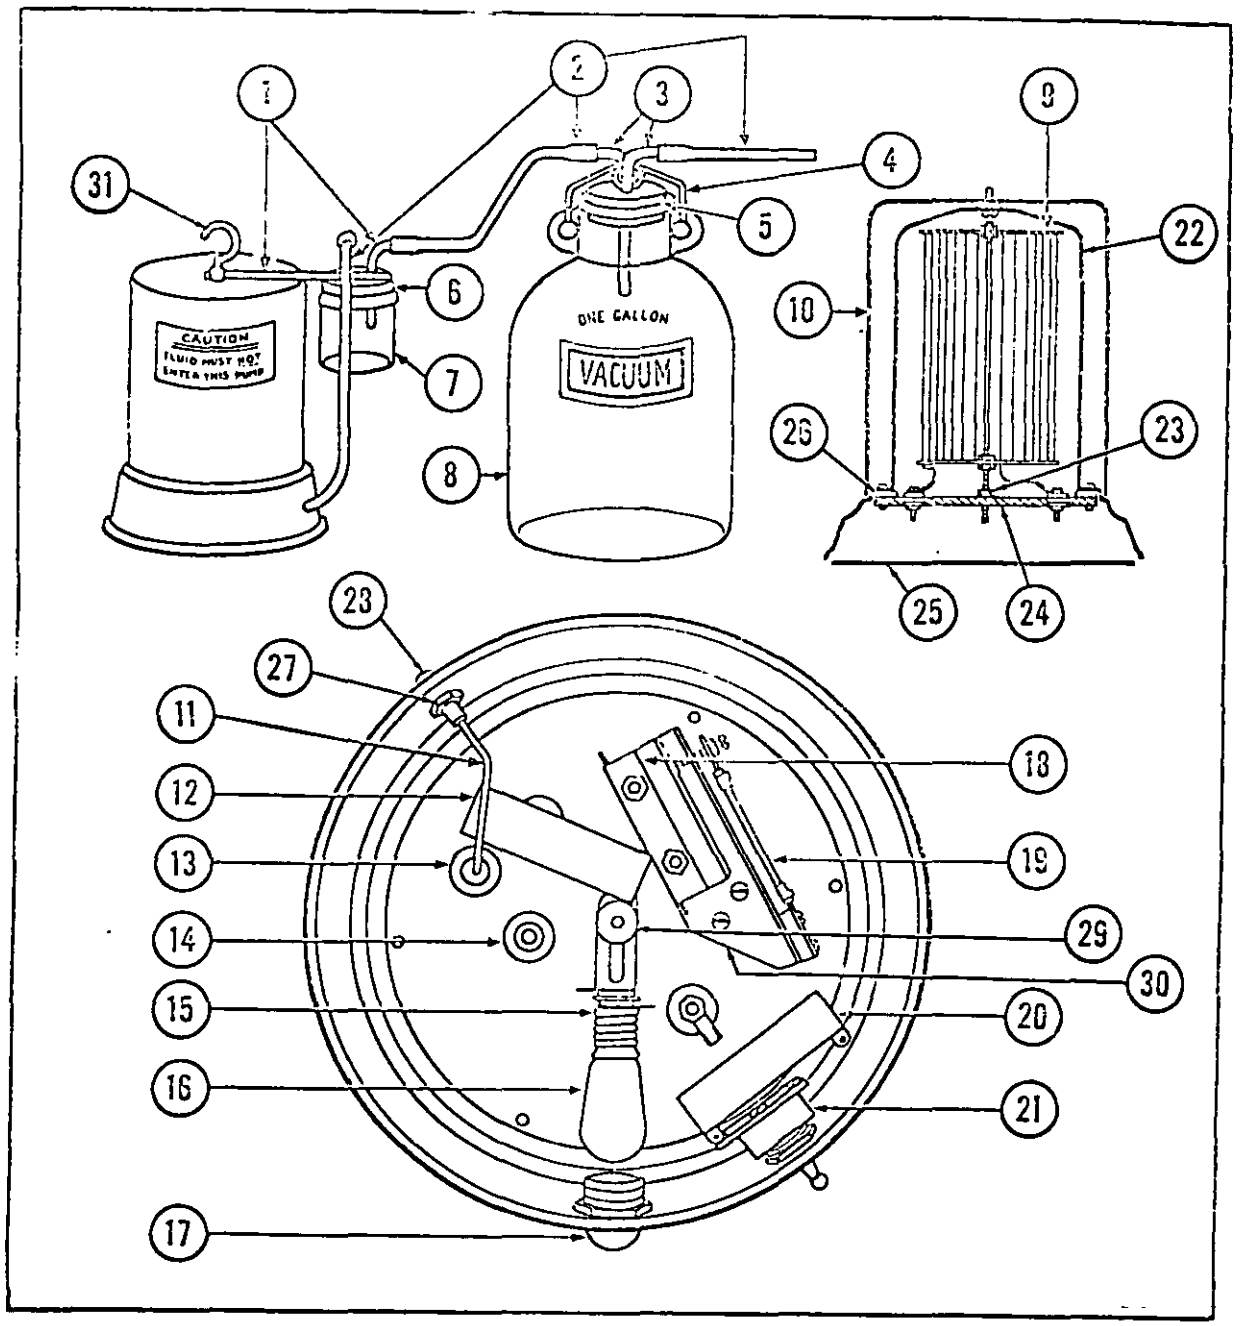


FIGURE 1

SUCTION APPARATUS, SURGICAL, Automatic, Thermotic, Portable, 110 volt, AC-DC

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.

3.9 Service data. The contractor shall furnish, with each unit, two copies of service data containing complete instructions for installation, operation, maintenance, and a list of component parts. The service data shall include such detailed information which shall permit ready installation and maintenance of the item. All information contained in the manual shall be suitably indexed to permit ready reference to the required information. Wiring diagrams shall be included for electrical items or components. Wiring diagrams, drawings, and descriptive material shall include adequate information so that the replacement parts can be ordered by the manufacturer's part number, and without confusion as to the item identification. Identical or interchangeable replacement parts shall be identified by a single part number only. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the contracting officer, via the cognizant Government inspector, two preliminary copies of his proposed service data, for review and comment by the Defense Medical Supply Center. The preliminary service data shall be submitted sufficiently early to permit adequate review by the Defense Medical Supply Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of required revisions and corrections in the final service data without delaying delivery under the contract or purchase order. The contractor shall mail 15 copies of the approved service data to the contracting officer for distribution.

3.10 Workmanship. Workmanship shall be first class throughout. The suction apparatus shall be free from defects which detract from its appearance or may impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105.

	Inspection level	AQL (percent defective)
For visual examination		
Major defects	II	1.0
Total (major and minor combined) defects	II	4.0

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105.

Characteristic	Requirement	Test procedure	Inspection level
Performance	3.4	4.4.1	S-4
Dielectric strength	3.5	4.4.2	100%

The acceptance number for each test shall be zero for all lots regardless of sample size.

4.3 Examination. The suction apparatus shall be examined to determine compliance with all requirements contained in this specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Categories and defects*	
Major	
101	Heating element wire disconnected.
102	Pilot lamp disconnected or burned-out.
103	Any part missing, broken, or otherwise unusable.
104	Nameplate missing, incomplete, or illegible.
105	Service data missing or does not include all specified information.
106	Exposed edges not free of burrs and sharpness.
Minor	
201	Instruction plate not permanently secured to suction apparatus.
202	Pump cover soiled, scratched or otherwise improperly finished.
203	Finish scratched, marred, or otherwise defective.

* Examination shall not be restricted to the classified possible defects listed above.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Performance. The surgical suction apparatus shall be set up and operated in accordance with the manufacturer's instructions. The suction shall be measured using a mercury manometer to determine compliance with 3.4.

4.4.2 Dielectric strength. The assembled surgical suction apparatus shall be subjected to a gradually increasing potential of twice the rated voltage plus 1000 volts, or 1230 volts, applied between the current-carrying parts and the metal enclosure and maintained at this value for a period of one minute.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One (1) suction apparatus, as specified, constitutes one unit.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Each unit shall be packed in a box constructed in accordance with PPP-B-636, type CF, class weather-resistant, V3c, style FOL-L. Carton shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure shifting of, or damage to contents. Closure shall be in accordance with appendix to box specification. In addition, waterproofing shall be in accordance with 30.4.2 of appendix.

5.2.1.2 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.3 Marking.

5.3.1 Exterior container. Marking shall be in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commerically available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency. - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft cirulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

FORM APPROVED BUDGET BUREAU NO. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use of the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity.

SPECIFICATION SUCTION APPARATUS, SURGICAL, AUTOMATIC, THERMOTIC, PORTABLE, 110 VOLT, AC-DC. MILITARY SPECIFICATION MIL-S-76299(DA), dated 12 October 1964

ORGANIZATION

CITY AND STATE

CONTRACT NO.

QUANTITY OF ITEMS PROCURED

DOLLAR AMOUNT
$

MATERIAL PROCURED UNDER A ☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?
   ☐ YES ☐ NO IF "YES" IN WHAT WAY?

4. REMARKS (ATTACH ANY PERTINENT DATA WHICH MAY BE OF USE IN IMPROVING THIS SPECIFICATION. IF THERE ARE ADDITIONAL PAPERS, ATTACH TO FORM AND PLACE BOTH IN AN ENVELOPE ADDRESSED TO PREPARING ACTIVITY)

SUBMITTED BY (PRINTED OR TYPED NAME AND ACTIVITY)

DATE

DD FORM 1426

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:22Z
Check the source to verify that this is the current version before use.