MILITARY SPECIFICATION

DILATOR SET, UTERINE

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a set of six (assorted sizes) double ended uterine dilators, of the Hank design, with stops for governing the depth of penetration.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
CCC-C-419	Cloth, Cotton, Duck, Unbleached, Plied-Yarns, (Army and Numbered).
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case, and Sheet Overwrap, Water-Vaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-STD-123	Marking for Domestic Shipment (Civilian Agencies).

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General Requirements. The uterine dilator set shall be in accordance with the applicable requirements of GG-I-526, and the following option exercises under that specification.

3.2 Material. The uterine dilators shall be fabricated from Class 3, Type 303 or 304 material.

3.3 Hardness. After proper stress relieving, the Rockwell hardness of the uterine dilator set shall be B75 to B85.

3.4 Style, design, and dimensions. The style, design, and dimensions of the uterine dilator set shall be in accordance with Figure 1. The dilator set shall be supplied in a case as specified in 3.4.1.

3.4.1 Case. The case shall be fabricated from type III, 9.85 ounce Army duck in accordance with Federal Specification CCC-C-419. The case shall be provided with retaining loops of webbing for insertion of the dilators, and shall be of suitable size to adequately accommodate the set of six dilators. The case shall be of the roll-up type, and shall be provided with two inside flaps that completely cover and protect the dilators. Two tapes shall be firmly attached to one end of the case to keep it from unrolling by tying the free ends of tapes. The raw edges of the case shall be bound with tape. The raw ends of the tapes shall be dipped in vinyl or turned under and sewn to prevent their unraveling. The case and its component parts shall be vat dyed olive drab No. 7.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

3.6 Identification Marking. In addition to GG-I-526 requirements, uterine dilator sets of foreign manufacture shall also be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Shall be in accordance with GG-I-526.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in Table I. The unit of product for examination purposes shall be one uterine dilator set.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Table II. Sampling for Tests

Component (unit of product)	Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
1-Uterine Dilator (end item)	Composition analysis	3.2 and GG-I-526	GG-I-526	**	*
	Hardness	3.3 and GG-I-526	GG-I-526	S-2	*
	Dimensions	3.4	--------	S-1	*
	Boil test	GG-I-526	GG-I-526	S-2	*

* Acceptance number shall be zero for all sample sizes.
** Sufficient amount from each lot of each metal used in the construction of the uterine dilator set shall be selected for composition analysis.

4.3 Examination. The uterine dilator set shall be examined to determine compliance with specification requirements. Examination shall be conducted in accordance with MIL-STD-105 and the following classification of defects. Examination shall include, but shall not be limited to the defects listed in Table III.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Instrument not constructed as specified.
103	Instrument not free from sharp edges, rough areas, burrs, cracks, grind marks, or overlaps.
104	Case not as specified.
Minor	
201	Finish not as specified.
202	Identification marking not present, correct, complete, or legible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements in accordance with GG-I-526.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One dilator set, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	48 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method Ic-2.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with Fed. Std. 123.

5.3.2 Military activities.

5.3.2.1 Interior packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The double ended uterine dilators, of the Hank design, with stops for governing the depth of penetration shall be suitable for conservative dilation of the cervix, preparatory to diagnostic or therapeutic procedures.

6.2 Ordering data. The procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(c) Federal stock number.

6.3 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

FSN	Item Identification
6515-325-5500	DILATOR SET, UTERINE, Solid, Double-Ended, Hank, Set of 6

It does not include all types or sizes which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 8, dated 27 December 1966.

Custodians:
Army - MD
Navy - MS
Air Force - 03


Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1612

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

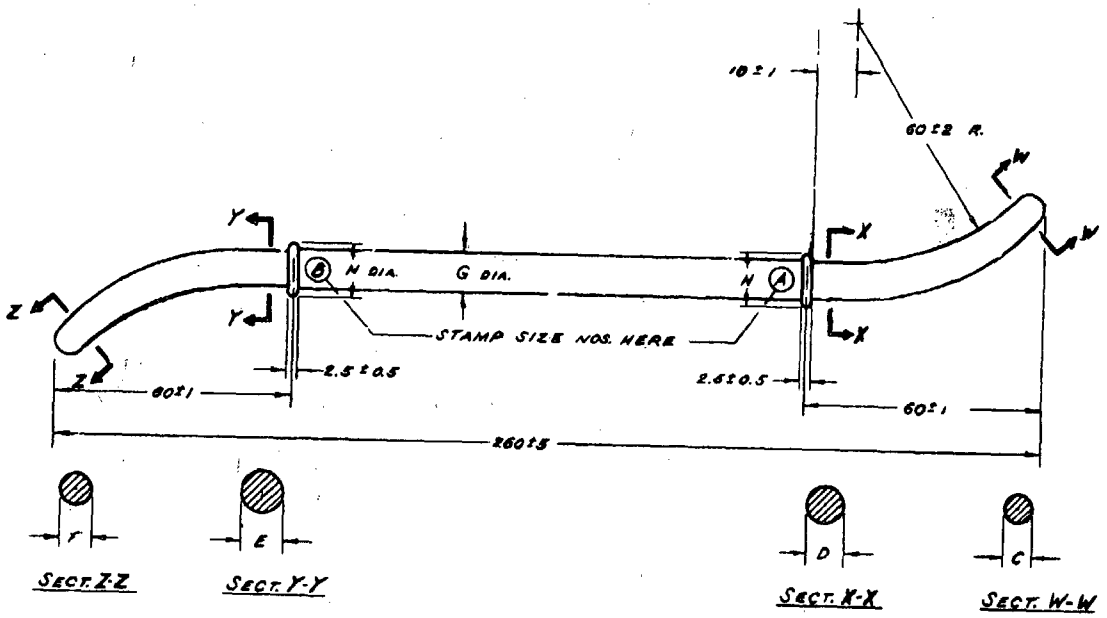

SIZE		SIZE No.	C	D	E	F	G	H
9 & 10	A	9	3.4 ± 0.1	4.5 ± 0.1			5.0 ± 0.1	8.5 ± 0.5
	B	10			5.0 ± 0.1	3.8 ± 0.1		
11 & 12	A	11	4.2 ± 0.1	5.5 ± 0.1			6.0 ± 0.1	9.5 ± 0.5
	B	12			6.0 ± 0.1	4.6 ± 0.1		
13 & 14	A	13	5.0 ± 0.1	6.8 ± 0.1			7.0 ± 0.1	10.5 ± 0.5
	B	14			7.0 ± 0.1	5.6 ± 0.1		
15 & 16	A	15	5.8 ± 0.1	7.5 ± 0.1			8.0 ± 0.1	11.5 ± 0.5
	B	16			8.0 ± 0.1	6.2 ± 0.1		
17 & 18	A	17	6.6 ± 0.1	8.5 ± 0.1			9.0 ± 0.1	12.5 ± 0.5
	B	18			9.0 ± 0.1	7.0 ± 0.1		
19 & 20	A	19	7.4 ± 0.1	9.5 ± 0.1			10.0 ± 0.1	13.5 ± 0.5
	B	20			10.0 ± 0.1	7.8 ± 0.1		

NOTE: (A)

ALL JOINTS TO BE SILVER SOLDERED
ALL DIMENSIONS IN MILLIMETERS

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION
MIL-D-36798

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO (If "yes", in what way?)

4. REMARKS (Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)

SUBMITTED BY (Printed or typed name and activity - Optional)

DATE

DD FORM 1 JAN 66 1426

REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

Source: https://assist.dla.mil ---Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.