MILITARY SPECIFICATION

SCISSORS, NASAL, ANGULAR, KNIGHT, 6-1/4 inch

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a nasal scissors, of the Knight design, having angular blades with points semi sharp.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Specifications, Dental and Surgical, General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Set-Up.

Military

MIL-P-116	Preservations, Methods of.
MIL-L-10547	Liners, Case and Sheet Overwrap; Water-Vaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:21Z
Check the source to verify that this is the currentversion before use.

STANDARDS

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General requirements. The nasal scissors shall be in accordance with the applicable requirements of GG-I-526 and the following option exercises under that specification.

3.2 Material. The nasal scissors shall be fabricated from Class 4, Type 420 material, except that the carbon content shall be a minimum of 0.30 percent.

3.3 Hardness. After proper stress relieving, the nasal scissors shall have a Rockwell hardness of C50 to C55 (with the exception of the screw).

3.4 Style, design and dimensions. Shall be a nasal scissors, of the Knight design, having angular blades with points semi sharp suitable for use in surgical operations on the nose. Shall be in accordance with Figure 1.


3.5 Finish. Finish shall be mirror, except blades shall be crocus.

3.5.1 Passivation. The entire item shall be properly passivated.

3.6 Cutting edges. Scissors shall cut a continuous length of at least 7/8 inch of the test material, when tested as specified in 4.4.1. This cutting requirement shall apply for the entire length of the cut specified, including the tips of the scissors. All three cuts made with each scissors tested shall meet the requirements of this specification.

3.7 Identification marking. In addition to GG-I-526 requirements, instruments of foreign manufacture shall also be marked "stainless".

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:21Z
Check the source to verify that this is the current version before use.

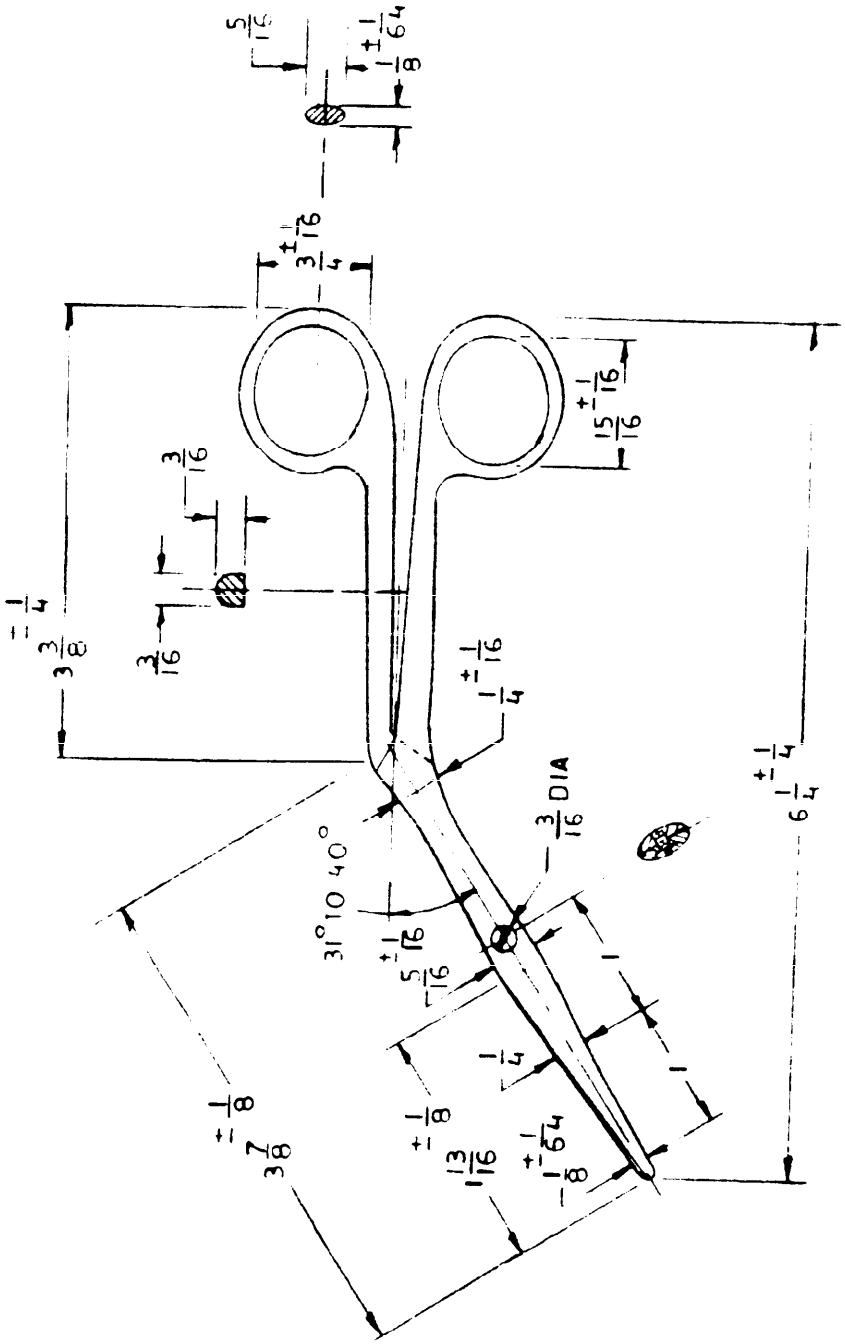

NOTE:
UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES AND
TOLERANCES ARE AS FOLLOWS:
FRACTIONS ±1/32

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Shall be in accordance with GG-I-526.

4.1.2 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the corrosion-resistant steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in Table I. The unit of product for examination purposes shall be one nasal scissors.

Table I. Sampling Criteria for Examination

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. Unit of product for test purposes shall be one nasal scissors.

Table II. Sampling Criteria for Tests

Component	Characteristic	Requirement	Test procedure	Inspection level	AQL
Nasal scissors	Composition analysis	3.2 and GG-I-526	GG-I-526	*	-
	Hardness	3.3 and GG-I-526	GG-I-526	S-2	1.0
	Dimensions	3.4	--------	S-2	1.5
	Copper sulfate test	GG-I-526	GG-I-526	S-2	1.0
	Boil test	GG-I-526	GG-I-526	S-2	1.0
	Scissors performance test	3.6 and GG-I-526	4.4.1 and GG-I-526	II	1.0

* Four ounces of each lot of metal used in the construction of the nasal scissors shall be selected for chemical analysis.

4.3 Examination. The nasal scissors shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in Table I and III. Inspection, however, shall not be restricted to defects listed in Table III. Any nasal scissors in the sample containing one or more defects shall be rejected and if the number of defective items in any sample exceeds the acceptance number for that sample, the lot represented by the sample shall be rejected.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Points of scissors sharp.
102	Scissors not free from cracks, pits, dents, nicks, or burrs.
103	Finish not uniform, or of finish specified.
104	Scissors not free from excessive play or excessive stiffness during cutting action.
105	Scissors not of the proper design specified.
Minor	
201	Identification marking not present, correct, complete or legible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Scissors performance test. The test material shall be surgical stockinet meeting the requirements of the Military Medical Purchase Description for Federal Stock No. 6510-204-0000, Stockinet, Surgical, 6 inches by 25 yards. Scissors to be tested shall be cleaned prior to test performance. Three separate, consecutive tests shall be performed for each scissors. Each test shall consist of making one cut through 2 plies of test material at right angles to the ribs of the material. Each cut shall be made using the scissors in the normal manner (i.e., with the examiner's fingers in the finger rings of the instrument) except that no lateral pressure shall be exerted.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One scissors, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	6 units	144 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IC-1.

5.1.3.5 Intermediate package. Intermediate package shall be a carton of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors shall be acceptable or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard boxes shall be closed by method II of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The nasal scissors are intended to be used in surgical operations on the nose.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number, title and date of this specification.
(b) Applicable Federal Stock Number (FSN).
(c) Selection of applicable level of packaging and packing required (see 5.1 and 5.2).

6.3 Federal Stock Number (FSN) coverage. This specification covers the following item listed in the Federal Supply Catalog:

Federal Stock Number	Item Identification
6515-364-7100	SCISSORS, NASAL, Angular, Knight, 6-1/4 inch

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

6.4 Supersession data. This specification includes the requirements of Purchase Description No. 6, dated 21 June 1966 for FSN 6515-364-7100 Scissors, Nasal, Angular, Knight, 6-1/4 inch.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1610

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS. The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers, vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE: MIL-S-36797

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:21Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

Defense Supply Agency

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DOD-304

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE AT1
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:21Z
Check the source to verify that this is the current version before use.