MILITARY SPECIFICATION

SUPPORT, LEG CALF, ELASTIC, SEAMLESS

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers the requirements for pressure control elastic stockings used to reduce the risk of pulmonary embolism.

1.2 Classification. Support stockings covered by this specification shall be of one type in the following sizes, as specified (see 6.2):

Size 1 - LARGE (Calf Measuring up to 17 Inches in Circumference).
Size 2 - MEDIUM (Calf Measuring up to 15 Inches in Circumference).
Size 3 - SMALL (Calf Measuring up to 12 Inches in Circumference).

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-566	BOX, Folding, Paperboard.
PPP-B-585	BOX, Wood, Wirebound.
PPP-B-601	BOX, Wood, Cleated-Plywood.
PPP-B-621	BOX, Wood, Nailed and Lock-Corner.
PPP-B-636	BOX, Fiberboard.
PPP-B-676	BOX, Setup.

Military

MIL-L-10547	LINERS, Case and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-STD-191	Textile Test Methods.
FED-STD-601	Rubber: Sampling and Testing.
FED-STD-751	Stitches, Seams and Stitching.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications, standards, drawings, and publications required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer).

3. REQUIREMENTS

3.1 First article. When specified (see 6.2), before production is commenced, 12 finished pairs of socks shall be submitted or made ready for the contracting officer or his authorized representative for inspection as specified in 4.2. The approval of the preproduction sample authorizes the commencement of production but does not relieve the supplier of responsibility for compliance with all applicable provisions of this specification. The preproduction sample shall be manufactured by the supplier in the same facilities to be used for the manufacture of the production item.

3.2 Material.

3.2.1 Cotton yarn. The top and leg yarn shall be 28/1 ± 2 count, carded and combed, natural cotton yarn. Testing shall be as specified in 4.3.1.1.

3.2.2 Elastic yarn. The yarn shall be heat resistant 100 ± 5 gauge extruded or molded natural rubber core or a 112 ± 5 gauge cut natural rubber core. The elastic yarn shall have 3,400 ± 200 yards per pound and a minimum of 320 percent elongation when tested as specified in 4.3.1.1. The elastic yarn may be covered or uncovered, at the manufacturer's option.

3.2.3 Cotton yarn. The heel yarn shall be 60/3 ± 2 count, carded and combed, mercerized cotton yarn. Testing shall be as specified in 4.3.1.1

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:25Z
Check the source to verify that this is the currentversion before use.

3.2.4 Nylon yarn. The yarn shall be 260 ± 5% denier, 16 filament nylon. Testing shall be as specified in 4.3.1.1.

3.2.5 Seaming thread. The thread for seaming the edge of the turn-over top shall be nylon, natural white, commercial size 4, 1 or 2 ply; or cotton thread of equivalent size and ply. Testing shall be as specified in 4.3.1.1.

3.2.5.1 Color code size indicator. At the manufacturer's option, in addition to the size marking specified in 3.3, colored seaming thread may be used as a size indicator. When this option is used, the size color code shall be: small-blue, medium-white, large-red.

3.3 Label. Each stocking shall have a size marking applied and centered on the knitted top. The size marking shall conform to type III, class 9 of DDD-L-20. The color of the marking medium shall be green. The size marking shall be clearly legible and show good fastness to laundering transference (wool method). The minimum height of the characters for each size sock shall be 1/4 inch.

3.4 Color. The color of the finished stockings shall be natural.

3.5 Design. The support stockings shall be seamless, circular knit, proportioned pressure control, with a cuffed top, reinforced heel, and a toe with a true ribbed cuff.

3.6 Construction.

3.6.1 Knitting. The stockings shall be knit seamless in one integral unit, on a 176 needle circular machine having a cylinder diameter of 3 1/2 inches.

3.6.1.1 Open toe cuff. The open toe cuff shall be a true 1 x 1 rib knit, using 2 ends of 28/1 yarn specified in 3.2.1. The cuff edge shall have a turn-over, well defined, non-raveling welt, free from loose ends.

3.6.1.2 Foot. The foot shall be knit with a plain stitch using 1 end of 28/1 yarn and 1 end of elastic yarn as specified in 3.2.1 and 3.2.2 in the same feed.

3.6.1.3 Heel. The heel shall be knit with a plain stitch using 1 end of 60/3 yarn and 1 end of 260 denier nylon as specified in 3.2.3 and 3.2.4. A minimum of 26 gore needles shall be used in knitting the heel.

3.6.1.4 Body or leg. The body or leg shall be knit with a plain stitch using 1 end of 60/3 yarn and 1 end of elastic yarn as specified in 3.2.1 and 3.2.2 in the same feed.

3.6.1.5 Top. The top shall be knit with a plain stitch using 2 ends of 28/1 yarn as specified in 3.2.1.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:25Z
Check the source to verify that this is the currentversion before use.

3.6.2 Turn-over top. The top shall have a 3/4 inch minimum turn-over. The turn-over edge shall be seamed using the thread specified in 3.2.5. The stitch type shall be 521, with a minimum of 12 stitches per inch.

3.6.3 Length of loose ends. All ends of yarn on the inside of the finished stocking shall be trimmed to not less than 1/4 inch nor more than 1 inch.

3.6.4 Finishing. The stockings shall not be finished. Scouring or boarding is not required.

3.6.5 Pairing. The stockings shall be matched and paired, so that there will be no greater difference in foot length than 1/4 inch, and in leg length, 1/2 inch. The use of thread, twine or staple to secure a pair of stockings will not be permitted.

3.6.6 Instruction label. An instruction label shall be legibly printed on a separate sheet of white paper and inserted with each pair of stockings into the immediate polyethylene envelope or container. The instruction label shall state substantially as follows:

SUPPORT, LEG, CALF

ELASTIC STOCKINGS

For Controlled Compression

FITTING CHART

SMALL	MEDIUM	LARGE
Calf measuring up to 12" in circumference	Calf measuring up to 15" in circumference	Calf measuring up to 17" in circumference

Medium size will be used by most patients

HOW TO PUT ON

1. Turn stocking inside out down to the foot and fit the foot first.
2. Fit the heel section, then bring top of calf section at least to bottom of knee and smooth out all wrinkles.
3. Pull the toe section forward to eliminate wrinkles across the instep and heel.

CAUTION: DO NOT TURN DOWN ELASTIC MATERIAL AT THE TOP.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:25Z
Check the source to verify that this is the current version before use.

3.6.6 Instruction label (cont'd.)

WASHING INSTRUCTIONS:

1. May be hand washed or washed in regular washing machine. Do not use excessive bleach.

2. Machine dryable. (CAUTION) Do not allow stocking to remain in machine after they are dry. Prolonged subjection to high temperatures can reduce the wear life of the HEAT RESISTANT RUBBER.

CAUTION: Keep salves or ointments from contact with stockings, as they may have ingredients harmful to rubber.

As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer, via the cognizant Government inspector, two preliminary copies of his proposed Instructions, for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary text shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final text without delaying delivery under the contract or purchase order. Should the supplier have furnished acceptable Instructions for use for the identical item within two years preceding the date of contract and proposes to furnish Instructions identical with those previously accepted, then the requirement for review of the draft may be waived upon request to the Contracting Officer.

3.7 Physical requirements.

3.7.1 Measurements, courses and weights. The measurements, courses and weights of the stockings shall conform to table I. All measurements in table I shall be made with the stocking laid out flat under no tension. Testing shall be as specified in 4.3.3.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

Table I. Measurements, courses and weights

	See Figure 1	Size			Tolerance
		Small	Medium	Large	
Top:					
Number of courses 3/	C	84	84	84	± 4
Length (inches)		1 1/2	1 1/2	1 1/2	± 1/8
Turn-over (inches)		3/4	3/4	3/4	Min.
Body or leg:					
Number of courses 1/	A	576	624	684	± 4
Length (inches)		10 1/2	11 1/2	13	Min.
Foot:					
Number of courses 2/	B	130	130	130	± 4
Length (inches)		2 1/2	2 1/2	2 1/2	Min.
Toe cuff:					
Number of courses 4/	D	40	40	40	± 4
Length (inches)		3/4	3/4	3/4	Min.
Conditional weight per dozen pairs (pounds & ounces)		1-11	1-12	2-0	Min.

1/ Leg courses shall be counted from the first short butt heel gore needle to bottom edge of top.

2/ Foot courses shall be counted from the first short butt heel gore needle to bottom edge of toe cuff.

3/ Top courses shall be counted from joining line of leg fabric to edge of turn-over.

4/ Toe cuff courses shall be counted from bottom edge of welt to joining line of foot fabric.

3.7.2 Stretch. The stocking shall stretch (crosswise) to a minimum of 6 inches when measured across a point midway between top of heel and bottom of top, when tested as specified in 4.3.3.

3.8 Workmanship. The stockings shall conform to the quality and grade of product established by this specification. The occurrence of defects shall not exceed the applicable acceptable quality levels.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Certificate of compliance. Where certificates of compliance are submitted, the Government reserves the right to check test such items to determine the validity of the certification.

4.2 First article inspection. When required, the first article sample submitted in accordance with 3.1, shall be inspected as specified in 4.3.2.1 and 4.3.2.2 for compliance with design, construction, workmanship and dimensional requirements.

4.3 Inspection. Sampling for inspection shall be performed in accordance with MIL-STD-105, except where otherwise indicated.

4.3.1 Component and material inspection. In accordance with 4.1 above, components and materials shall be inspected and tested in accordance with all the requirements of referenced specifications, drawings and standards unless otherwise excluded, amended, modified or qualified in this specification or applicable purchase documents.

4.3.1.1 Testing of components. In addition to the quality assurance provisions of the referenced specifications, testing shall be performed on the components listed in table III. The methods of testing specified in FED-STD-191 wherever applicable and as specified herein, shall be followed. The lot size shall be expressed in units of one spool, cone or tube and the sample unit shall be one spool, cone or tube. All test reports shall contain the individual values utilized in expressing the final result. The sample size shall be in accordance with table II and the lot shall be unacceptable if one or more units fail to meet any requirement specified.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:25Z
Check the source to verify that this is the currentversion before use.

Table II. Sample size

Lot size	Sample size
800 or less	2
801 up to and including 22,000	3
22,001 and over	5

Table III. Component tests

Component	Characteristic	Requirement reference	Test method	No. of determinations per sample unit	Results reported as
Cotton yarn	Material identification	3.2.1 & 3.2.3	1/	-	-
	Count	3.2.1 & 3.2.3	4020	-	-
	Combed	3.2.1 & 3.2.3	1/	-	-
	Mercerization	3.2.3	1/	-	-
Nylon yarn	Material identification	3.2.4	1/	-	-
	Denier and filament	3.2.4	1/	-	-
Core of elastic yarn	Gauge	3.2.2	211 (FED-STD-601) 2/	6	Average of 6 determinations to nearest whole number
	Identification	3.2.2	15011 (FED-STD-STD-601)	1	Pass or fail

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

Table III. Component tests (cont'd.)

Component	Characteristic	Requirement reference	Test method	No. of determinations per sample unit	Results reported as
Elastic yarn	Yards per pound	3.2.2	4010	-	-
	Elongation	3.2.2	4.4.1	5	Average of 5 determinations to nearest percent
Nylon or cotton sewing thread	Material identification	3.2.5	1/	-	-
	Ply	3.2.5	Visual	1	Pass or fail

1/ Unless otherwise specified, a certificate of compliance shall be submitted and will be acceptable for the stated requirements.

2/ Gauge shall be determined as follows:

$$\text{Gauge} = \frac{1}{\text{Average width of rubber core (inches)}}$$

4.3.2 Examination of the end item. Defects found during this examination shall be classified in ac ordance with the lists shown in 4.3.2.1 and 4.3.2.2. The sample unit for these examinations shall be one individual stocking. The lot size shall be expressed in units of one individual stocking. The inspection levels and acceptable quality levels for these examinations shall be in accordance with 4.3.2.3.

4.3.2.1 Visual examination. The finished stockings shall be visually examined for defects listed in table IV.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:25Z
Check the source to verify that this is the currentversion before use.

Table IV. Classification of defects

Defect	Classification Major	Minor
Any holes, runs or dropped stitches.	X	
Thin areas, mends.	X	
Welt omitted, cut, frayed, raveled.	X	
Welt uneven or not clearly defined.		X
Poor fashioning of heel gore resulting in tight tension, lumps and dog-ears that will not level out.	X	
Loose or floated ends:		
Not trimmed as specified.		X
Ends floating more than 1 inch inside of sock.		X
Any floated ends on outside of sock.	X	
Pattern of knit:		
Not as specified throughout entire sock.	X	
Sock not knitted as an integral unit.	X	
Elastic yarn omitted.	X	
End out for more than one course - body.	X	
Nonuniform in overall appearance, not well shaped.		X
Slubby yarn more than three times normal diameter.		X
Streaks, stains, or spots, clearly noticeable. 1/		X
Rancid or bad odor.	X	
Vegetable matter - clearly noticeable. 1/		X
Loosely knit - slack or sleazy.	X	
Label missing, incorrect, illegible.	X	

1/ At normal inspection distance (approximately 3 feet).

4.3.2.2 Examination for dimensions. Examination for dimensions shall be in accordance with the classification of defects listed below. The sample size shall be drawn in pairs.

Defects

Leg length Foot length Top length Toe cuff length	More or less than specified tolerance.
Pairing	Mismated by more than 1/4 inch in foot length or 1/2 inch in leg length (tallied only for one sock in any pair).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

4.3.2.3 Inspection levels and acceptable quality levels (AQL's). The inspection levels and AQL's expressed in defects per 100 units shall be as follows:

Examination	Inspection level	AQL	
		Major	Total (Major and Minor)
4.3.2.1 Visual	I	1.5	4.0
4.3.2.2 Measurements	S-3	- (1 class)	4.0

4.3.3 Testing of the end item. The test methods listed in table V shall be in accordance with FED-STD-191 except as otherwise noted, and as described herein. The physical and chemical values specified in section 3 apply to the average of the number of test specimens selected for a sample unit for test purposes as specified in the applicable test methods. When the data in the "Number of determinations per sample unit" and "Results reported as" columns are not specified in table V they shall be as required by the referenced test method. The lot size shall be expressed in units of one stocking each. Except as indicated below for weight and stretch determinations, the sample size shall be in accordance with table II and the lot shall be unacceptable if one or more units fail to meet any requirement specified. The sample unit for test purposes shall be as follows:

Weight determination:	Twelve pairs of stockings from each size represented. The sample size shall be one unit regardless of lot size.
Stretch determination:	Five individual stockings from each size in the lot. The sample size shall be one unit regardless of lot size.
All other test determinations:	Five individual stockings representing each size in the lot proportionately.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

Table V. End item tests

Characteristic	Requirement reference	Test method	Number of determinations per sample unit	Results reported as:
Type of knit	3.6.1.1 3.6.1.2 3.6.1.3 3.6.1.4 3.6.1.5	1/	-	-
Weight per dozen pairs (conditioned)	3.7.1	Scale	1	To nearest 0.25 ounce
Number of courses:				
Leg	3.7.1	Count	1	Nearest whole number
Foot	3.7.1	Count	1	Nearest whole number
Top	3.7.1	Count	1	Nearest whole number
Toe cuff	3.7.1	Count	1	Nearest whole number
Stretch (crosswise):				
Leg	3.7.2	2/	5	Average of 5 determinations to nearest 0.1 inch

1/ Unless otherwise specified, a certificate of compliance shall be submitted and will be acceptable for the stated requirements.

2/ The crosswise stretch measurement shall be evaluated on a Houchin modification of a Schieffer machine described in Method 7560 of FED-STD-191 and as shown on figure 2. The modified apparatus differs from the apparatus shown in FED-STD-191 with regard to the shape and size of the separating form. In lieu of the foot-like form, a rectangular form of dimensions 2 inches by 4 inches shall be used. The stocking shall be pulled over the form so that the 2-inch edges shall be parallel to the foot of the stocking. The indicator pin shall be inserted in the upper 2-inch edge of the separating form and a 10-pound weight slowly applied so as to cause separation of the upper and lower slotted form with resultant stretch of the stocking under a uniform load over the 2-inch edges. The stockings shall be evaluated after the weight has hung freely for 30 seconds, and shall be expressed in inches as the distance between the upper and lower edges of the separated forms.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:25Z
Check the source to verify that this is the current version before use.

4.3.4 Examination of preparation for delivery requirements. An examination shall be made to determine that packaging, packing and marking requirements of section 5 of this specification are complied with. Defects shall be scored in accordance with table VI. The sample unit shall be one shipping container fully prepared for delivery with the exception that it need not be sealed. Defects of closure listed shall be examined on shipping containers fully prepared for delivery. The lot size shall be the number of shipping containers in the end item inspection lot. The inspection level shall be S-2 and the AQL shall be 2.5 defects per hundred units.

Table VI. Classification of Preparation for Delivery Defects

Examine	Defect
Marking (exterior and interior)	Omitted; incorrect; illegible; of improper size, location, sequence, or method of application. Size shown on stockings not the same as on the containers. 1/
Materials	Any component missing. Any component damaged, affecting serviceability.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, loose strapping, inadequate stapling. Bulged or distorted container.
Content	Number of bundles per container is more or less than specified. Number per bundle is more or less than required. 1/

1/ For this defect, one bundle shall be examined from each shipping container in the sample.

4.4 Test.

4.4.1 Elastic yarn elongation. A specimen of yarn at least 6 inches in length shall be measured while under no tension and then stretched to its extreme, without breaking, and again measured with a suitably graduated scale. A scale reading directly in percent elongation may be used. Five specimens, randomly selected, shall be tested from each sample unit. The elongation shall be the average of specimens tested and shall be calculated as follows:

$$\text{Elongation, percent} = \frac{S - R}{R} \times 100$$

Where: S = extreme stretch measurement
R = relaxed (original) measurement

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One pair of leg supports of the size specified, constitutes one unit of issue.

5.1.2 Packaging quanitites. The number of units of issue indicated in Table VII shall be packaged in each unit, intermediate, and exterior container as applicable, for the required level of protection specified in the procurement document.

Table VII. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	240 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit of issue. One pair of stockings shall be neatly folded and packaged in a suitable polyethylene bag of appropriate size. Closure of the bag shall be adequate to prevent spilling of contents under normal handling and to prevent the entry of dust. In addition, each bag shall have a laundry instruction sheet enclosed.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and constructed in accordance with PPP-B-566 or PPP-B-676 except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Each fiberboard box shall conform to the special requirements specified in Table II of PPP-B-636.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure of wood boxes shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II of PPP-B-636. In addition, each fiberboard box shall conform to the special requirements specified in Table I of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Unit package. Each unit package shall be marked in accordance with IL-STD-129. Marking may be printed on the bag or on a label inserted within he bag in such a manner as to permit ready identification. In addition, marking hall include the size. A color coded size indicator is acceptable.

5.3.2 Intermediate packages. Each intermediate package shall be marked in ccordance with MIL-STD-129. When labels are utilized, waterproofing shall be equired only when applicable carton is fabricated of water-resistant material. ontract or purchase order number, size, and name of contractor shall be shown.

5.3.3 Exterior container. Exterior container shall be marked in accordance ith MIL-STD-129. The size shall also be shown.

6. NOTES

6.1 Intended use. The support, leg calf is intended for use by Department f Defense personnel to reduce the risk of pulmonary embolism.

6.2 Ordering data. Procurement documents should specify the following:

a. Title, number and date of this specification.
b. Federal stock number (FSN).
c. Specify size support required (see 1.2).
d. Whether first article sample is required.
e. Selection of applicable levels of packaging and packing (See 5.1 and 5.2).

6.3 This specification does not include all types, classes, grades, or sizes f the commodity indicated by the title of this specification or those which are ommercially available, but is intended to cover the types and sizes which are ormally procured to meet military requirements.

ustodians:
Army - MD
Navy - MS
Air Force - 03

eview activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No.: 6515-1638

Review information is current as of the date of this document. For future coordination changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:25Z
Check the source to verify that this is the current version before use.

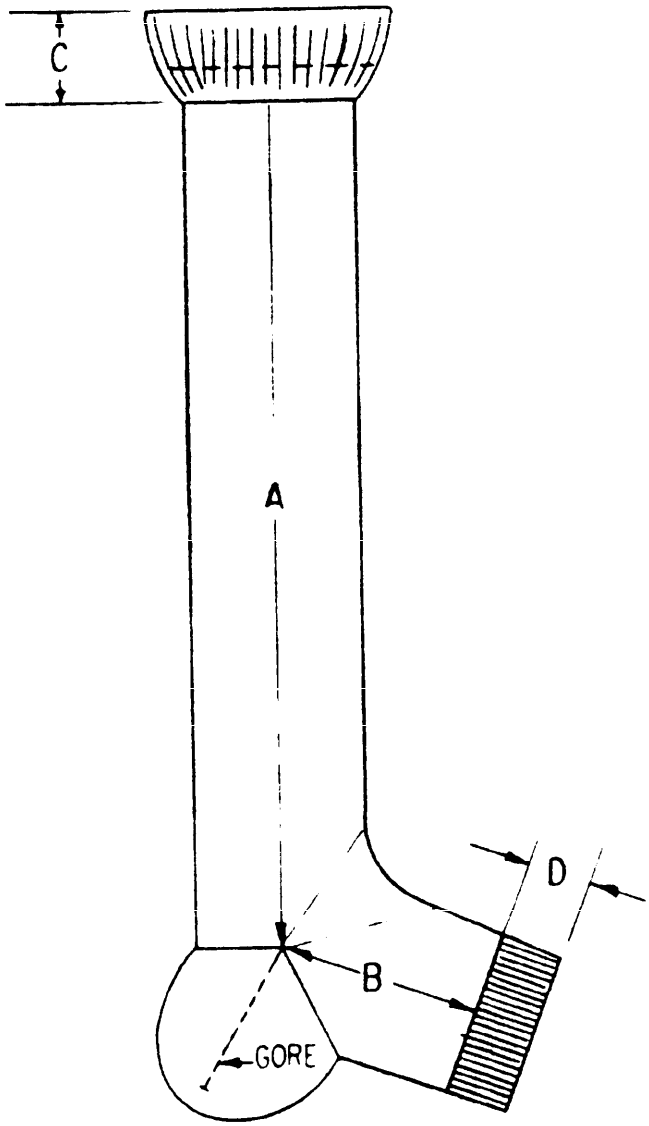


FIGURE 1

SUPPORT LEG CALF

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

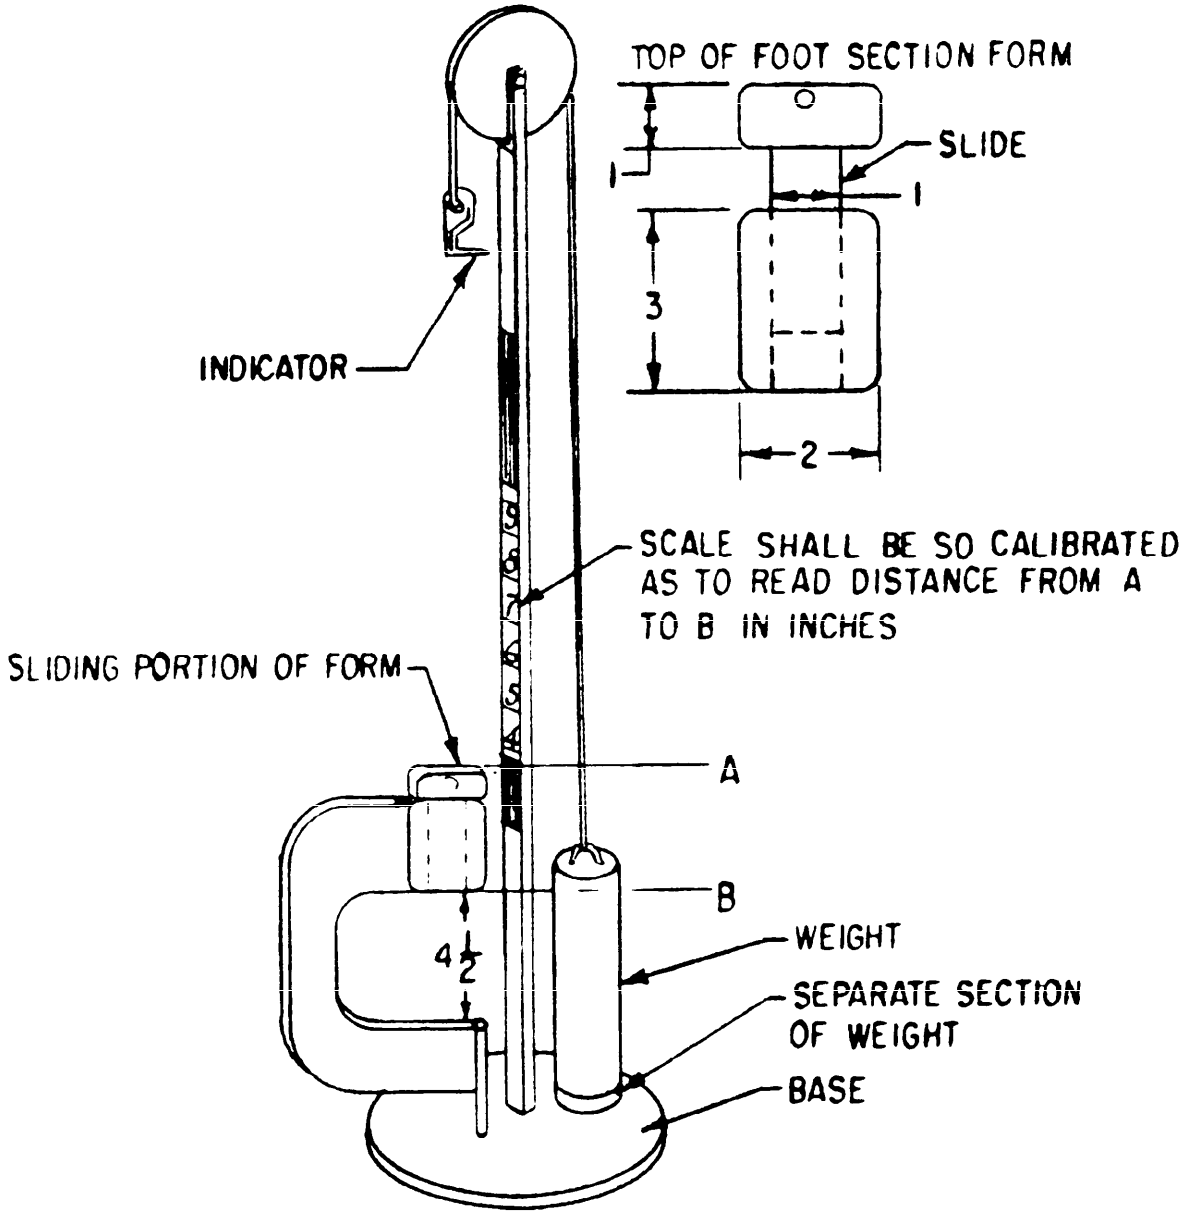


FIGURE 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budge: Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)* | DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 64 WHICH MAY BE USED.

S/N-0102-014-1801 C-25254

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:25Z
Check the source to verify that this is the current version before use.

FOLD

POSTAGE AND FEES PAID

OFFICIAL BUSINESS

Commander
Defense Personnel Support Center
ATTN: DPSC-ATTS
Material Standards Branch
Technical Operations Division
Directorate of Medical Materiel
2800 South 20th Street
Philadelphia, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:25Z
Check the source to verify that this is the current version before use.