A-A-0051848(DM)
12 March 1987

INTERIM COMMERCIAL ITEM DESCRIPTION

FORCEPS, COAGULATION (Malis, Titanium)

The General Services Administration has authorized the use of this interim commercial item description which was developed by the Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-RST, 2800 South 20th Street, Philadelphia, PA, 19101, based upon currently available technical information.

This interim commercial item description covers one size and type of bipolar electrosurgical forceps of the Malis design.

Salient characteristics.

Material. Forceps shall be manufactured from Ti-6Al-4V titanium of composition in accordance with American Society for Testing and Materials (ASTM) Standard B348 for Grade 5 titanium alloy.

Style and design. Forceps shall be in accordance with Figure 1. The tips shall taper to a fine smooth-pointed tip. Tips shall meet exactly when closed in the normal manner. The base of the forceps (around the connector pins) shall be insulated with a plastic material. The tips shall be formed such that current flow is restricted to only the distal tips.

Steam sterilization. Plastic and epoxy materials used in the manufacture of the forceps shall be capable of repeated steam sterilization.

Finish. The finish shall be uniform and free from burrs, chips, pits, rough areas and grind or tool marks.

Tests. Forceps shall be tested for continuity (connector pin-to-tip) and resistance (pin-to-pin and pin-to-outside-of-insulation cup).

Workmanship. The forceps shall be processed in such a manner as to be uniform and free from defects which affect life, utility, or appearance.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:02Z
Check the source to verify that this is the current version before use.

Product Quality Level

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One forceps, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The forceps shall be examined to determine compliance with all requirements contained in this specification.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one forceps. Sampling shall be level S-1 with an AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE 1: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-7944	FORCEPS, COAGULATION, Malis, Bipolar, Titanium, 6 inch (15.2 cm) Long, Extra Fine Tip.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:02Z
Check the source to verify that this is the current version before use.

NOTE 2: Intended use. Forceps are intended for use in electrosurgery. Forceps may be used in a bloody surgical field or under irrigation fluids. Forceps are intended for use with a bipolar electrosurgical generator without a patient grounding plate.

NOTE 3: Cord compatibility. Forceps are tended for use with Cord, Electrical, Bipolar (NSN 6515-01-139-7942).

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4030

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

FIGURE 1.

FORCEPS, COAGULATION, MALIS, 6 INCH

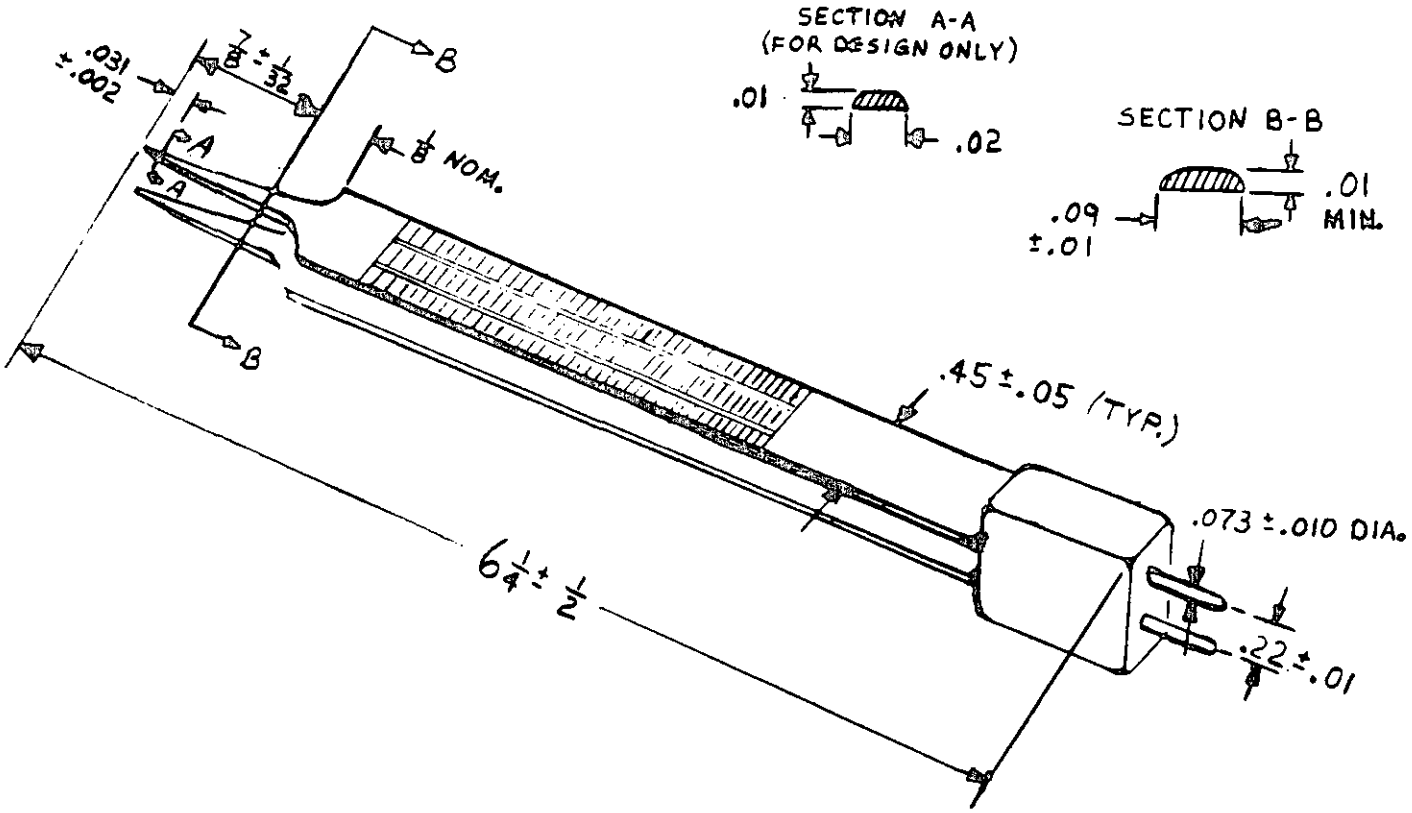

NOTES:

1. TIP SEPERATION .59 TO .69 IN FULLY OPEN POSITION.
2. ALL DIMENSIONS ARE INCHES.
3. DO NOT SCALE.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:02Z
Check the source to verify that this is the current version before use.